
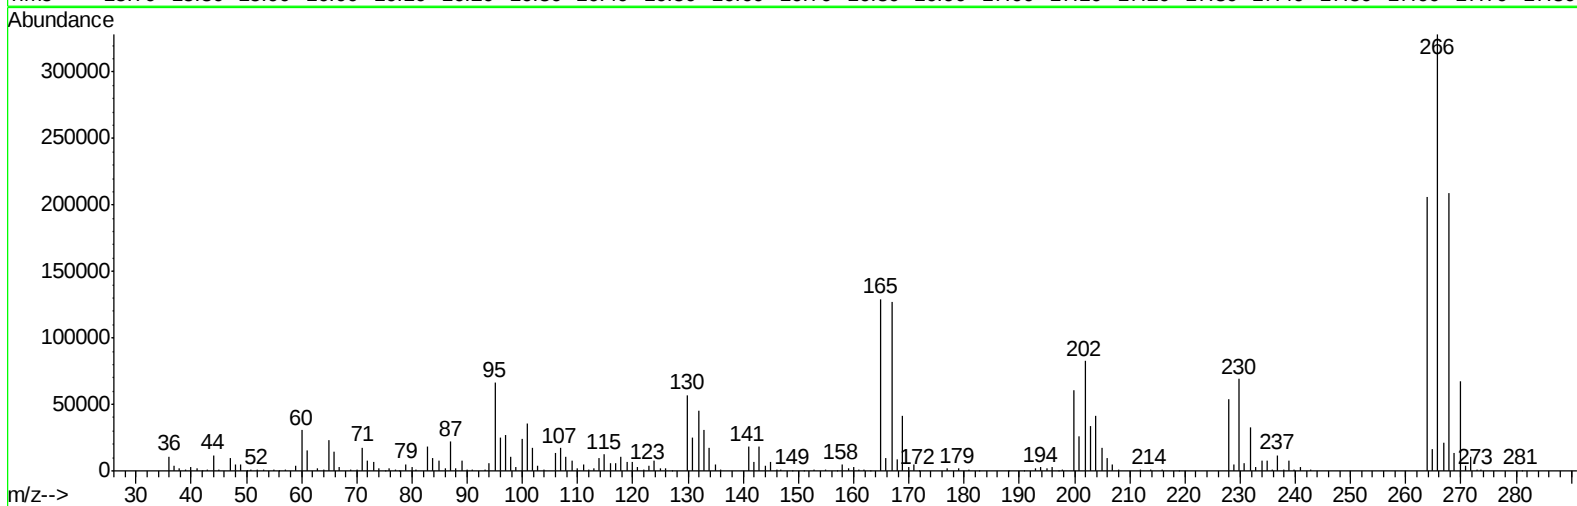


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN092719\
Data File : BN007881.D
Acq On : 27 Sep 2019 10:46
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 03:07:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

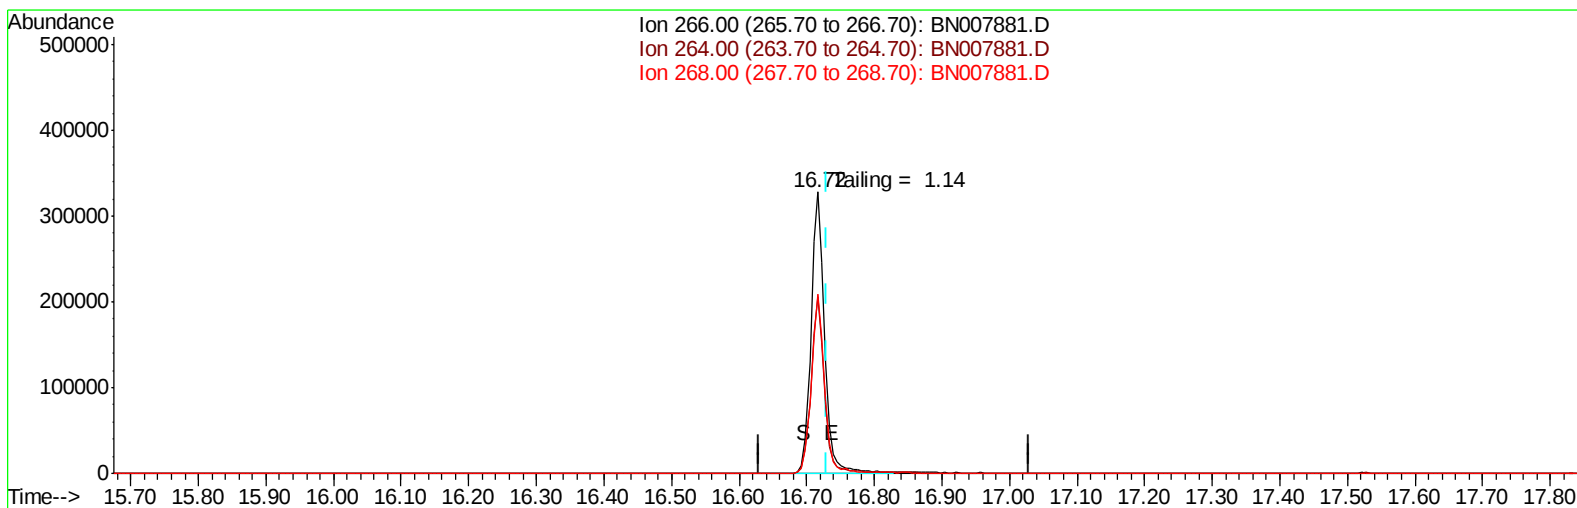

TIC: BN007881.D

(22) Pentachlorophenol

16.716min (-0.014) 0.00ng

response 458628

Ion	Exp%	Act%
266.00	100	100
264.00	62.50	62.83
268.00	67.80	63.57
0.00	0.00	0.00