


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092719\
 Data File : BN007881.D
 Acq On : 27 Sep 2019 10:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

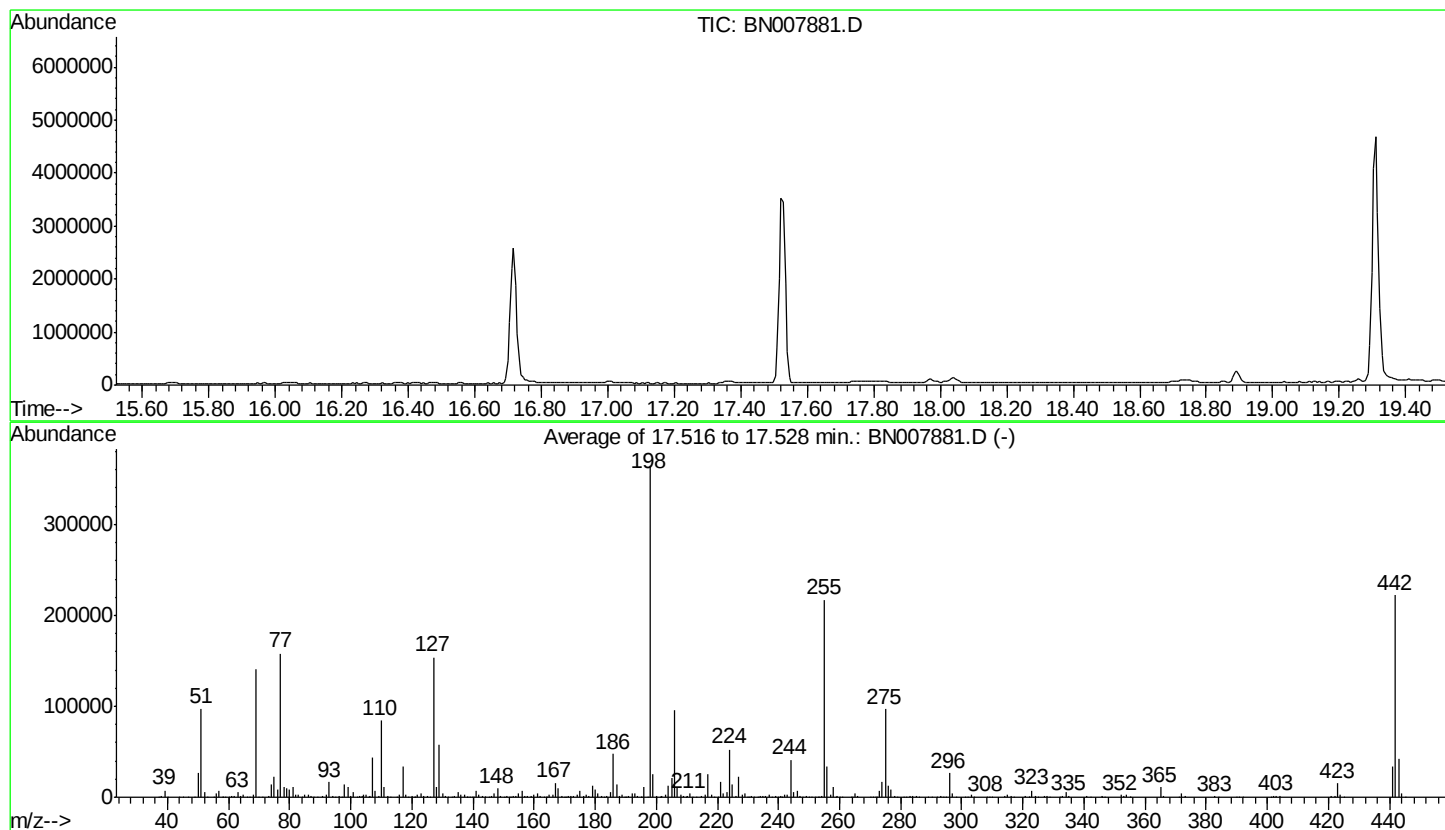

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	97852	PASS
68	69	0.00	2	1.6	2303	PASS
69	198	0.00	100	38.8	141340	PASS
70	69	0.00	2	0.5	653	PASS
127	198	10	80	42.1	153576	PASS
197	198	0.00	2	0.2	647	PASS
198	198	100	100	100.0	364608	PASS
199	198	5	9	6.8	24701	PASS
275	198	10	60	26.5	96706	PASS
365	198	1	100	3.1	11184	PASS
441	198	0.01	100	9.5	34501	PASS
442	198	50	100	61.0	222229	PASS
443	442	15	24	18.9	42002	PASS