

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027932.D
 Acq On : 28 Sep 2023 18:53
 Operator : MA/JU
 Sample : PB155827BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK827

Quant Time: Sep 29 04:00:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	4624	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	18163	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	12050	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	26219	0.400	ng/ul	0.00
17) Chrysene-d12	21.542	240	24012	0.400	ng/ul	0.00
23) Perylene-d12	24.015	264	23549	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	32816	5.634	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	9724	0.353	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	25215	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.596	166	3106	0.058	ng/ul#	14
20) Pyrene	19.752	202	3125	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.860	252	6263	0.074	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027932.D
Acq On : 28 Sep 2023 18:53
Operator : MA/JU
Sample : PB155827BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK827

Quant Time: Sep 29 04:00:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




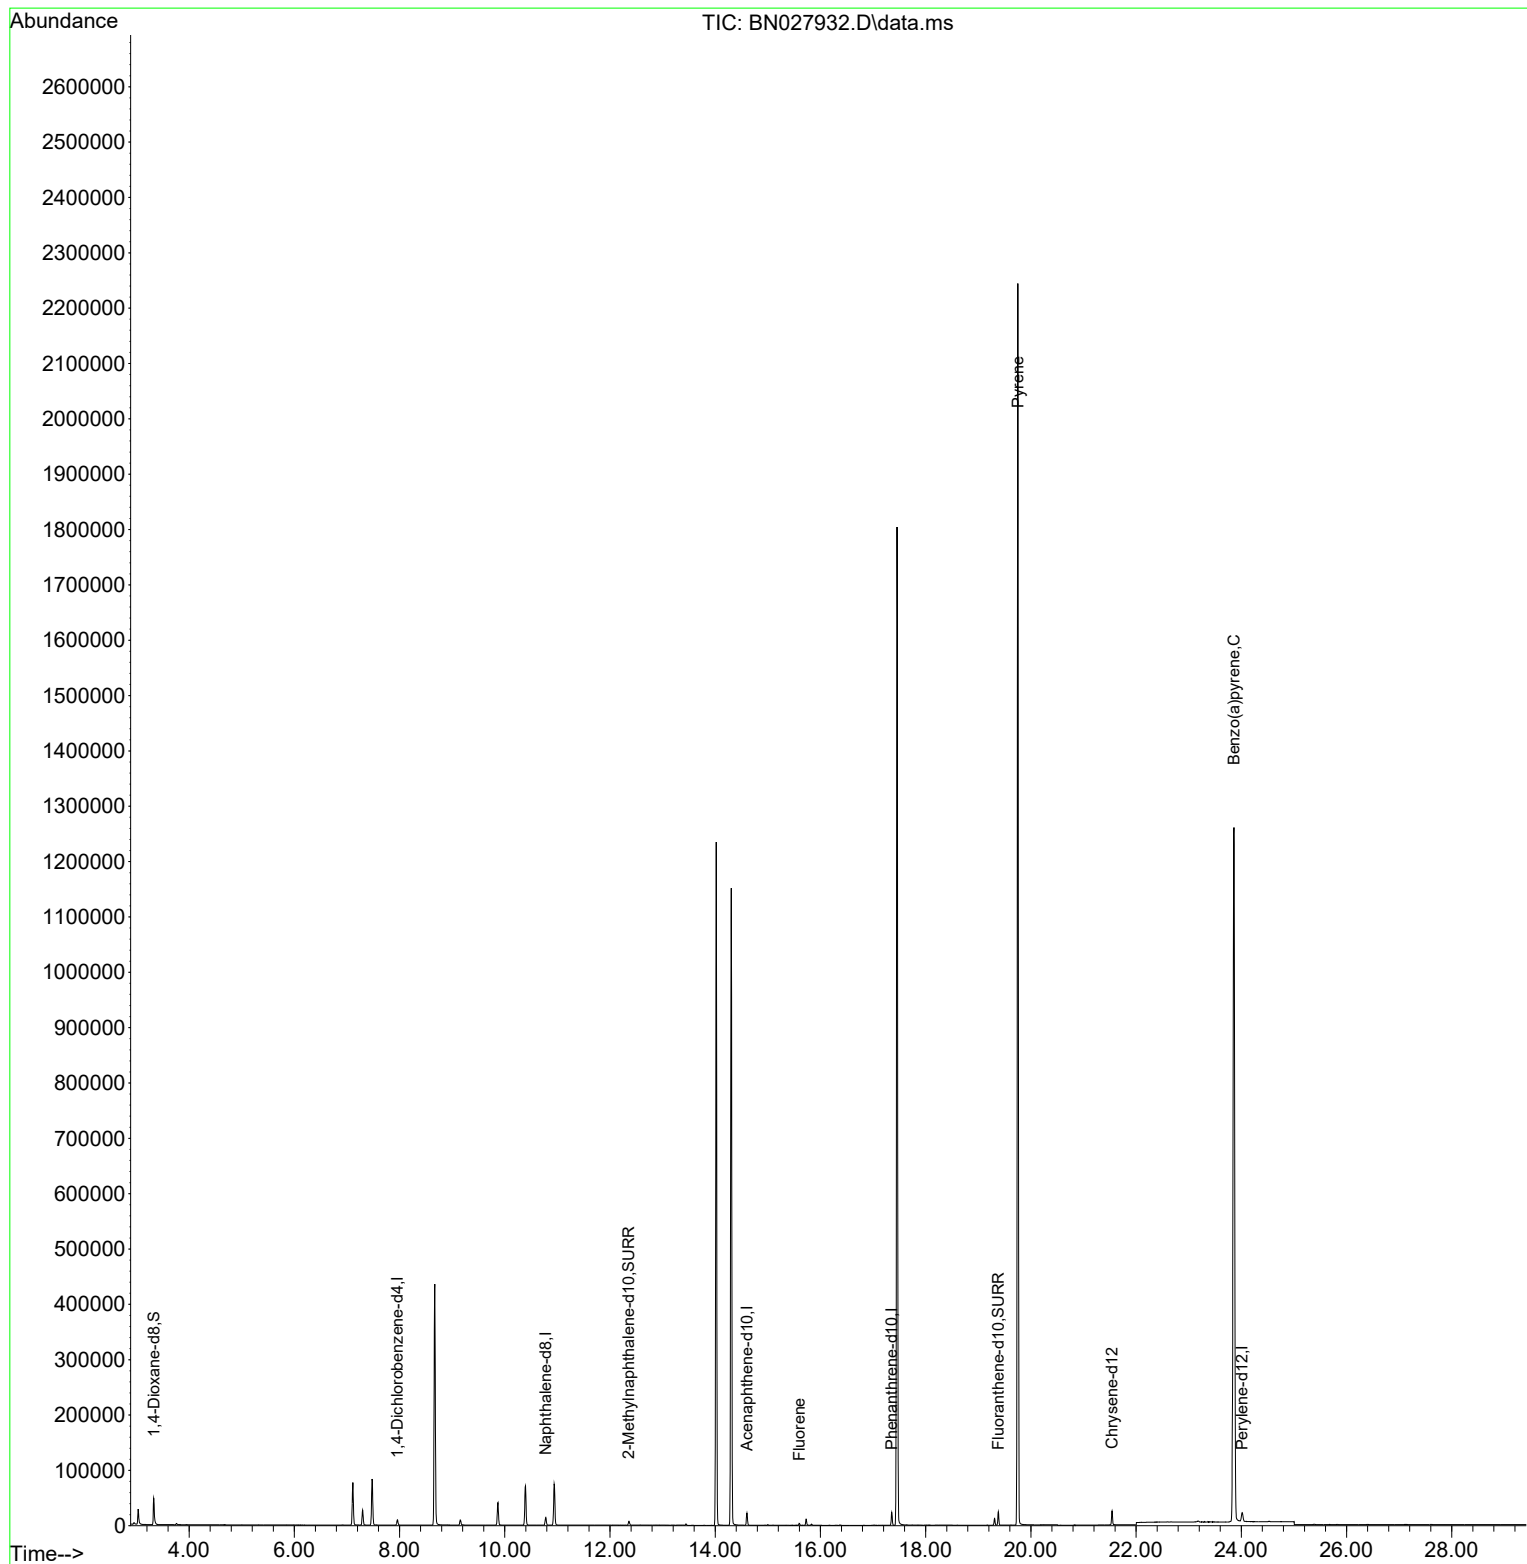


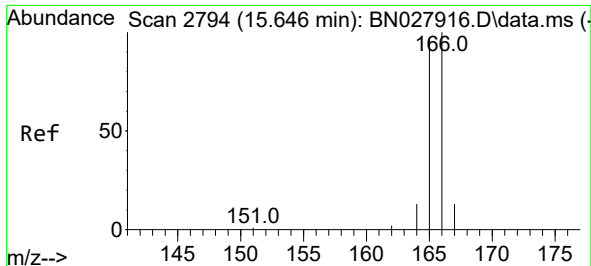

#12
Fluorene
Concen: 0.058 ng/ul
RT: 15.596 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN027932.D
Acq: 28 Sep 2023 18:53




Instrument :
BNA_N
ClientSampleId :
SBLK827


Tgt Ion:166 Resp: 3106
Ion Ratio Lower Upper
166 100
165 7.8 78.0 117.0#
167 34.5 11.4 17.2#

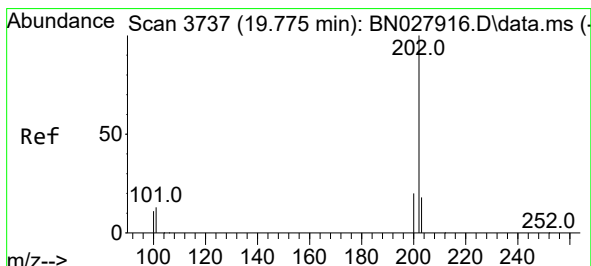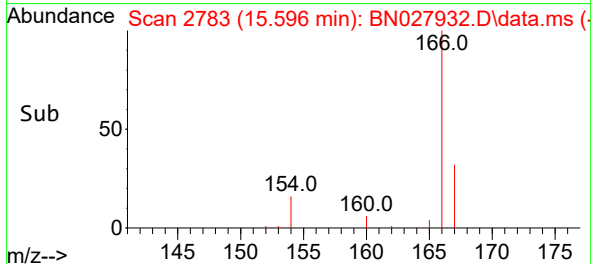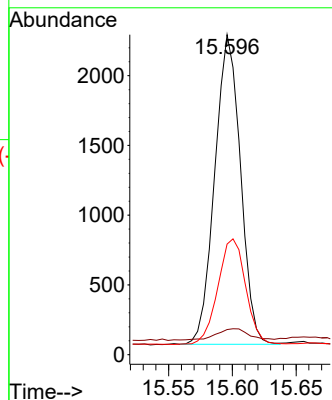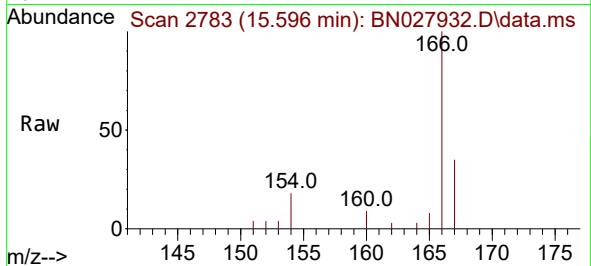

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.752 min Scan# 3732
Delta R.T. -0.023 min
Lab File: BN027932.D
Acq: 28 Sep 2023 18:53


Tgt Ion:202 Resp: 3125
Ion Ratio Lower Upper
202 100
101 149.8 11.4 17.0#
100 1039.0 9.1 13.7#

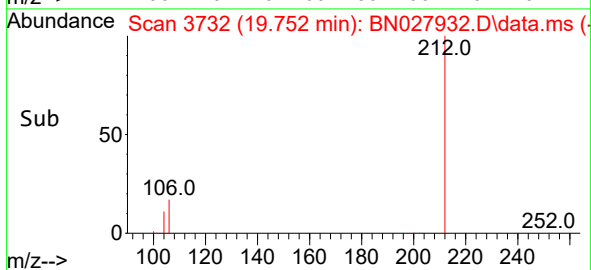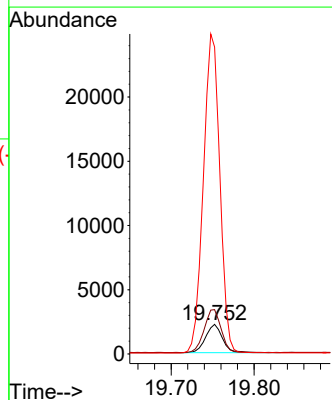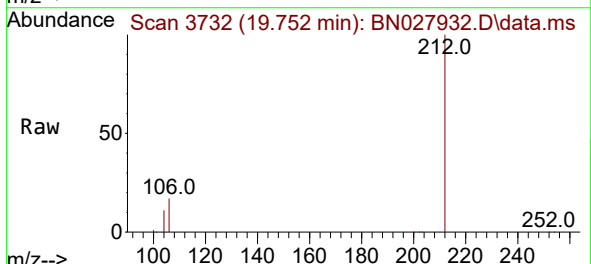

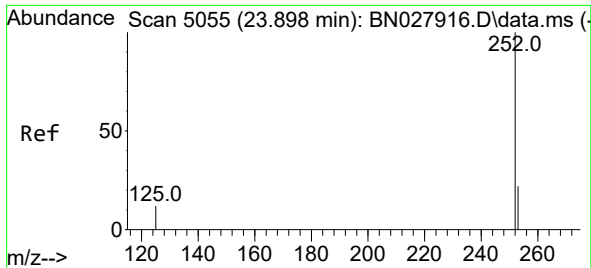

#26
 Benzo(a)pyrene
 Concen: 0.074 ng/ul
 RT: 23.860 min Scan# 5042
 Delta R.T. -0.035 min
 Lab File: BN027932.D
 Acq: 28 Sep 2023 18:53

Instrument :
 BNA_N
 ClientSampleId :
 SBLK827

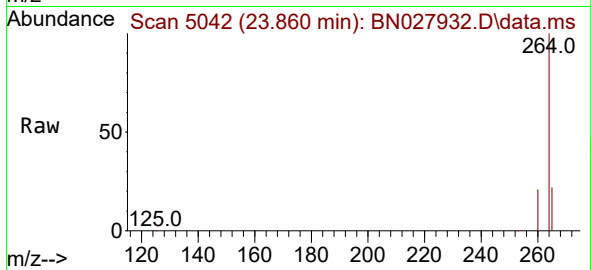

Tgt Ion:252 Resp: 6263
 Ion Ratio Lower Upper
 252 100
 253 54.2 21.9 32.9#
 125 53.7 15.5 23.3#

