

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027944.D
 Acq On : 29 Sep 2023 02:43
 Operator : MA/JU
 Sample : PB155752BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK752

Quant Time: Sep 29 04:01:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	3798	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	14749	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.601	164	10213	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	22411	0.400	ng/ul	0.00
17) Chrysene-d12	21.536	240	20189	0.400	ng/ul	0.00
23) Perylene-d12	24.009	264	19597	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	35272	7.373	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	10104	0.452	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	26908	0.436	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.596	166	3378	0.074	ng/ul#	14
20) Pyrene	19.747	202	3422	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.848	252	6719	0.096	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027944.D
Acq On : 29 Sep 2023 02:43
Operator : MA/JU
Sample : PB155752BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK752

Quant Time: Sep 29 04:01:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




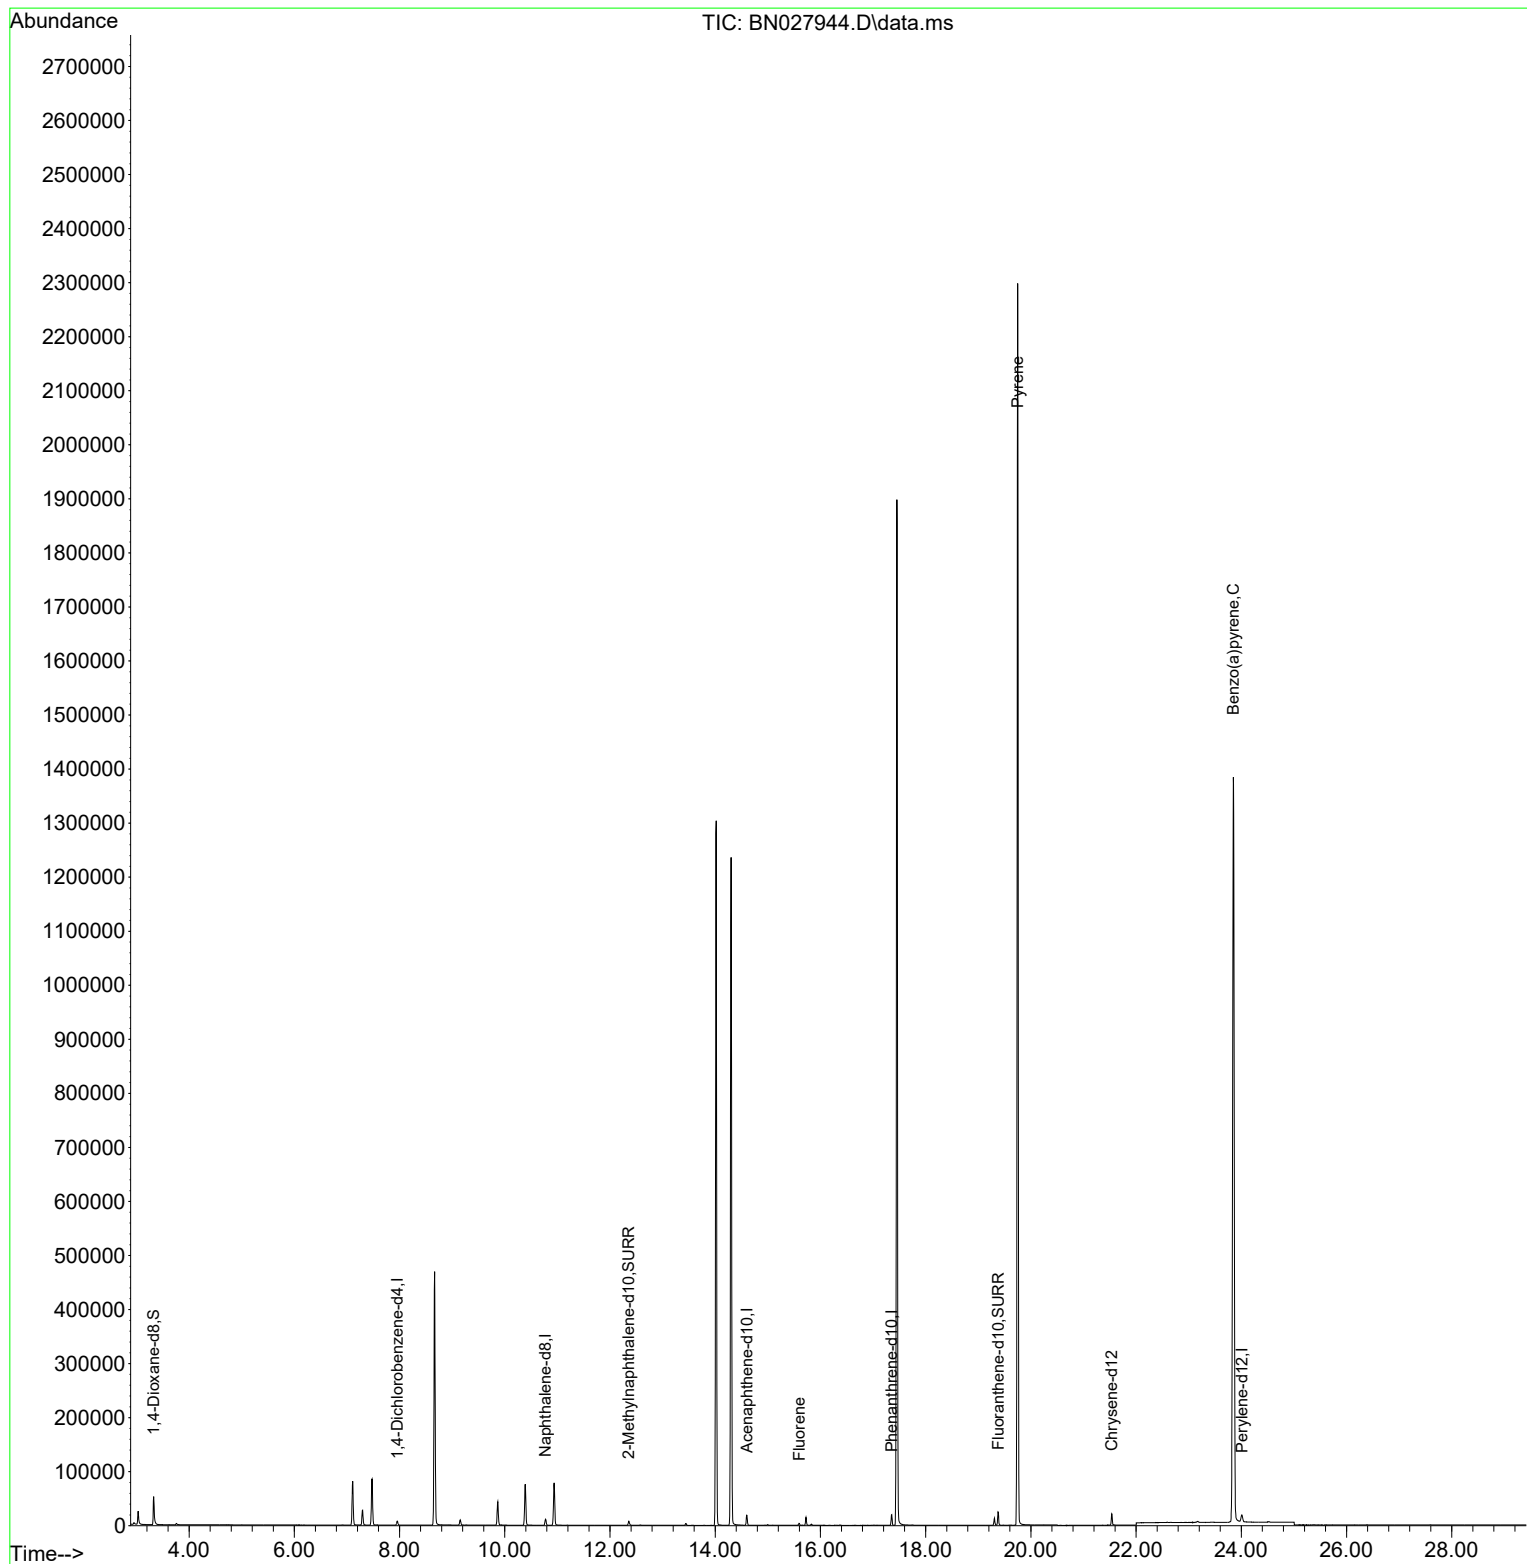


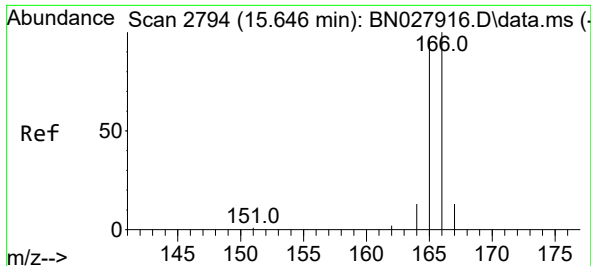

#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.596 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN027944.D
Acq: 29 Sep 2023 02:43




Instrument :
BNA_N
ClientSampleId :
SBLK752


Tgt Ion:166 Resp: 3378
Ion Ratio Lower Upper
166 100
165 8.3 78.0 117.0#
167 36.8 11.4 17.2#

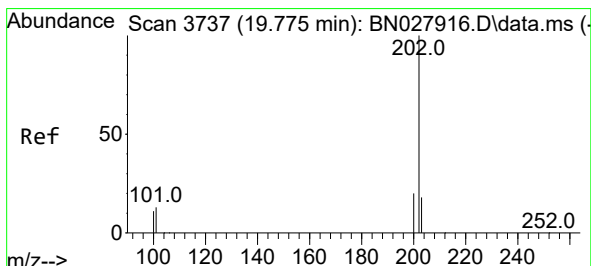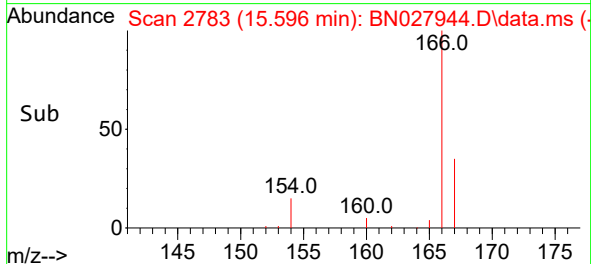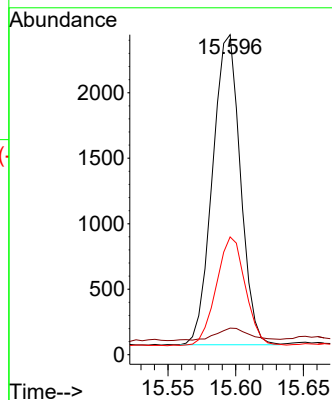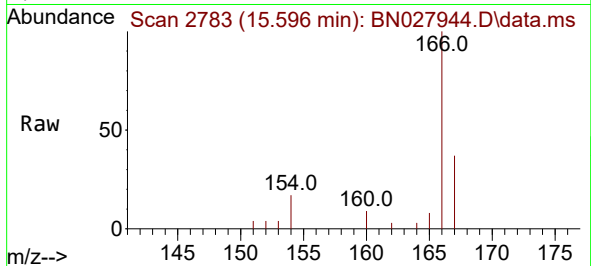

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.747 min Scan# 3731
Delta R.T. -0.028 min
Lab File: BN027944.D
Acq: 29 Sep 2023 02:43

Tgt Ion:202 Resp: 3422
Ion Ratio Lower Upper
202 100
101 155.8 11.4 17.0#
100 1135.0 9.1 13.7#

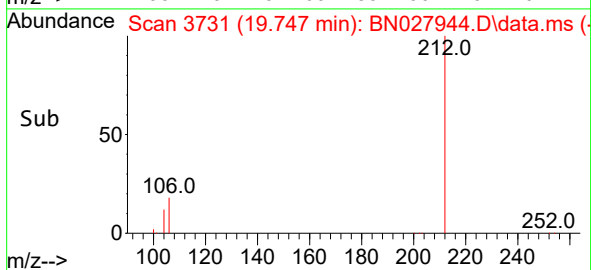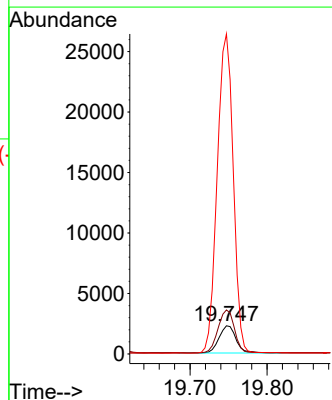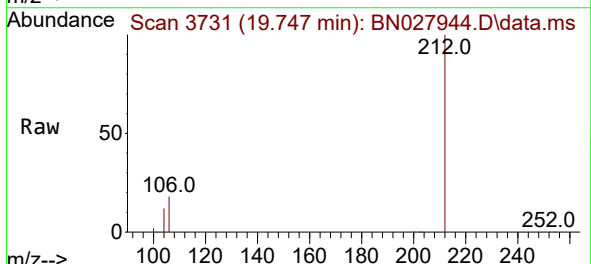

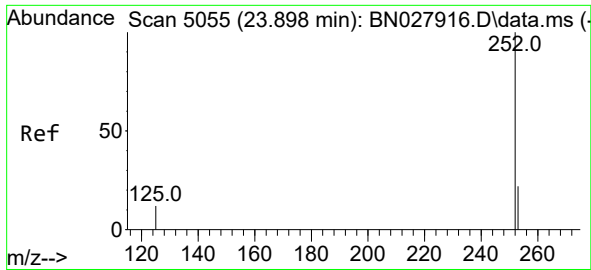

#26

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.848 min Scan# 50

Delta R.T. -0.047 min

Lab File: BN027944.D


Acq: 29 Sep 2023 02:43

Instrument :

BNA_N

ClientSampleId :

SBLK752

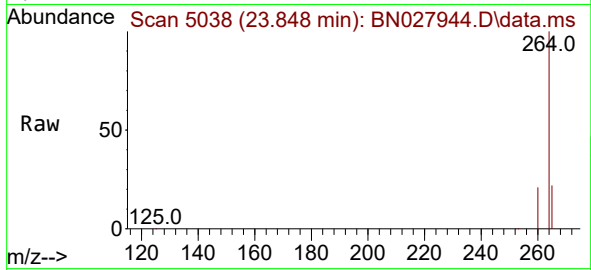

Tgt Ion:252 Resp: 6719

Ion Ratio Lower Upper

252 100

253 49.2 21.9 32.9#

125 41.7 15.5 23.3#

