

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027968.D
 Acq On : 29 Sep 2023 19:23
 Operator : MA/JU
 Sample : 04497-13
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBP6

Quant Time: Sep 30 01:06:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	7443	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	27416	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	16956	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	34874	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	22539	0.400	ng/ul	0.00
23) Perylene-d12	24.023	264	23105	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	18267	1.948	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	12919	0.311	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	27563	0.400	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	272	0.028	ng/ul#	43
20) Pyrene	19.757	202	4022	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.866	252	6167	0.074	ng/ul#	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027968.D
Acq On : 29 Sep 2023 19:23
Operator : MA/JU
Sample : 04497-13
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBBP6

Quant Time: Sep 30 01:06:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




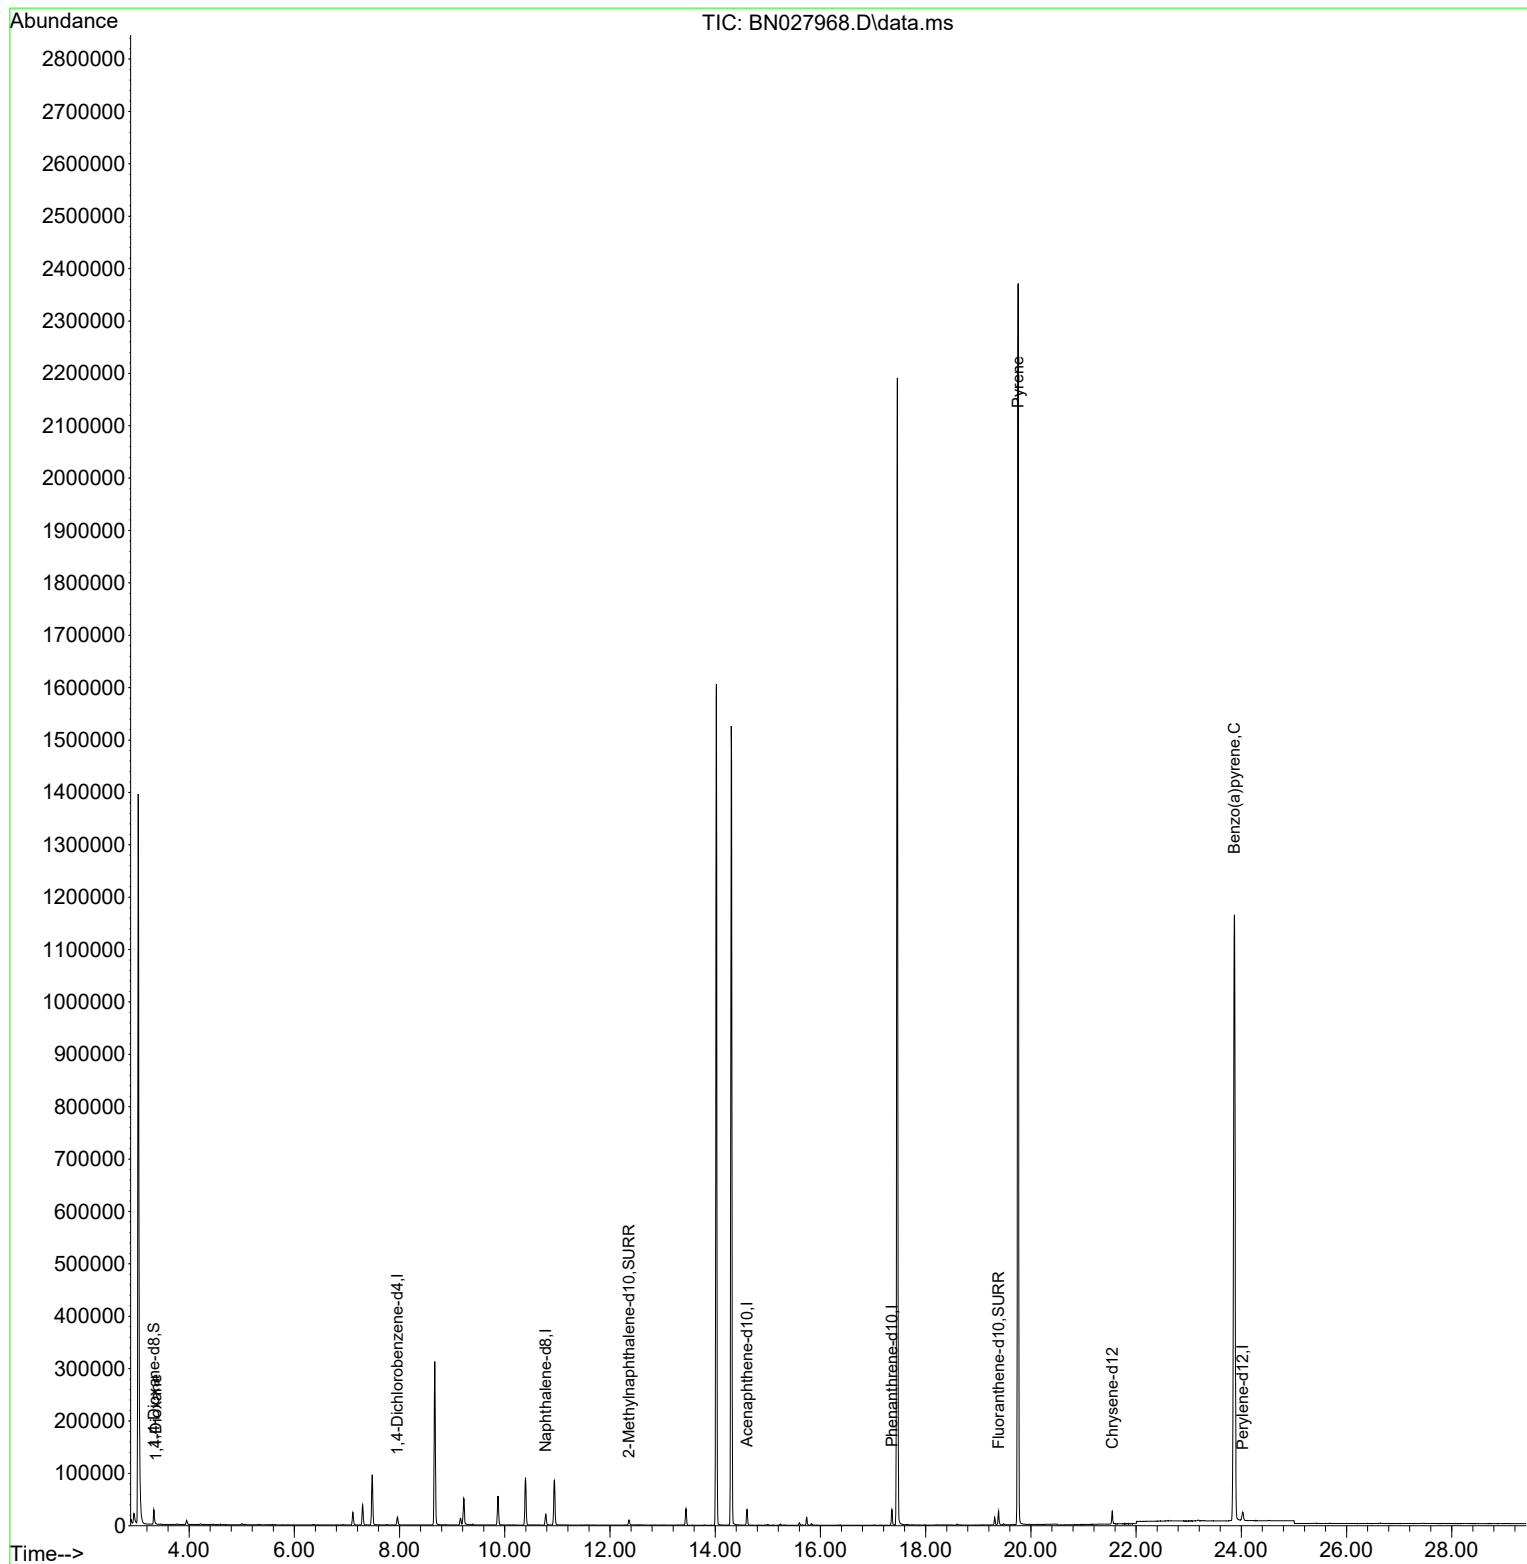


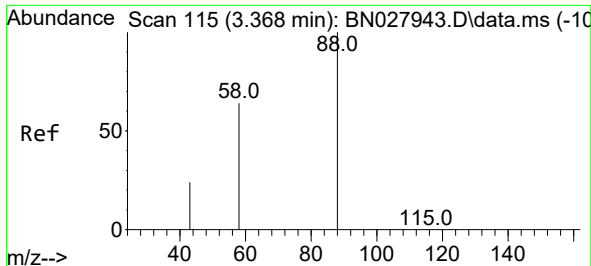

#2
1,4-Dioxane
Concen: 0.028 ng/ul
RT: 3.368 min Scan# 115
Delta R.T. 0.000 min
Lab File: BN027968.D
Acq: 29 Sep 2023 19:23




Instrument :
BNA_N
ClientSampleId :
BBBP6


Tgt Ion: 88 Resp: 272
Ion Ratio Lower Upper
88 100
43 97.8 39.6 59.4#
58 25.7 48.3 72.5#

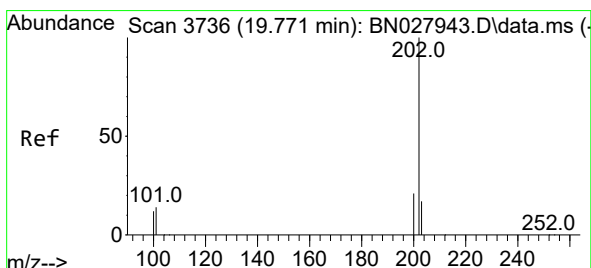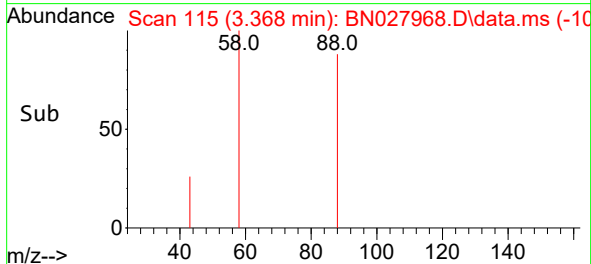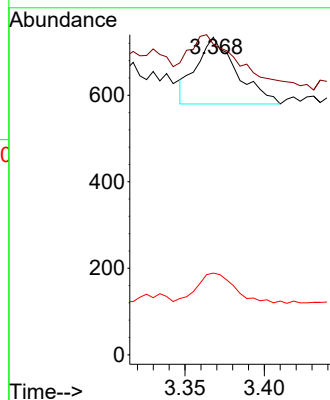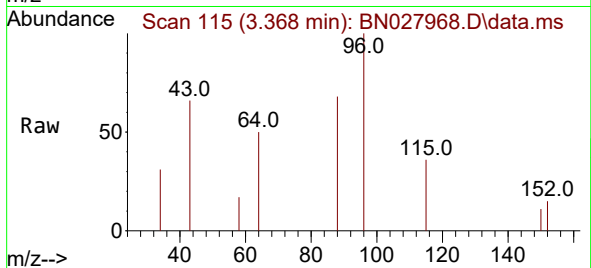

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.757 min Scan# 3733
Delta R.T. -0.019 min
Lab File: BN027968.D
Acq: 29 Sep 2023 19:23


Tgt Ion: 202 Resp: 4022
Ion Ratio Lower Upper
202 100
101 144.9 11.4 17.0#
100 974.5 9.1 13.7#

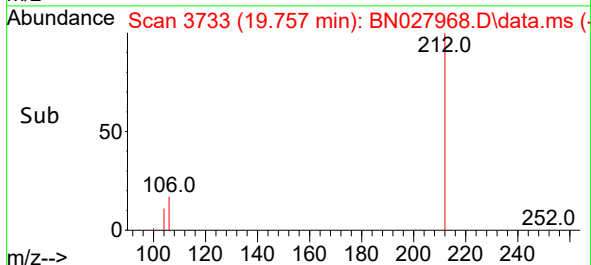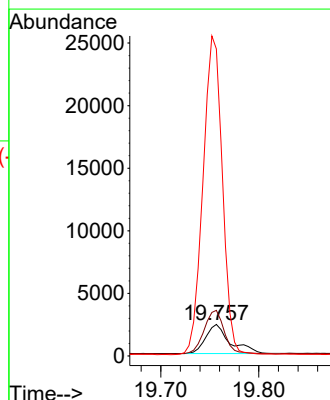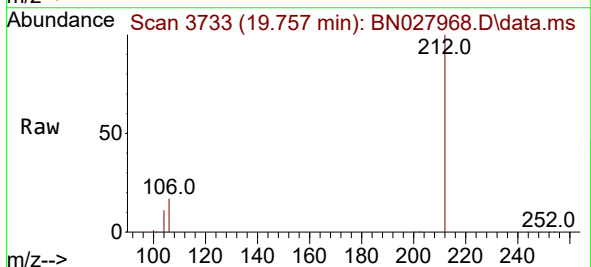

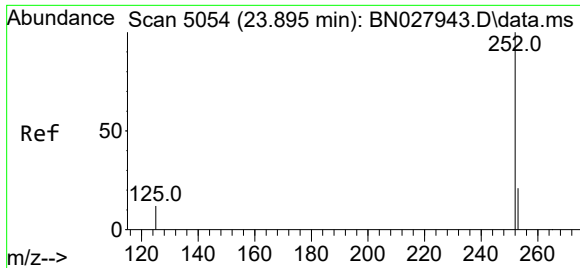

#26
 Benzo(a)pyrene
 Concen: 0.074 ng/ul
 RT: 23.866 min Scan# 50
 Delta R.T. -0.029 min
 Lab File: BN027968.D
 Acq: 29 Sep 2023 19:23

Instrument :
 BNA_N
 ClientSampleId :
 BBBP6

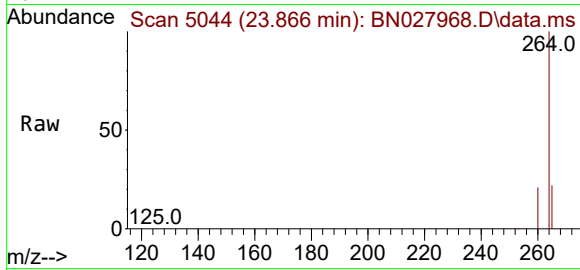

Tgt Ion:252 Resp: 6167

Ion	Ratio	Lower	Upper
252	100		
253	66.2	21.9	32.9#
125	60.8	15.5	23.3#

