

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027970.D
 Acq On : 29 Sep 2023 21:12
 Operator : MA/JU
 Sample : PB155869BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK869

Quant Time: Sep 30 01:06:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	7458	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	28076	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	17250	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	36102	0.400	ng/ul	0.00
17) Chrysene-d12	21.542	240	25200	0.400	ng/ul	0.00
23) Perylene-d12	24.021	264	24938	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	36793	3.917	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	9852	0.232	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	20624	0.268	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.596	166	3068	0.040	ng/ul#	15
20) Pyrene	19.752	202	2628	0.025	ng/ul#	1
26) Benzo(a)pyrene	23.860	252	4278	0.048	ng/ul#	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027970.D
Acq On : 29 Sep 2023 21:12
Operator : MA/JU
Sample : PB155869BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK869

Quant Time: Sep 30 01:06:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




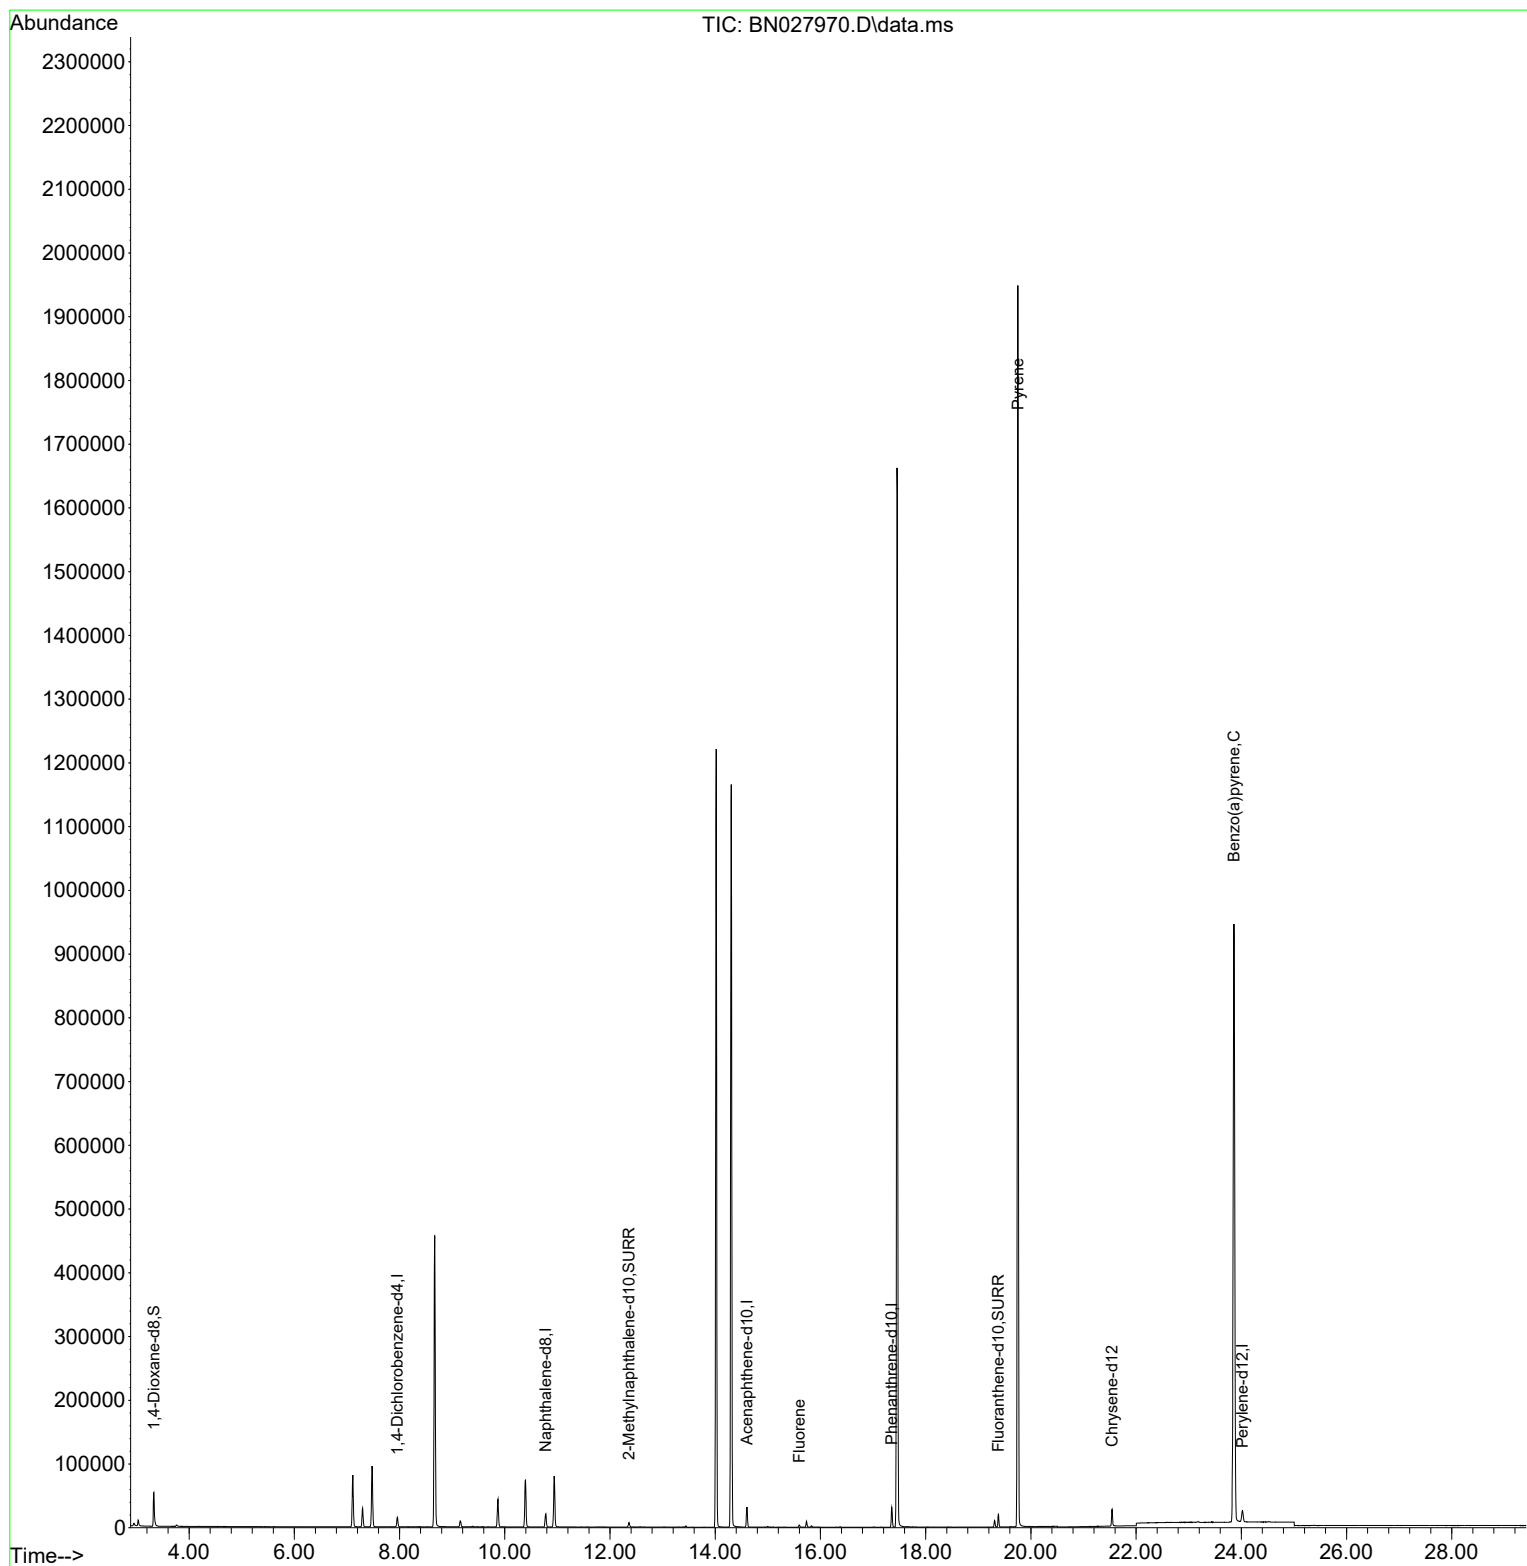


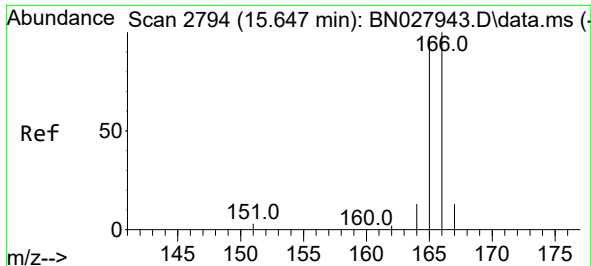

#12
Fluorene
Concen: 0.040 ng/ul
RT: 15.596 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN027970.D
Acq: 29 Sep 2023 21:12




Instrument :
BNA_N
ClientSampleId :
SBLK869


Tgt Ion:166 Resp: 3068
Ion Ratio Lower Upper
166 100
165 8.7 78.0 117.0#
167 33.8 11.4 17.2#

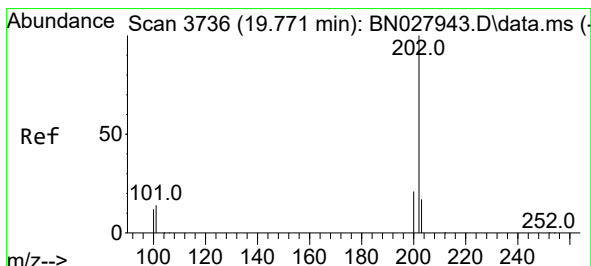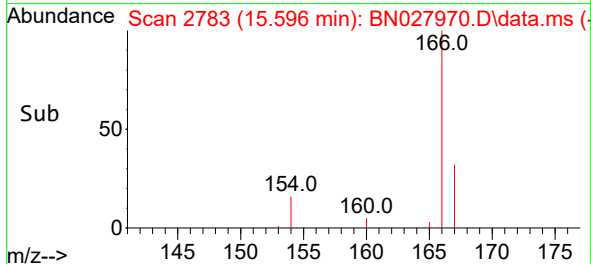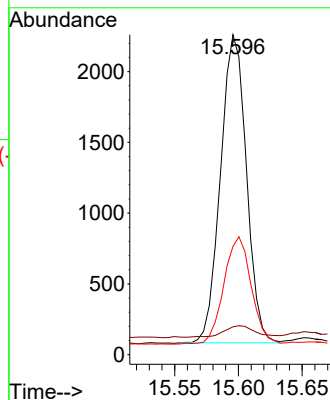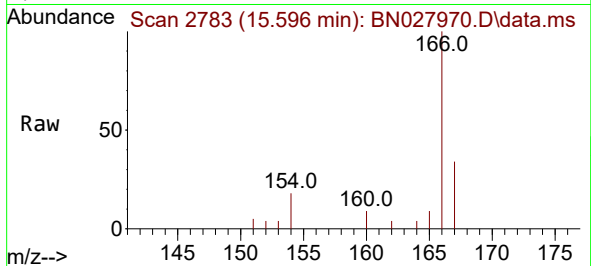

#20
Pyrene
Concen: 0.025 ng/ul
RT: 19.752 min Scan# 3732
Delta R.T. -0.023 min
Lab File: BN027970.D
Acq: 29 Sep 2023 21:12


Tgt Ion:202 Resp: 2628
Ion Ratio Lower Upper
202 100
101 147.6 11.4 17.0#
100 1026.8 9.1 13.7#

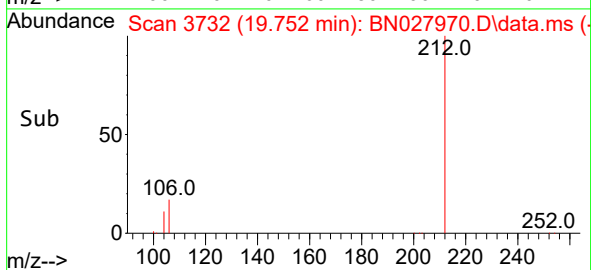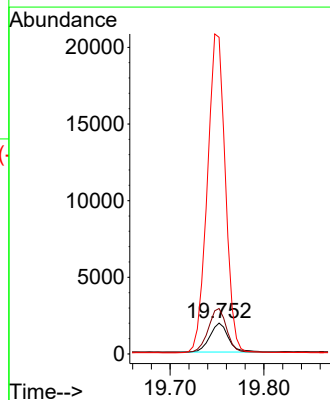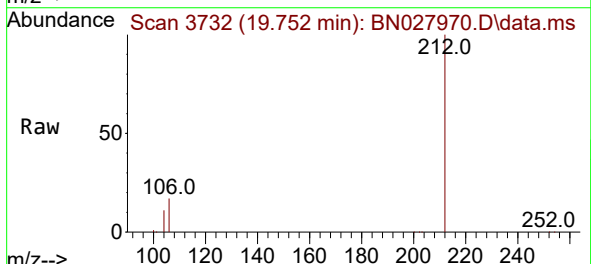

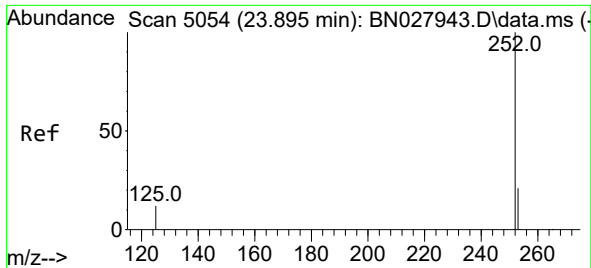

#26
Benzo(a)pyrene
Concen: 0.048 ng/ul
RT: 23.860 min Scan# 50
Delta R.T. -0.035 min
Lab File: BN027970.D
Acq: 29 Sep 2023 21:12

Instrument :
BNA_N
ClientSampleId :
SBLK869

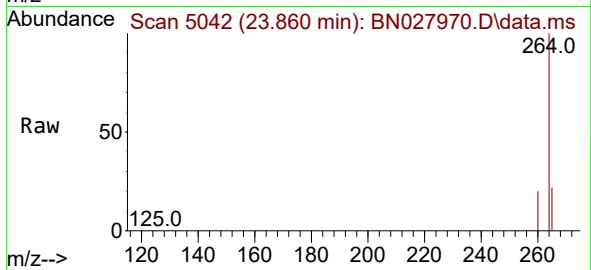

Tgt Ion:252 Resp: 4278
Ion Ratio Lower Upper
252 100
253 68.9 21.9 32.9#
125 59.7 15.5 23.3#

