

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027971.D
 Acq On : 29 Sep 2023 21:48
 Operator : MA/JU
 Sample : PB155872BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK872

Quant Time: Sep 30 01:06:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6056	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	23013	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	14199	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	30559	0.400	ng/ul	0.00
17) Chrysene-d12	21.542	240	23418	0.400	ng/ul	0.00
23) Perylene-d12	24.018	264	23584	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	33680	4.415	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	9203	0.264	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	20460	0.286	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.596	166	2893	0.046	ng/ul#	15
20) Pyrene	19.752	202	2631	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.860	252	4401	0.052	ng/ul#	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027971.D
Acq On : 29 Sep 2023 21:48
Operator : MA/JU
Sample : PB155872BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK872

Quant Time: Sep 30 01:06:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




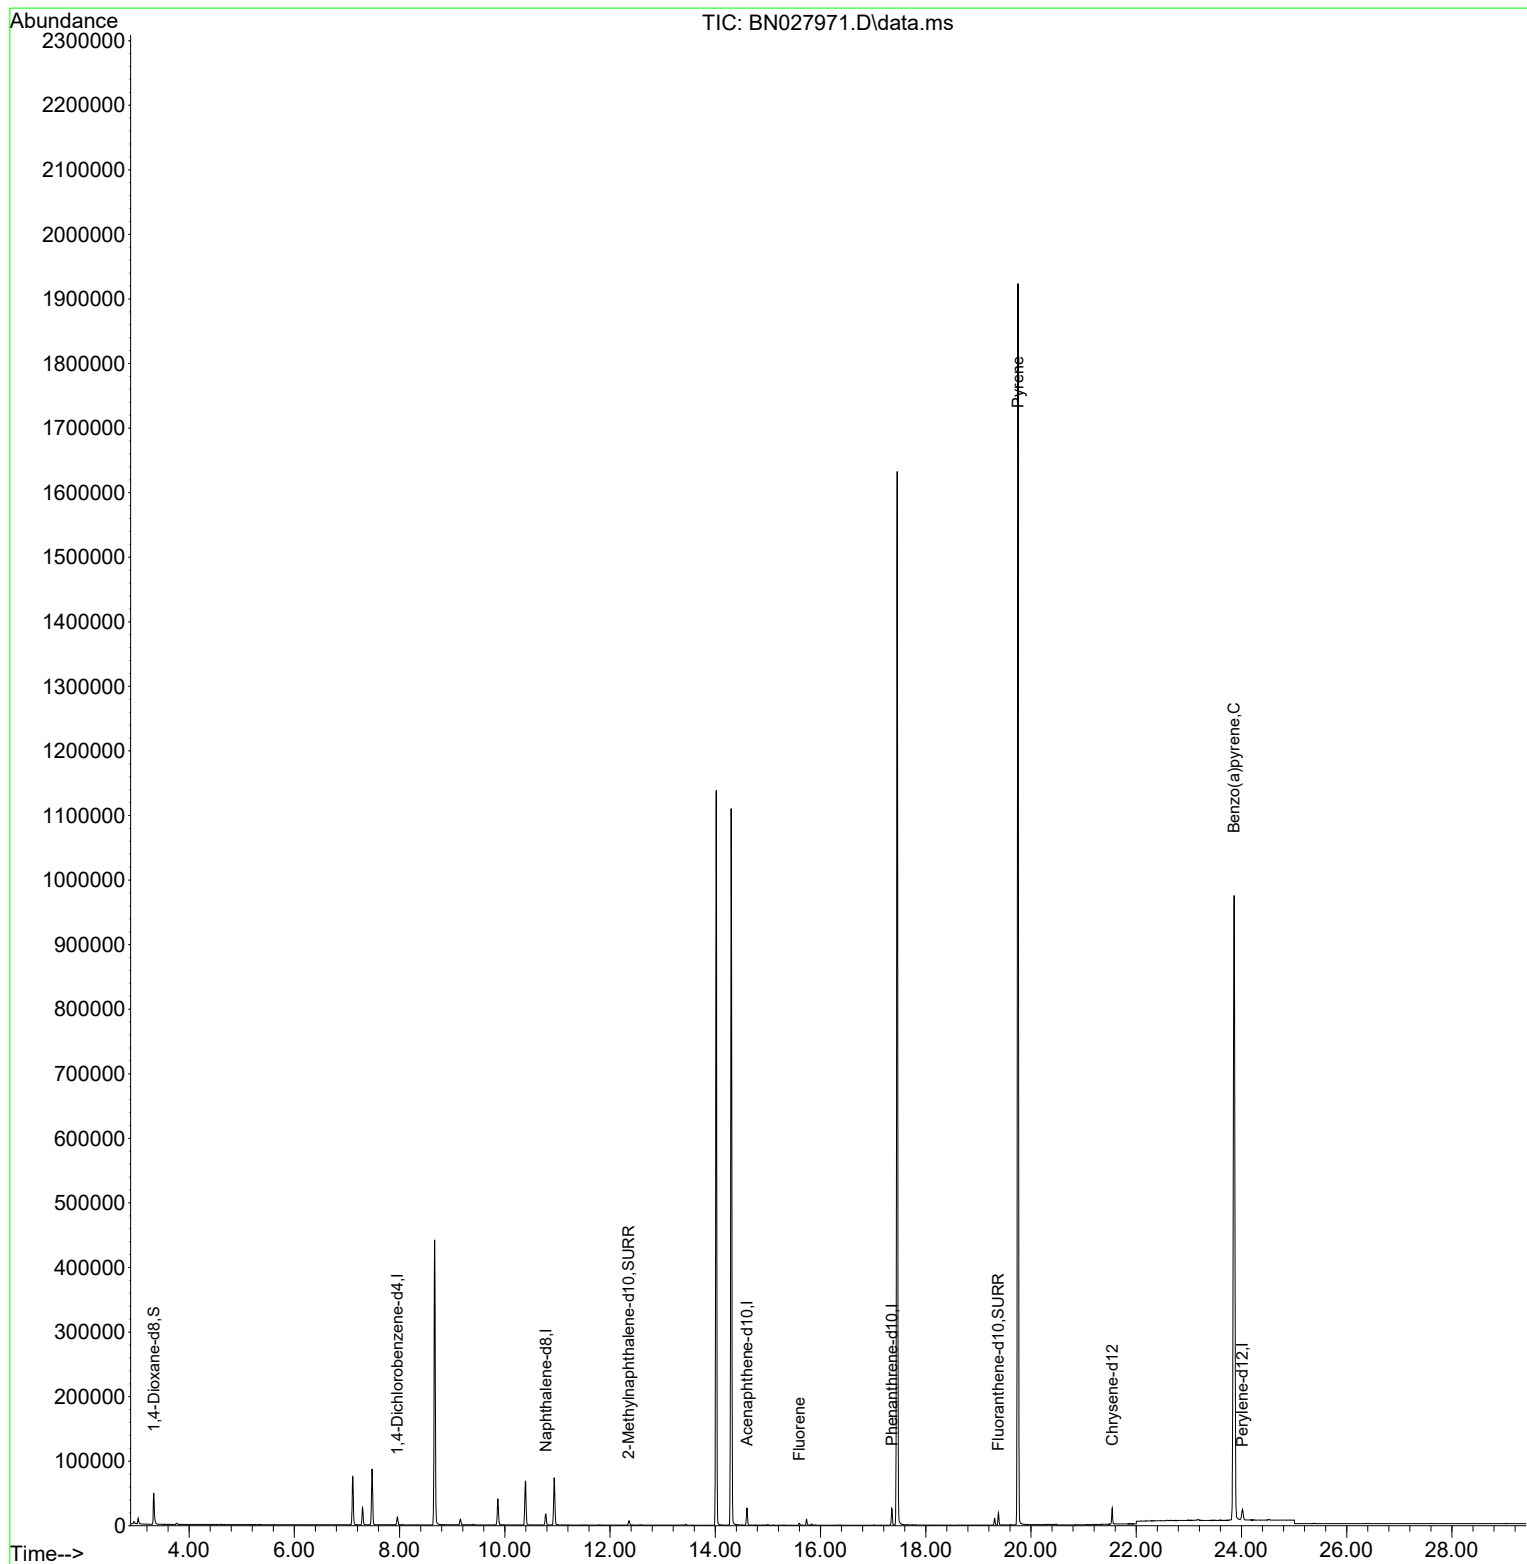


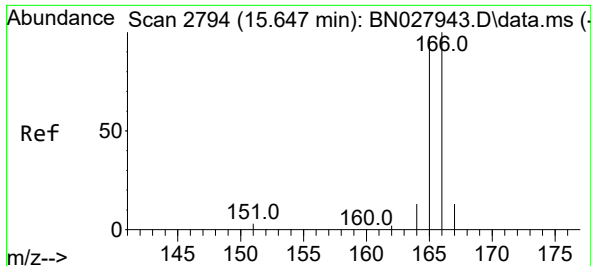

#12
Fluorene
Concen: 0.046 ng/ul
RT: 15.596 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN027971.D
Acq: 29 Sep 2023 21:48




Instrument :
BNA_N
ClientSampleId :
SBLK872


Tgt Ion:166 Resp: 2893
Ion Ratio Lower Upper
166 100
165 8.8 78.0 117.0#
167 35.2 11.4 17.2#

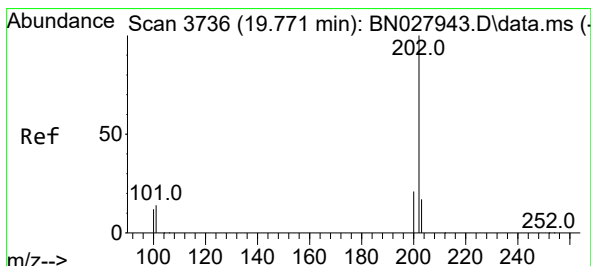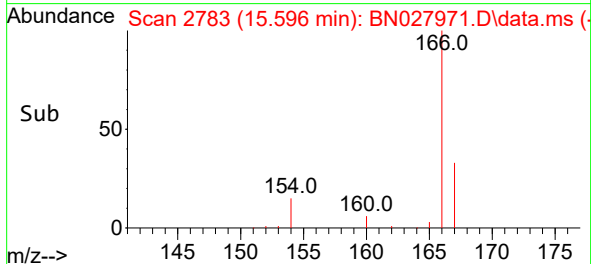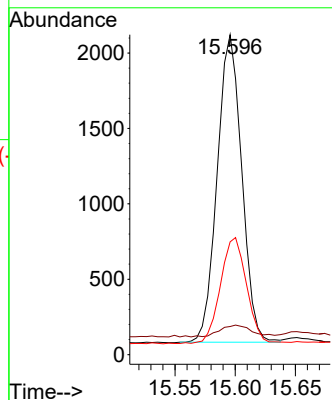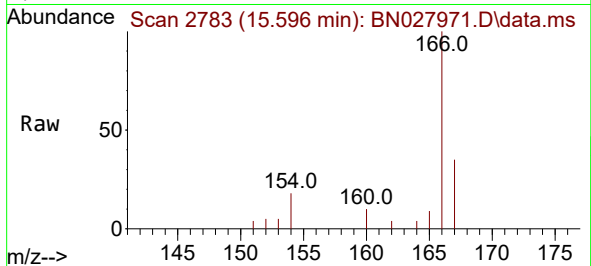

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.752 min Scan# 3732
Delta R.T. -0.023 min
Lab File: BN027971.D
Acq: 29 Sep 2023 21:48


Tgt Ion:202 Resp: 2631
Ion Ratio Lower Upper
202 100
101 150.3 11.4 17.0#
100 1034.0 9.1 13.7#

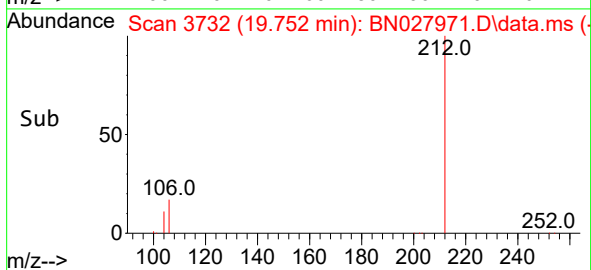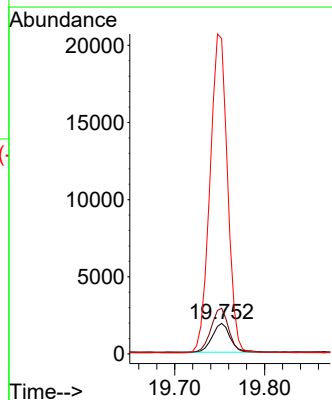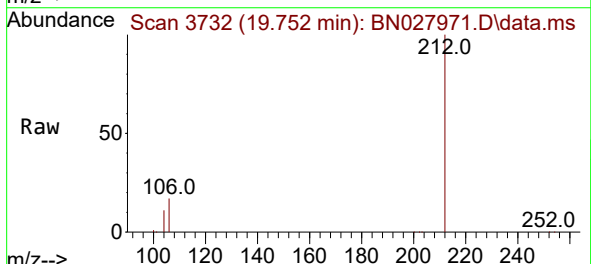

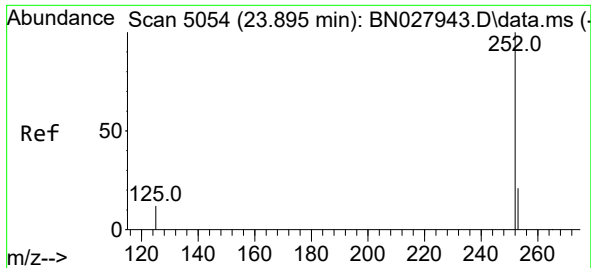

#26
Benzo(a)pyrene
Concen: 0.052 ng/ul
RT: 23.860 min Scan# 50
Delta R.T. -0.035 min
Lab File: BN027971.D
Acq: 29 Sep 2023 21:48

Instrument :
BNA_N
ClientSampleId :
SBLK872

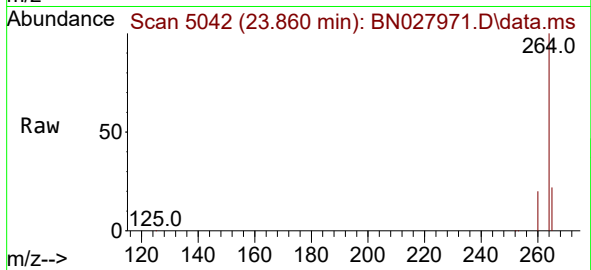

Tgt Ion:252 Resp: 4401
Ion Ratio Lower Upper
252 100
253 68.2 21.9 32.9#
125 59.5 15.5 23.3#

