

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027973.D
 Acq On : 29 Sep 2023 23:01
 Operator : MA/JU
 Sample : 04497-15
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ60

Quant Time: Sep 30 01:06:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6289	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	23778	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	14247	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	30282	0.400	ng/ul	0.00
17) Chrysene-d12	21.542	240	21027	0.400	ng/ul	0.00
23) Perylene-d12	24.018	264	20540	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.357	152	10812	0.300	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	25339	0.395	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	1007	0.122	ng/ul#	73
20) Pyrene	19.752	202	3343	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.857	252	5297	0.072	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027973.D
Acq On : 29 Sep 2023 23:01
Operator : MA/JU
Sample : 04497-15
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ60

Quant Time: Sep 30 01:06:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




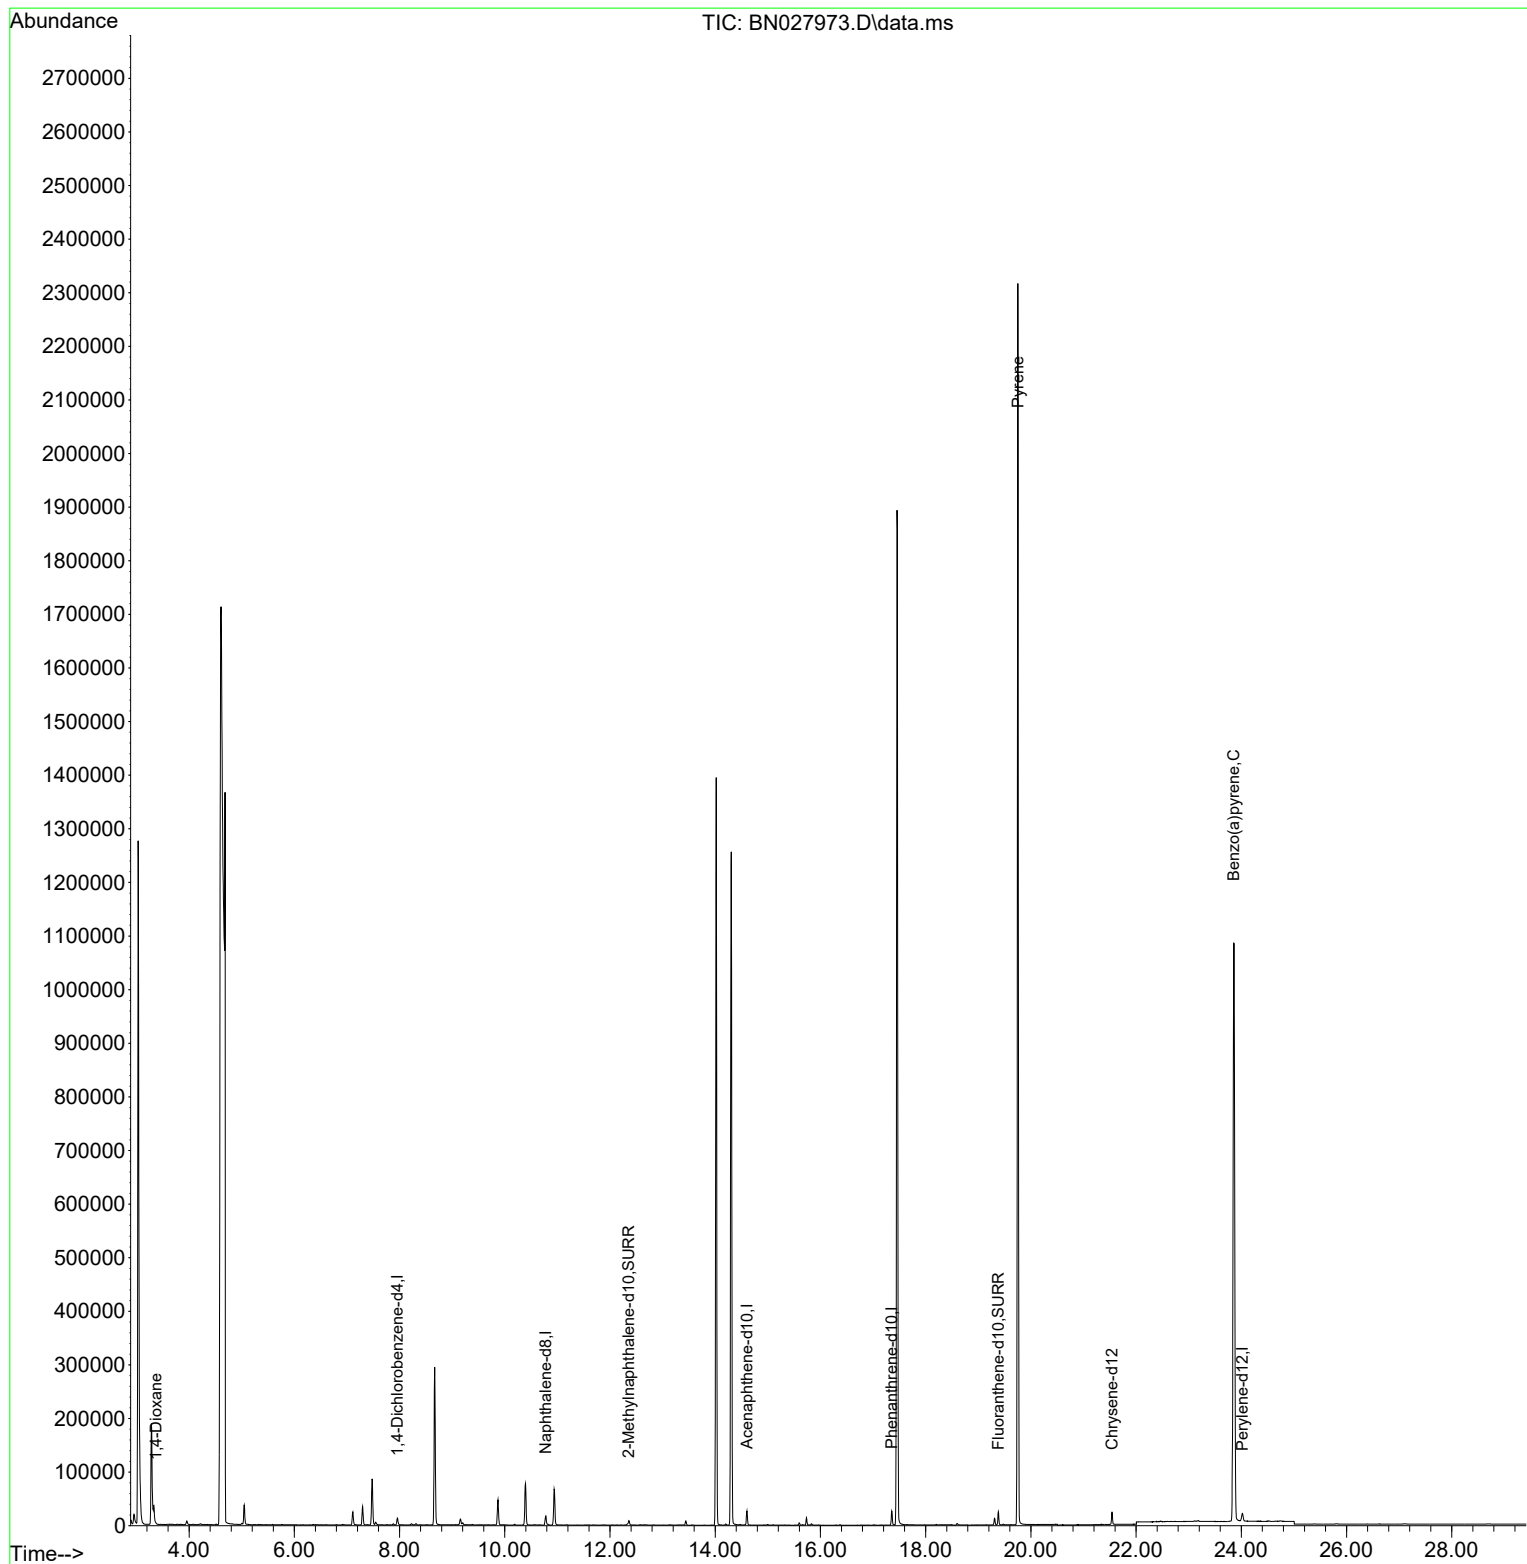


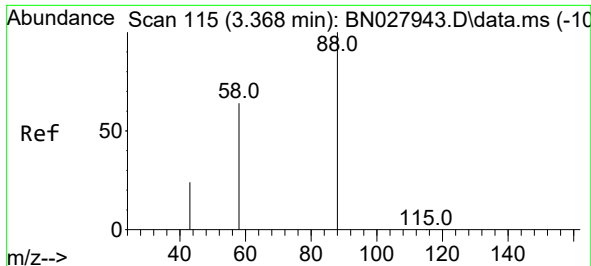

#2
1,4-Dioxane
Concen: 0.122 ng/ul
RT: 3.368 min Scan# 115
Delta R.T. 0.000 min
Lab File: BN027973.D
Acq: 29 Sep 2023 23:01




Instrument :
BNA_N
ClientSampleId :
BBJ60


Tgt Ion: 88 Resp: 1007
Ion Ratio Lower Upper
88 100
43 83.5 39.6 59.4#
58 53.7 48.3 72.5

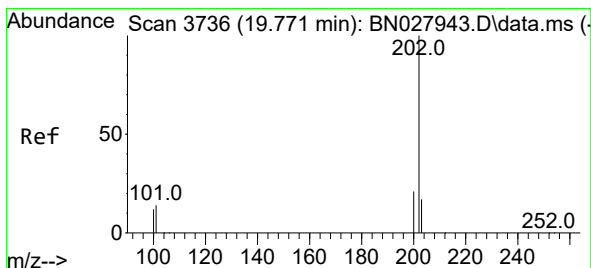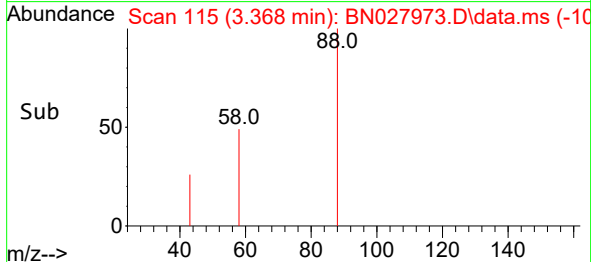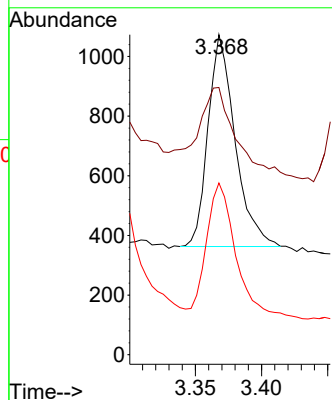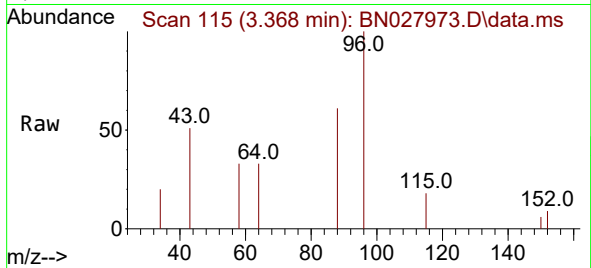

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.752 min Scan# 3732
Delta R.T. -0.023 min
Lab File: BN027973.D
Acq: 29 Sep 2023 23:01


Tgt Ion: 202 Resp: 3343
Ion Ratio Lower Upper
202 100
101 143.5 11.4 17.0#
100 997.7 9.1 13.7#

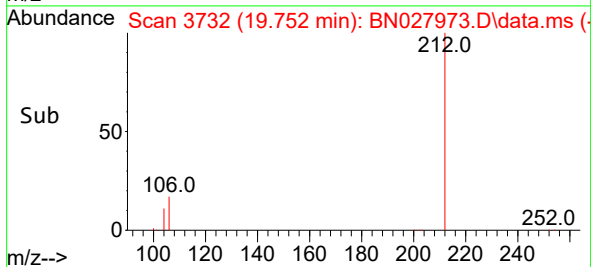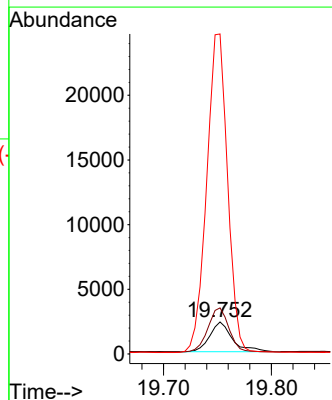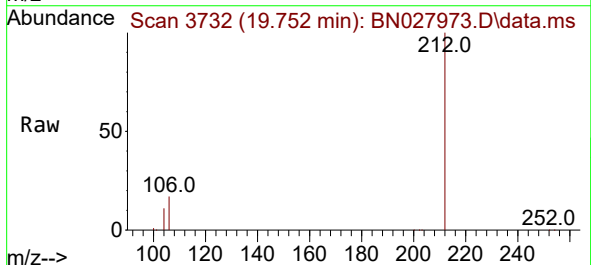

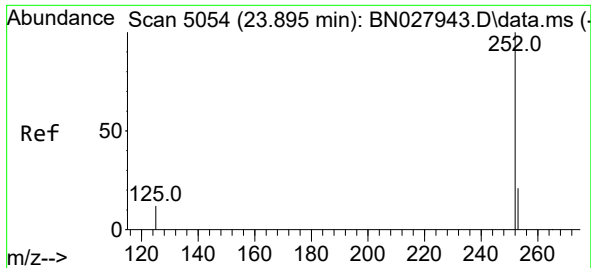

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.857 min Scan# 50
Delta R.T. -0.038 min
Lab File: BN027973.D
Acq: 29 Sep 2023 23:01

Instrument :
BNA_N
ClientSampleId :
BBJ60

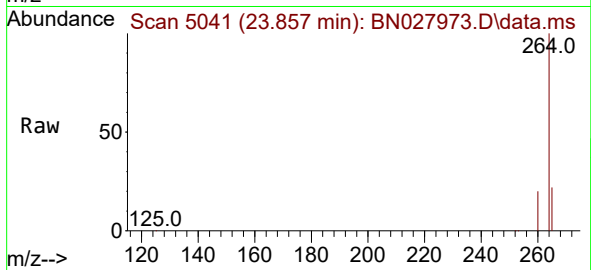

Tgt Ion:252 Resp: 5297
Ion Ratio Lower Upper
252 100
253 62.6 21.9 32.9#
125 56.6 15.5 23.3#

