




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027955.D
 Acq On : 29 Sep 2023 09:20
 Operator : MA/JU
 Sample : 04417-33DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYN2DL

Manual IntegrationsAPPROVED

Quant Time: Sep 29 10:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

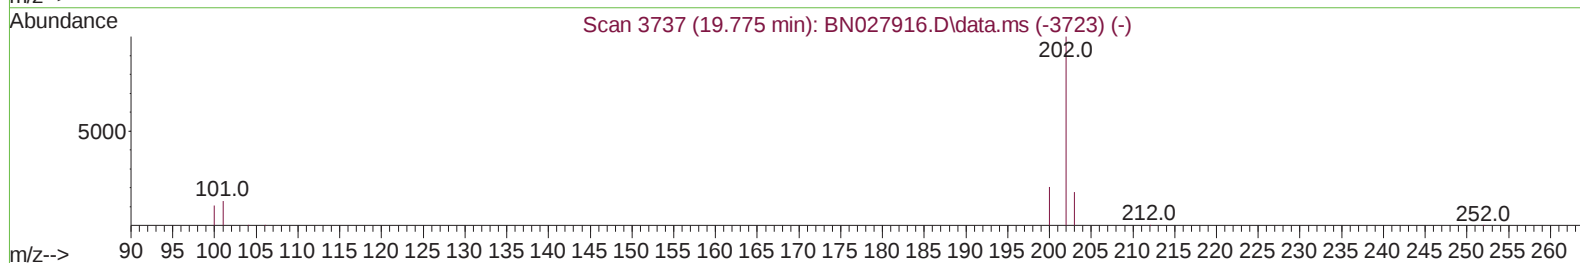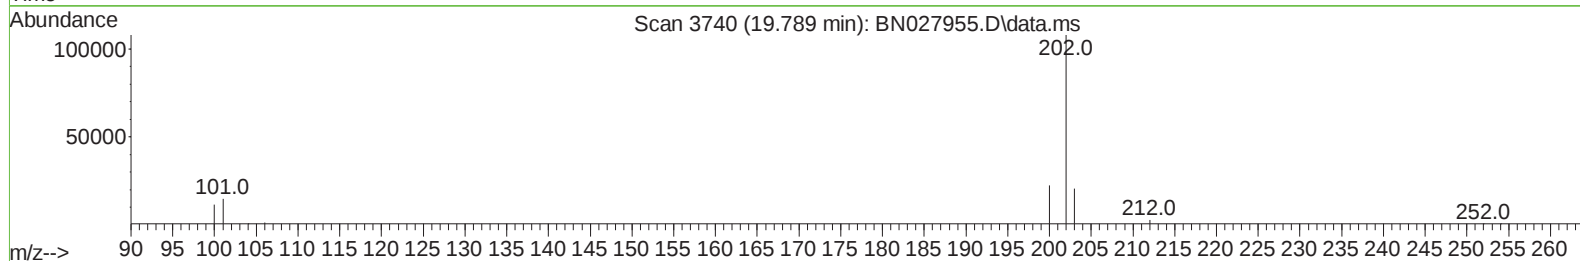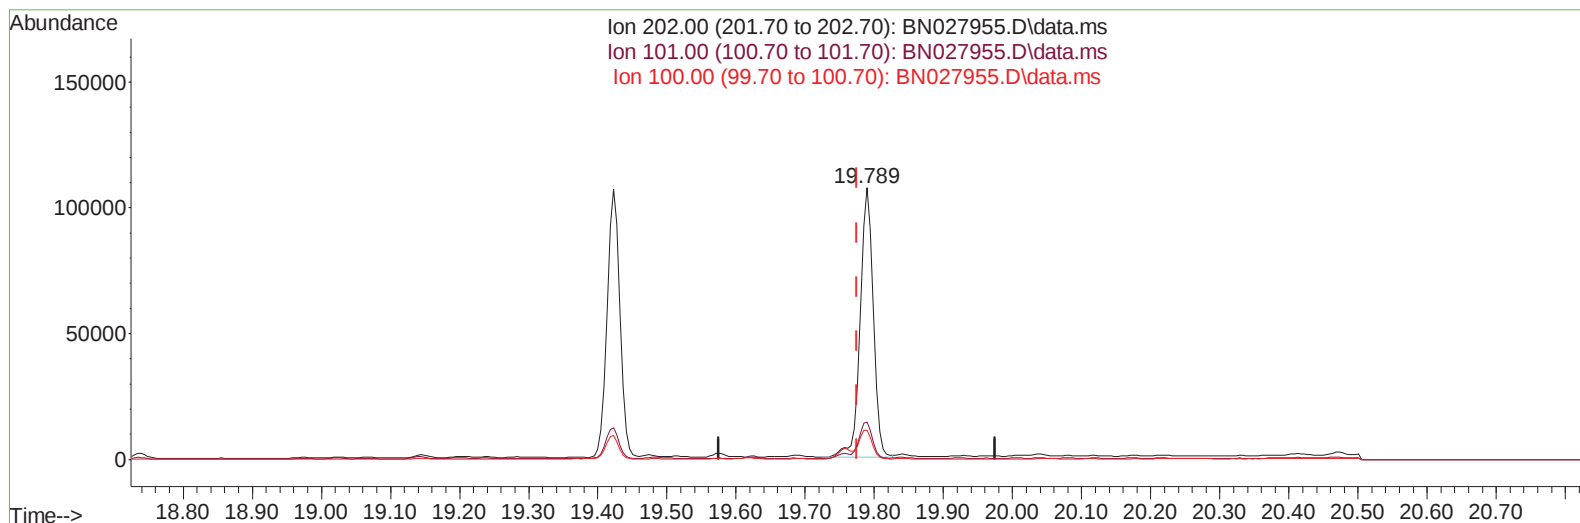

TIC: BN027955.D\data.ms

(20) Pyrene

19.789min (+ 0.014) 2.43 ng/u1

response 142084

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	13.82
100.00	11.40	10.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027955.D
 Acq On : 29 Sep 2023 09:20
 Operator : MA/JU
 Sample : 04417-33DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYN2DL

Manual IntegrationsAPPROVED

Quant Time: Sep 29 10:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

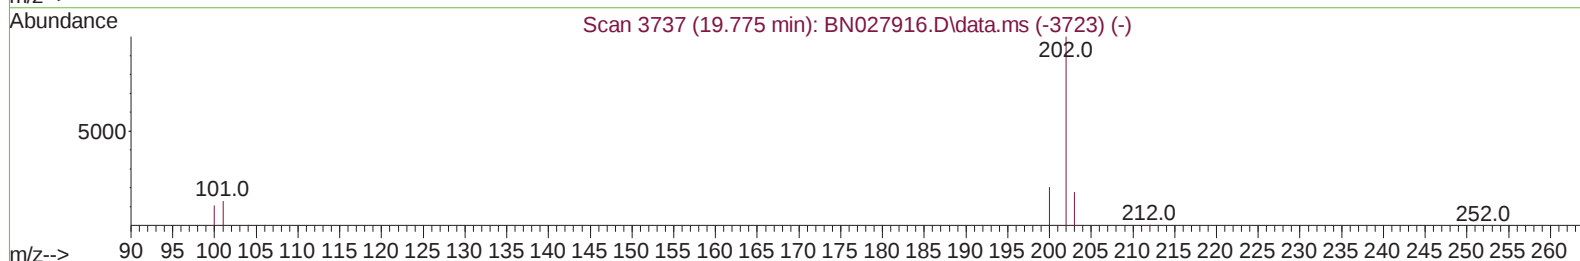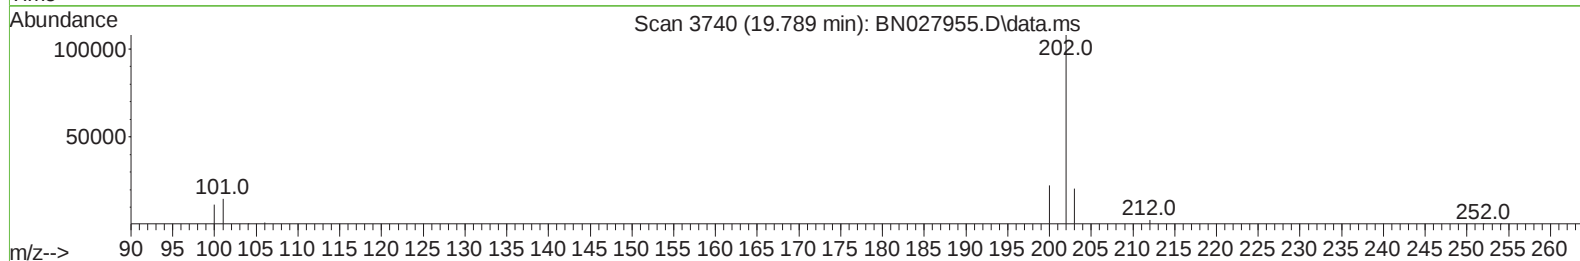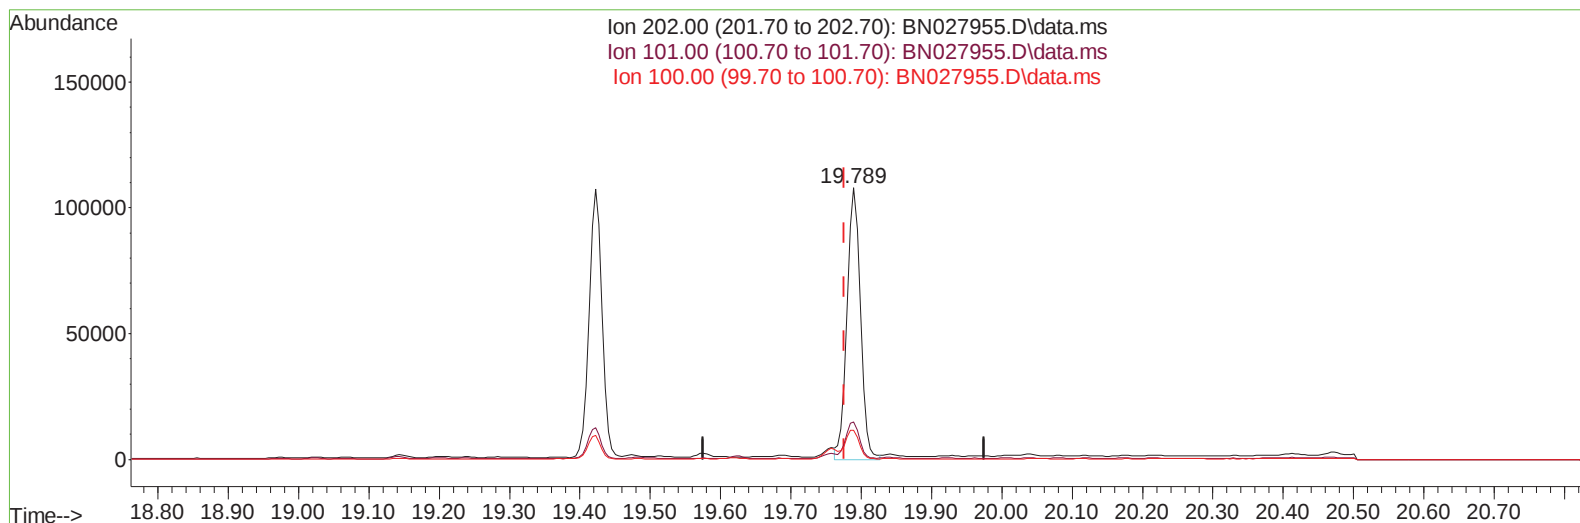

TIC: BN027955.D\data.ms

(20) Pyrene

19.789min (+ 0.014) 2.42 ng/ul m

response 141708

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	13.82
100.00	11.40	10.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027955.D
 Acq On : 29 Sep 2023 09:20
 Operator : MA/JU
 Sample : 04417-33DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYN2DL

Manual IntegrationsAPPROVED

Quant Time: Sep 29 10:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

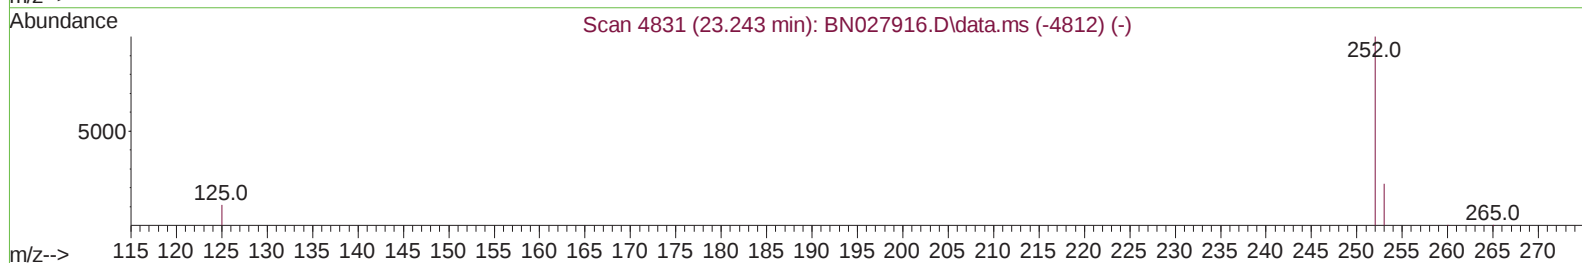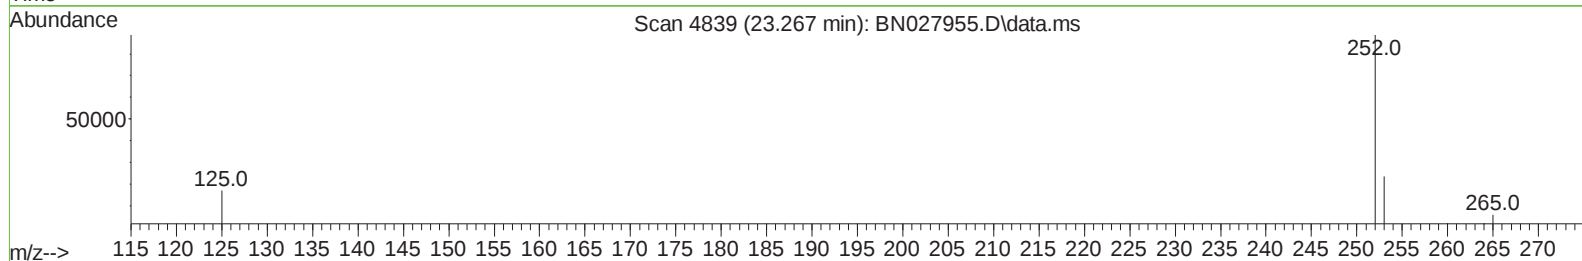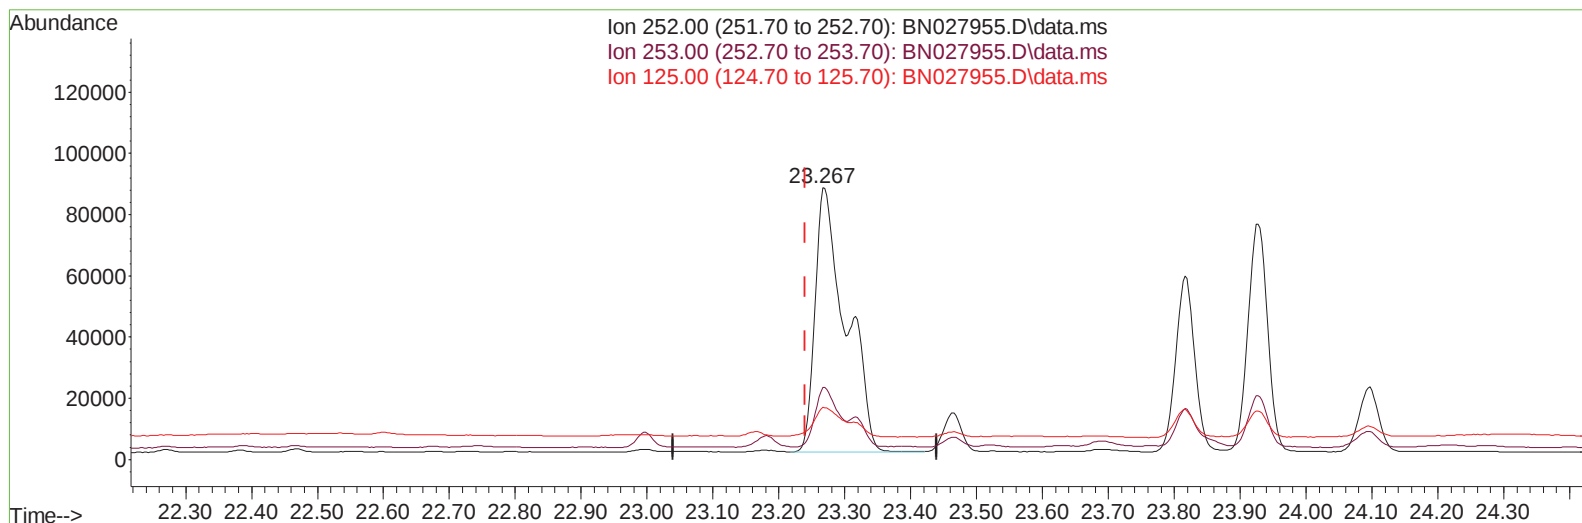

TIC: BN027955.D\data.ms

(24) Benzo(b)fluoranthene

23.267min (+ 0.026) 4.31 ng/u1

response 281116

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	26.49
125.00	15.70	19.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027955.D
 Acq On : 29 Sep 2023 09:20
 Operator : MA/JU
 Sample : 04417-33DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYN2DL

Manual IntegrationsAPPROVED

Quant Time: Sep 29 10:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

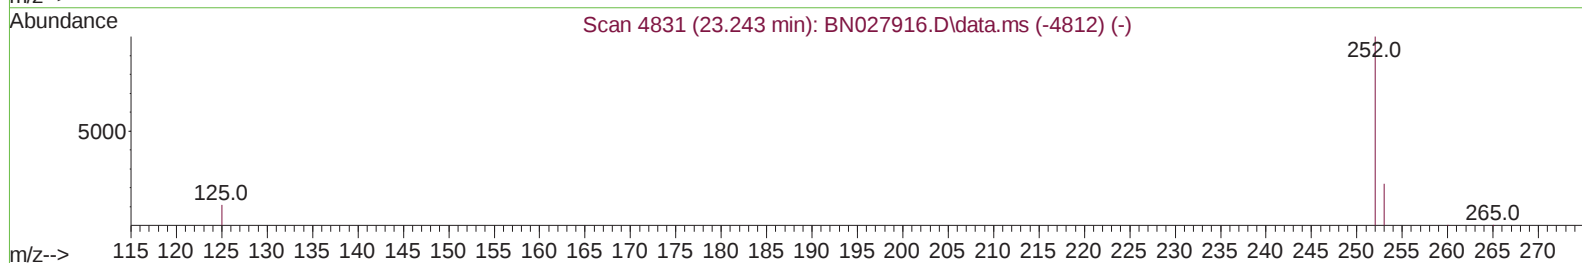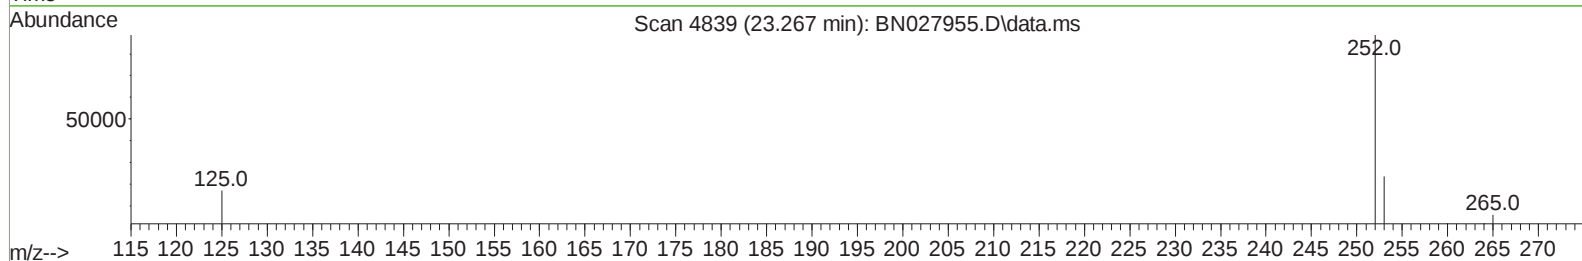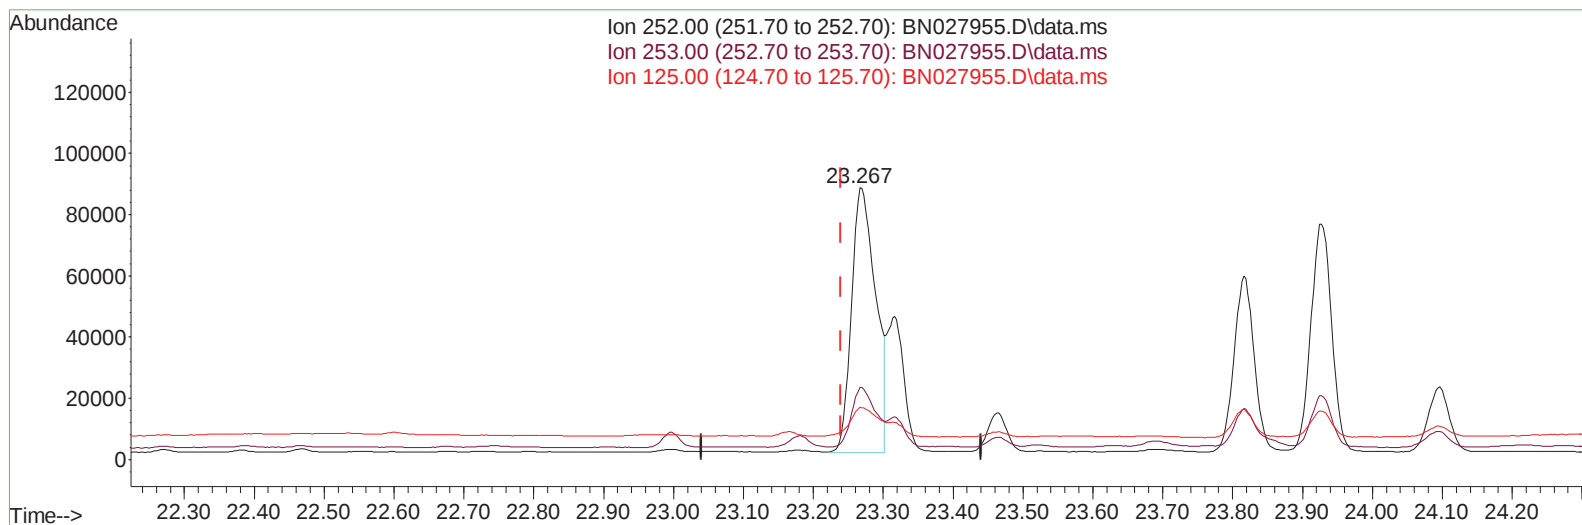

TIC: BN027955.D\data.ms

(24) Benzo(b)fluoranthene

23.267min (+ 0.026) 3.17 ng/u1 m

response 206857

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	26.49
125.00	15.70	19.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027955.D
 Acq On : 29 Sep 2023 09:20
 Operator : MA/JU
 Sample : 04417-33DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYN2DL

Manual IntegrationsAPPROVED

Quant Time: Sep 29 10:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

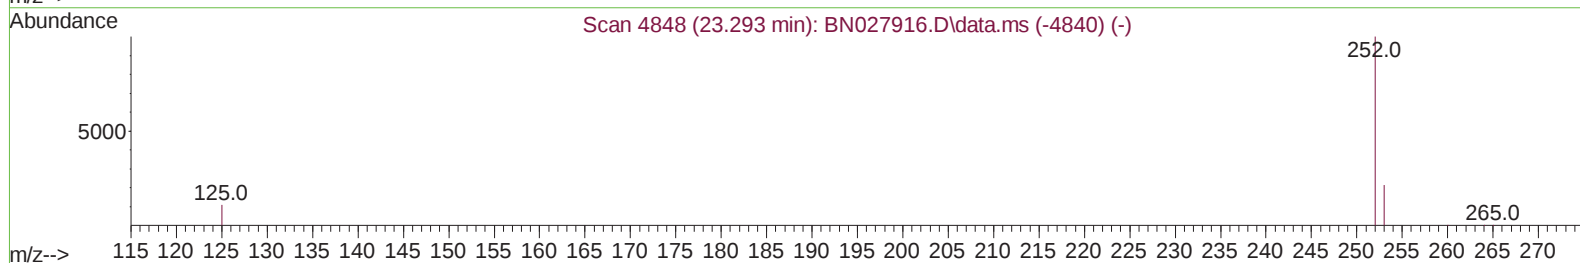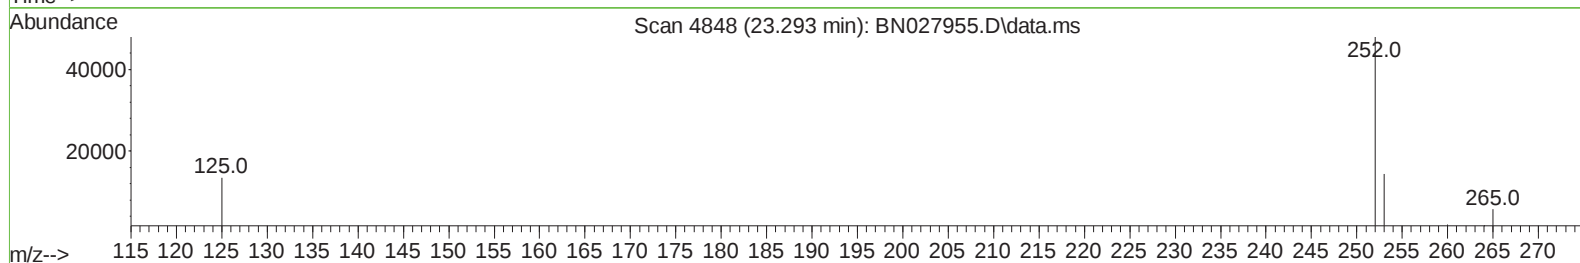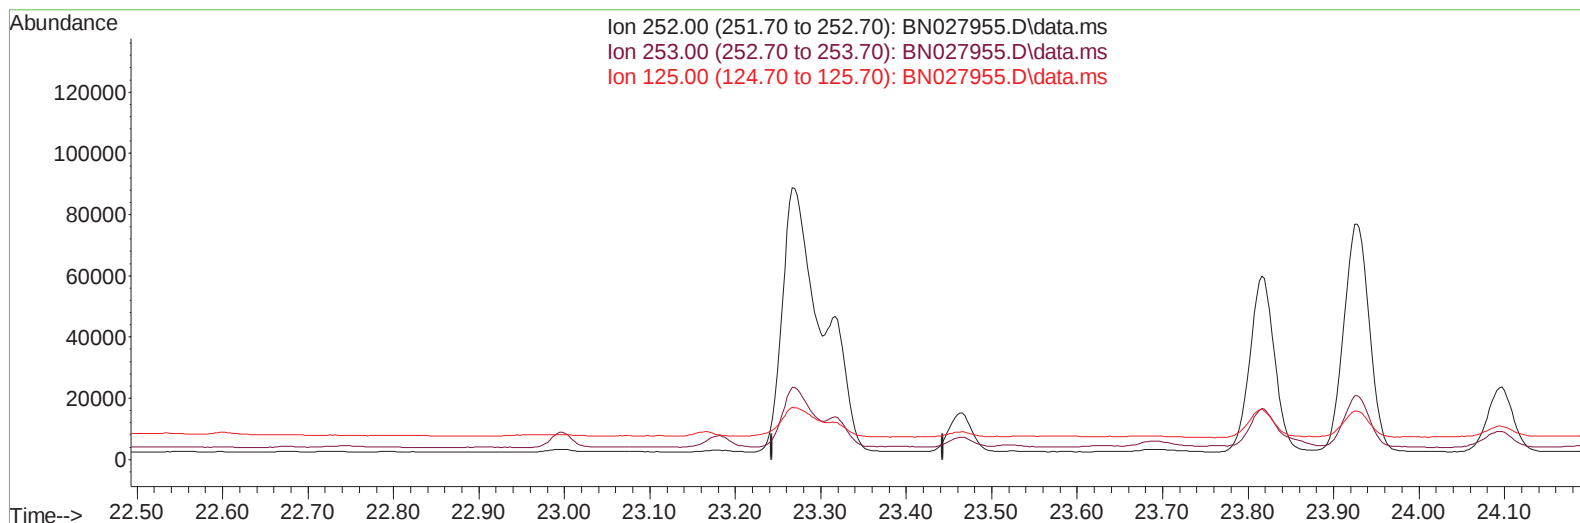

TIC: BN027955.D\data.ms

(25) Benzo(k)fluoranthene

23.293min (-23.293) 0.00 ng/u1

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	24.90	0.00#
125.00	15.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027955.D
Acq On : 29 Sep 2023 09:20
Operator : MA/JU
Sample : 04417-33DL 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZYN2DL

Manual IntegrationsAPPROVED

Quant Time: Sep 29 10:47:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023

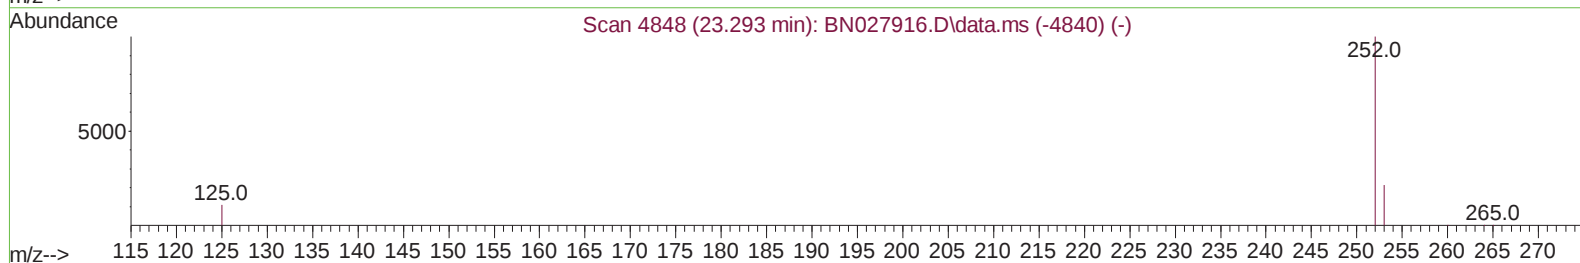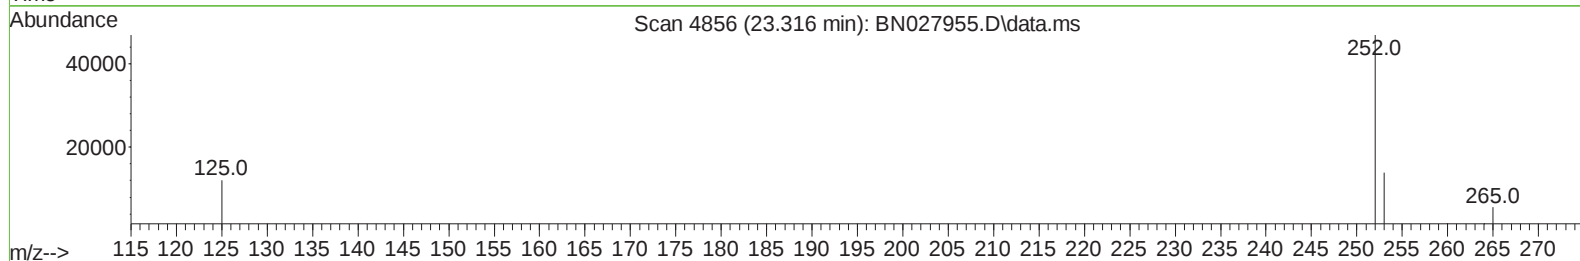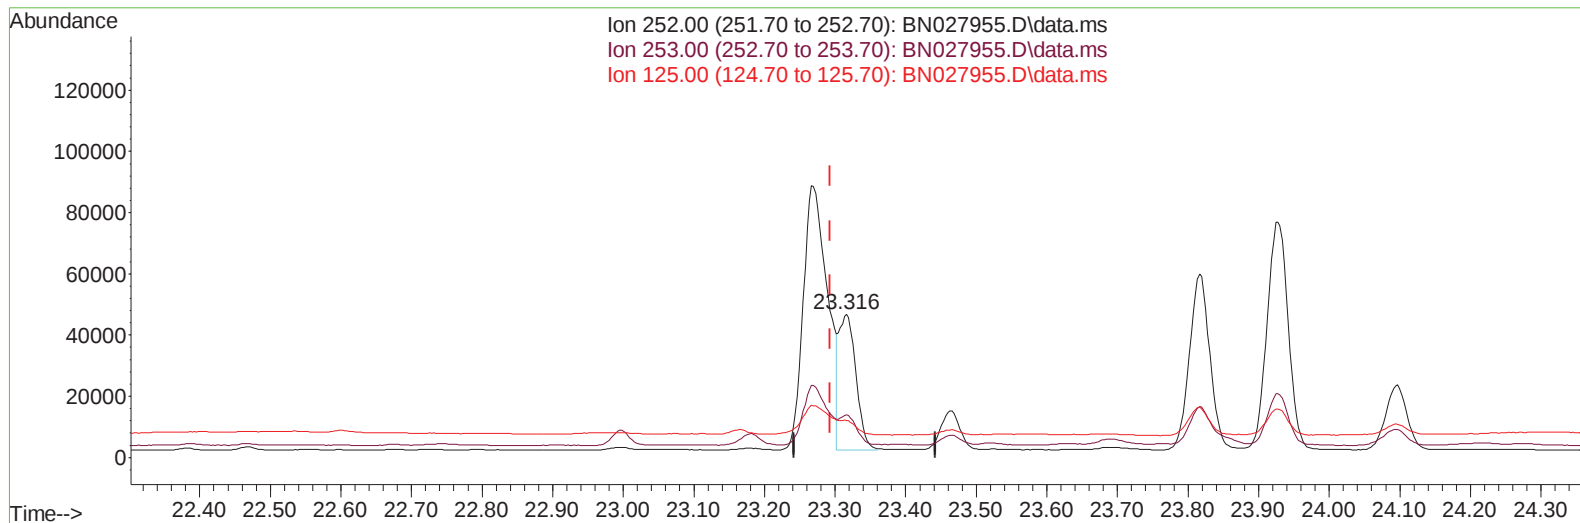

TIC: BN027955.D\data.ms

(25) Benzo(k)fluoranthene

23.316min (+ 0.023) 1.18 ng/ul m

response 74674

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.90	29.78
125.00	15.80	25.81#
0.00	0.00	0.00