




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027967.D
 Acq On : 29 Sep 2023 18:47
 Operator : MA/JU
 Sample : 04497-12
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ14

Manual IntegrationsAPPROVED

Quant Time: Sep 30 01:25:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

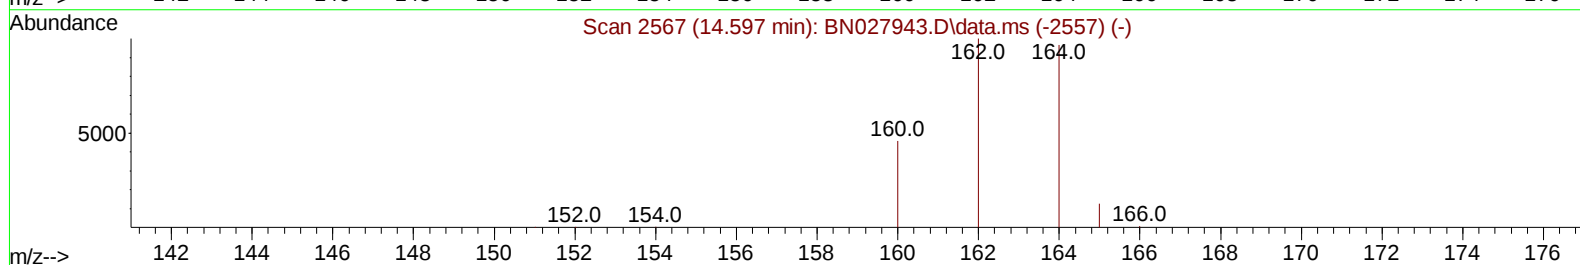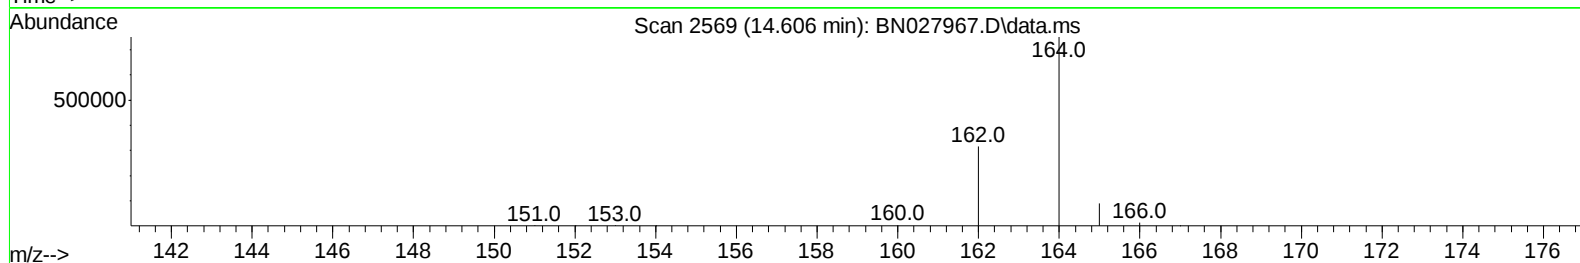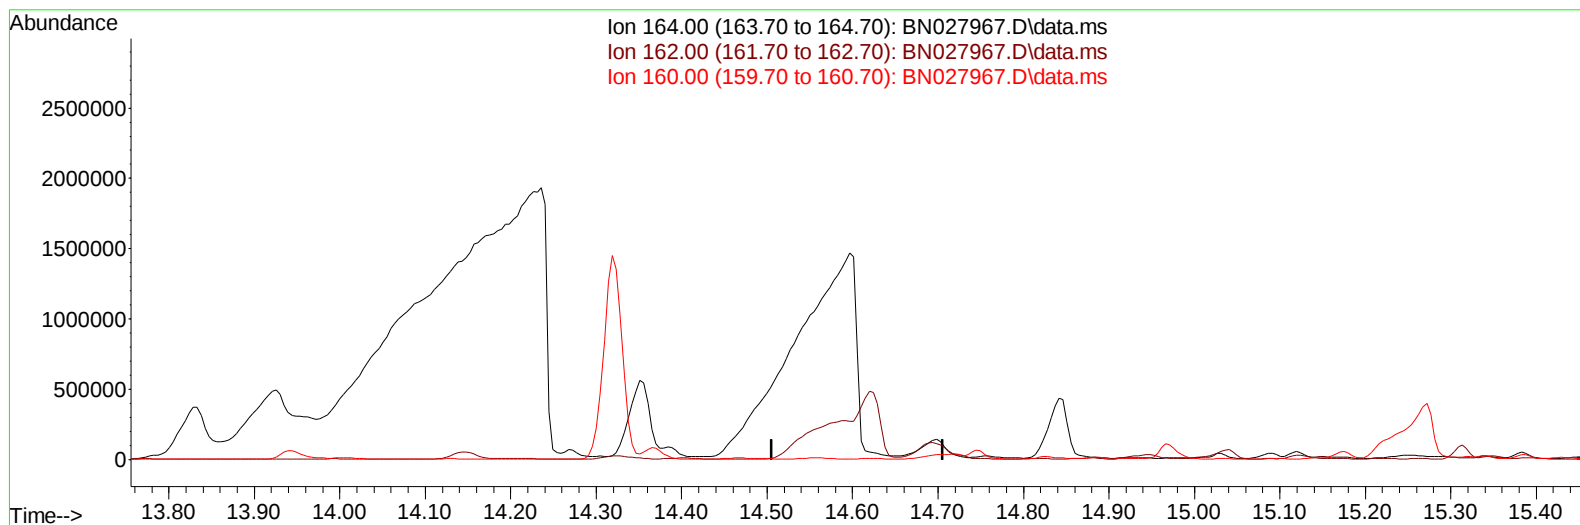

TIC: BN027967.D\data.ms

(9) Acenaphthene-d10 (I)

14.606min (-14.606) 0.00 ng/u1

response 0

Ion	Exp%	Act%
164.00	100.00	0.00
162.00	103.00	0.00#
160.00	50.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027967.D
 Acq On : 29 Sep 2023 18:47
 Operator : MA/JU
 Sample : 04497-12
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ14

Manual IntegrationsAPPROVED

Quant Time: Sep 30 01:25:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

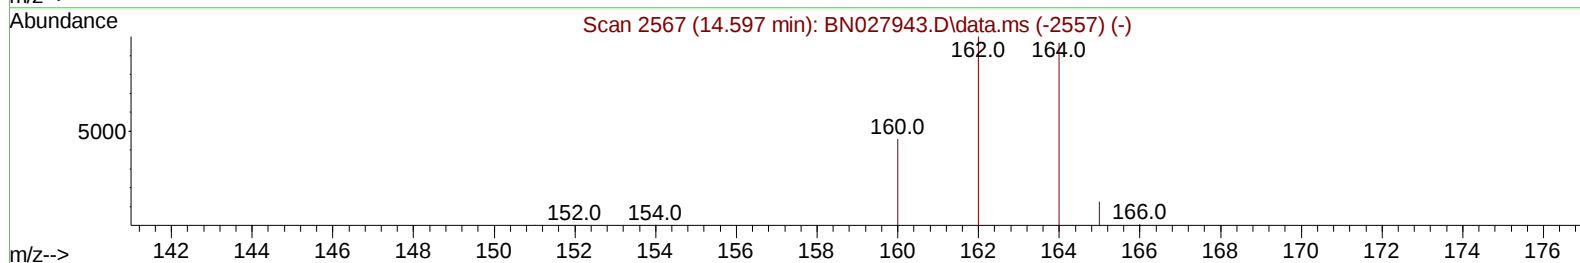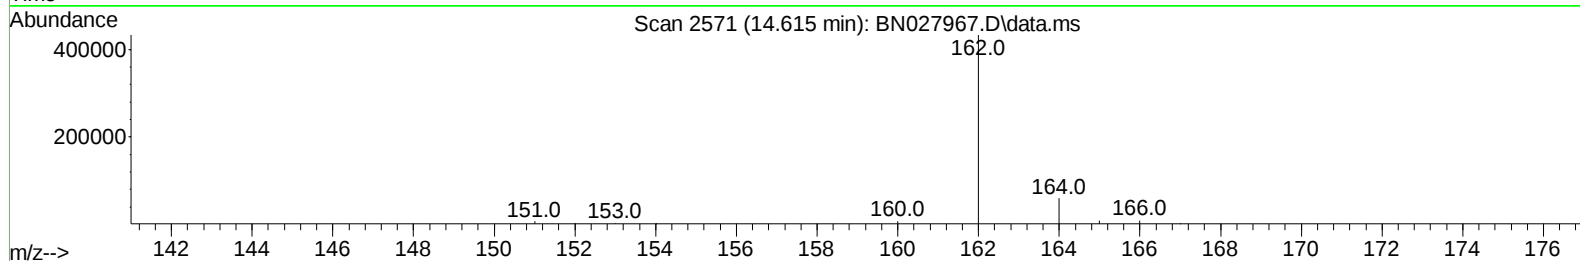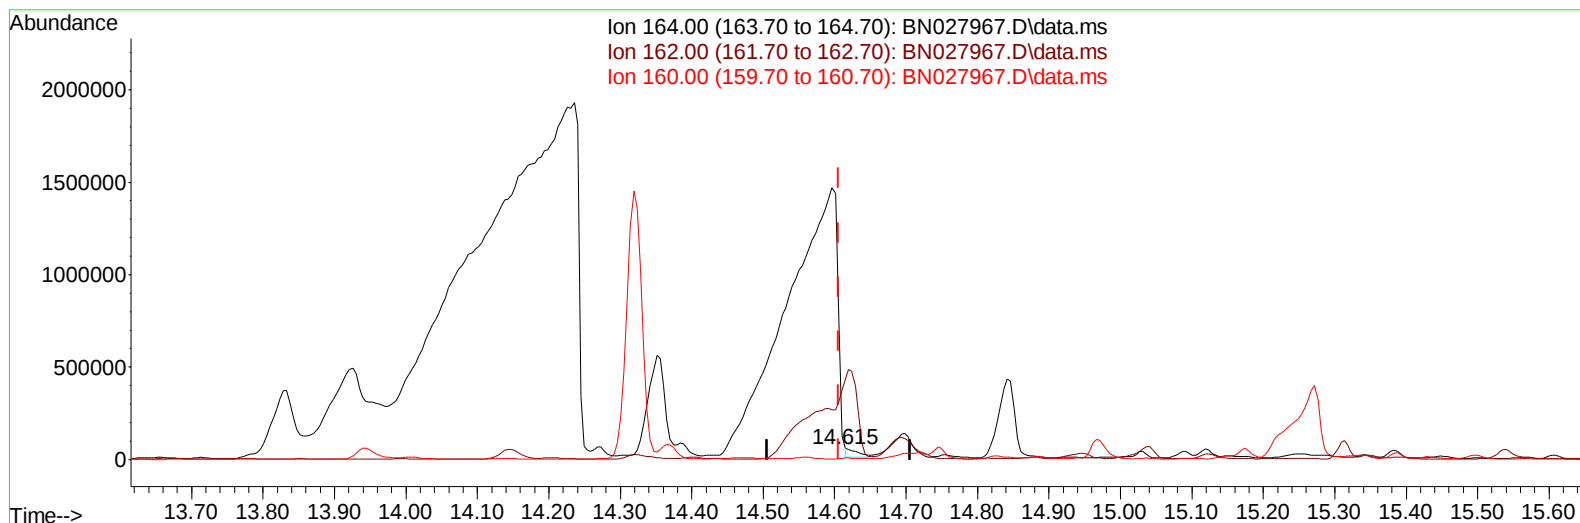

TIC: BN027967.D\data.ms

(9) Acenaphthene-d10 (I)

14.615min (+ 0.009) 0.40 ng/ul m

response 48689

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.00	722.41#
160.00	50.90	12.58#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027967.D
 Acq On : 29 Sep 2023 18:47
 Operator : MA/JU
 Sample : 04497-12
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ14

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

Quant Time: Sep 30 01:25:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.962	152		9284	0.400	ng/ul	0.00
4) Naphthalene-d8	10.790	136		34315	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.615	164		48689m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.371	188		42044	0.400	ng/ul	# 0.02
17) Chrysene-d12	21.548	240		26753	0.400	ng/ul	0.01
23) Perylene-d12	24.027	264		26720	0.400	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.330	96		21017	1.797	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152		29359	0.565	ng/ul	0.00
18) Fluoranthene-d10	19.390	212		25933	0.317	ng/ul	0.00
Target Compounds							Qvalue
10) Acenaphthylene	14.374	152		3204072	15.065	ng/ul#	72
19) Fluoranthene	19.422	202		3337	0.031	ng/ul#	50
20) Pyrene	19.785	202		3142	0.028	ng/ul#	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027967.D
Acq On : 29 Sep 2023 18:47
Operator : MA/JU
Sample : 04497-12
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ14

Manual IntegrationsAPPROVED

Quant Time: Sep 30 01:25:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023

