




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027974.D
 Acq On : 29 Sep 2023 23:38
 Operator : MA/JU
 Sample : 04497-16
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ22

Manual IntegrationsAPPROVED

Quant Time: Sep 30 01:06:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

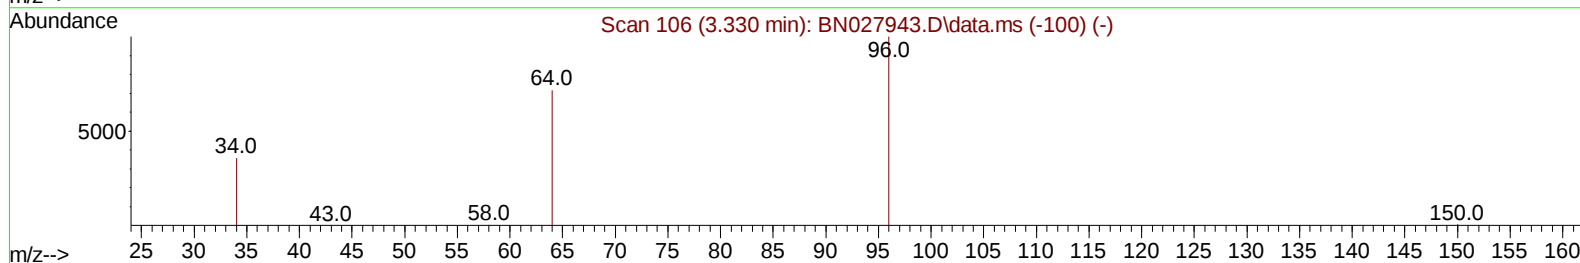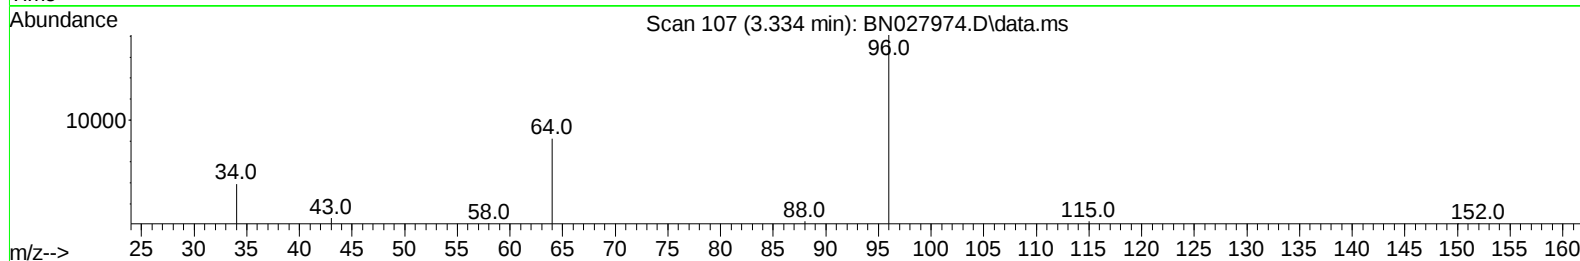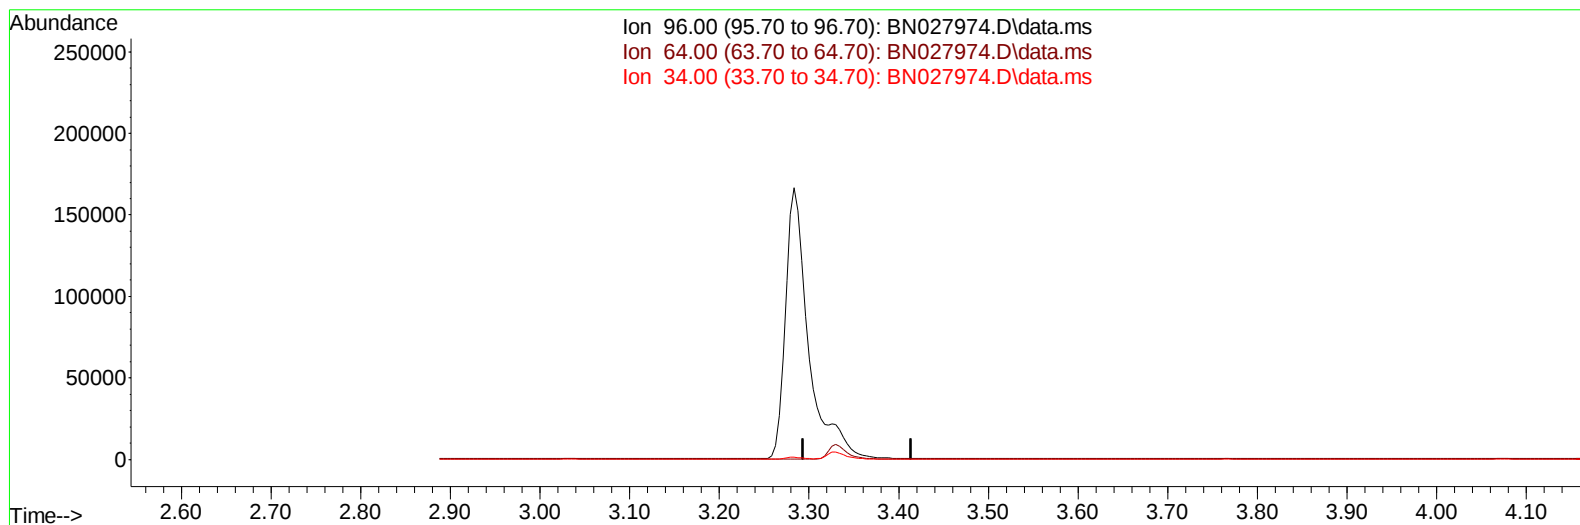

TIC: BN027974.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.334min (-3.334) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	66.40	0.00#
34.00	43.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027974.D
Acq On : 29 Sep 2023 23:38
Operator : MA/JU
Sample : 04497-16
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ22

Manual IntegrationsAPPROVED

Quant Time: Sep 30 01:06:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023

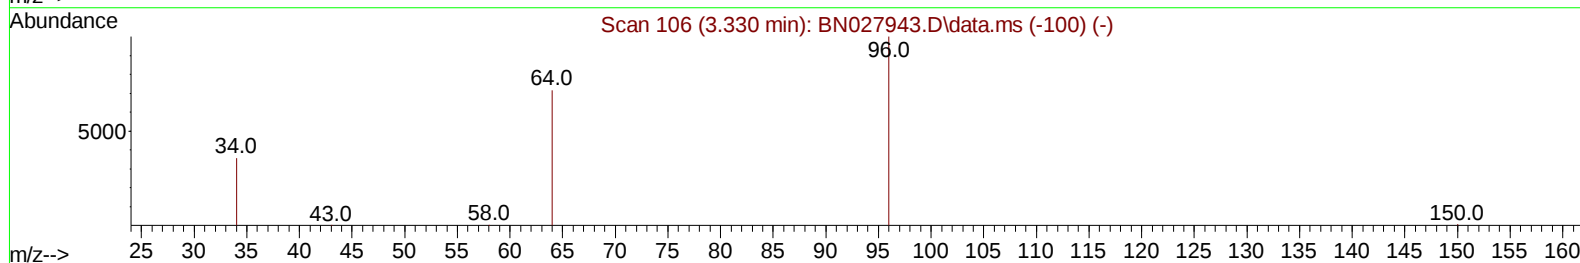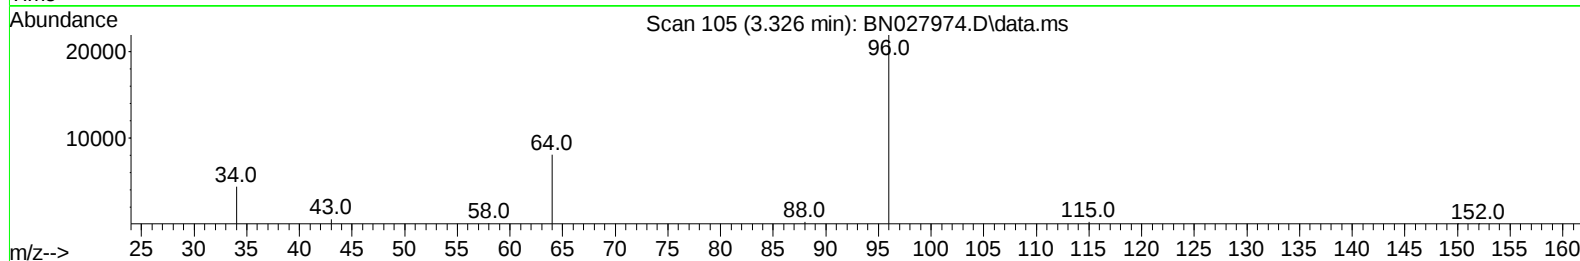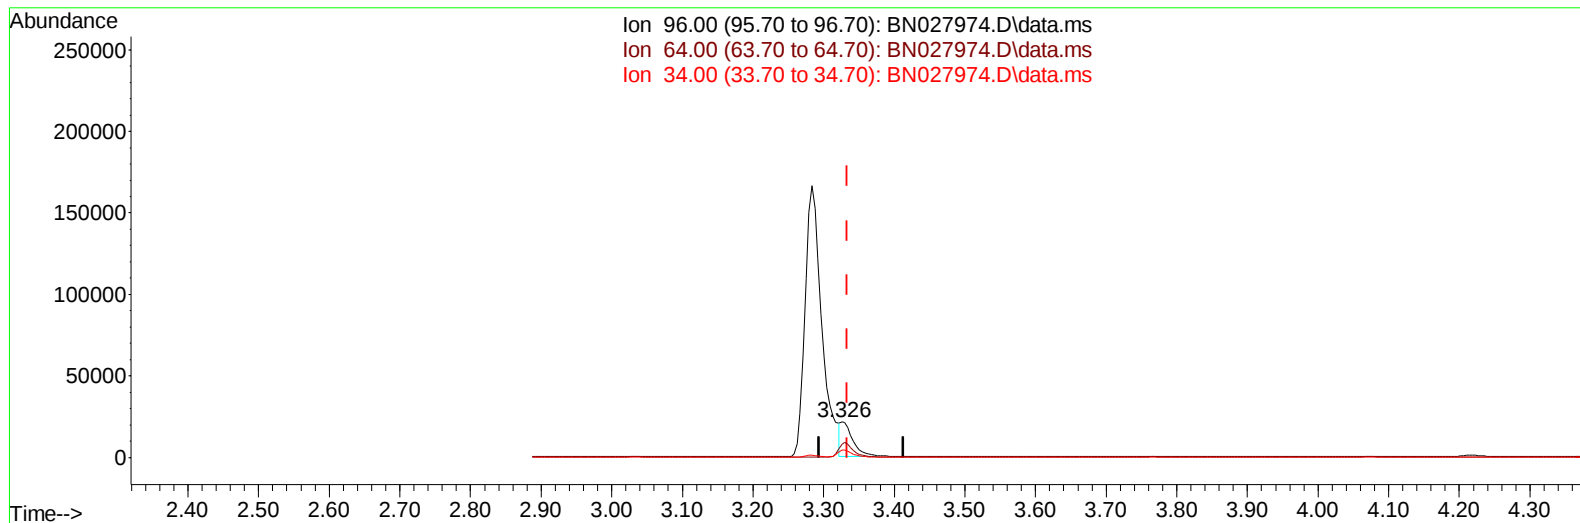

TIC: BN027974.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.326min (-0.008) 3.19 ng/ul m

response 25836

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.40	37.03#
34.00	43.80	20.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027974.D
 Acq On : 29 Sep 2023 23:38
 Operator : MA/JU
 Sample : 04497-16
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ22

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

Quant Time: Sep 30 01:06:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.958	152		6422	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136		24164	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164		14430	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188		31258	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240		22415	0.400	ng/ul	0.00
23) Perylene-d12	24.018	264		22027	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.326	96		25836m	3.194	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152		10945	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.380	212		23575	0.344	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.368	88		1066	0.127	ng/ul#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027974.D
Acq On : 29 Sep 2023 23:38
Operator : MA/JU
Sample : 04497-16
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ22

Manual IntegrationsAPPROVED

Quant Time: Sep 30 01:06:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023

