




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027978.D
Acq On : 30 Sep 2023 02:05
Operator : MA/JU
Sample : 04497-20
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBBP3

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:50:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023

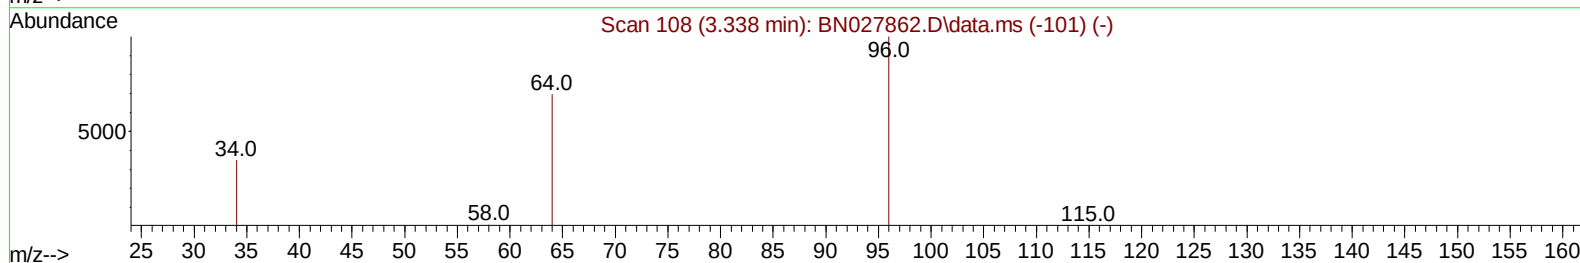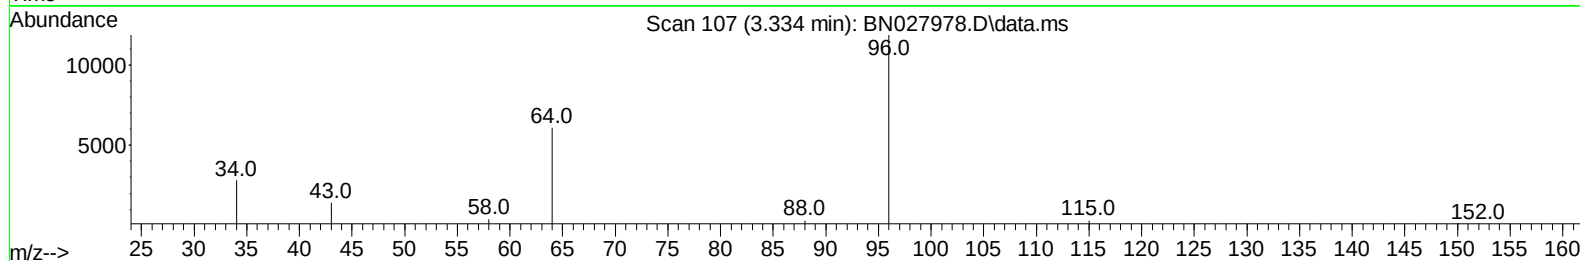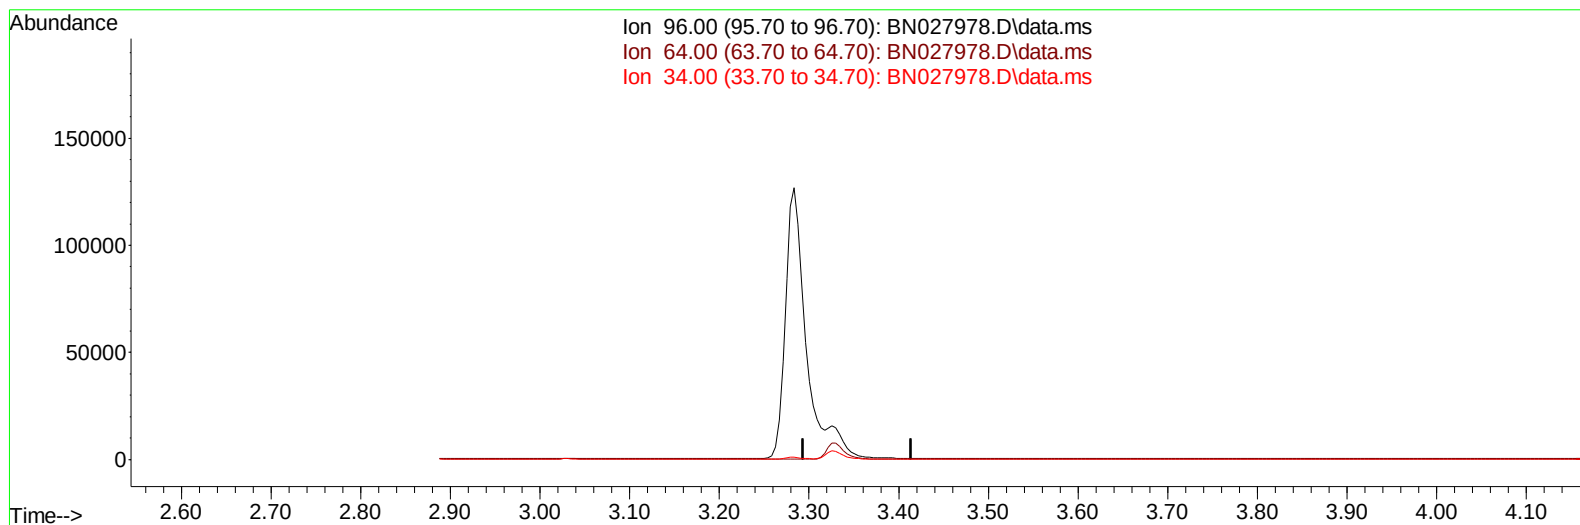

TIC: BN027978.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.334min (-3.334) 0.00 ng/ul

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	66.40	0.00#
34.00	43.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027978.D
 Acq On : 30 Sep 2023 02:05
 Operator : MA/JU
 Sample : 04497-20
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBP3

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:50:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

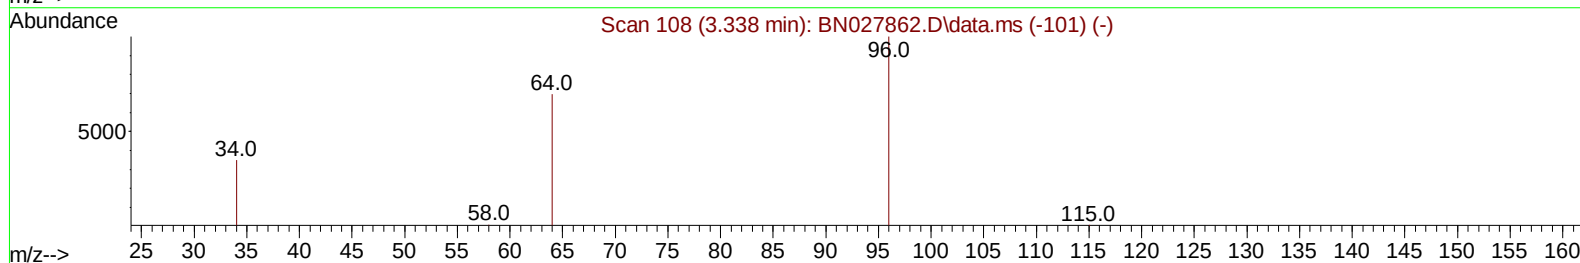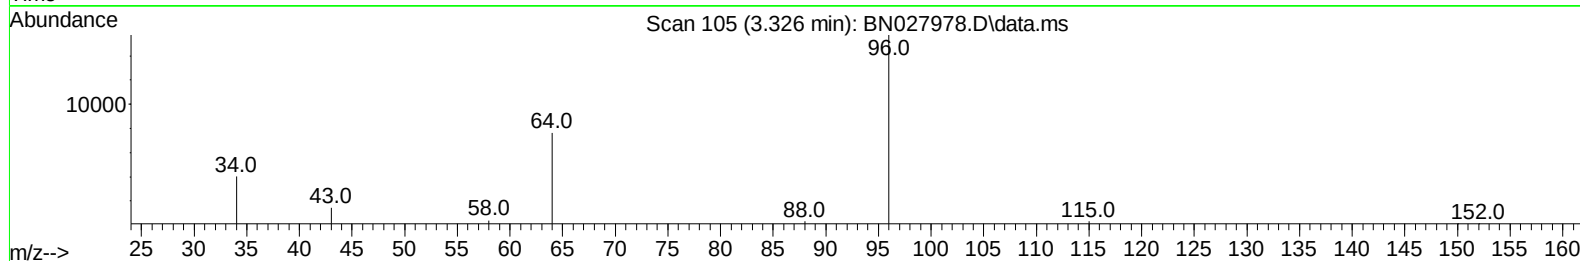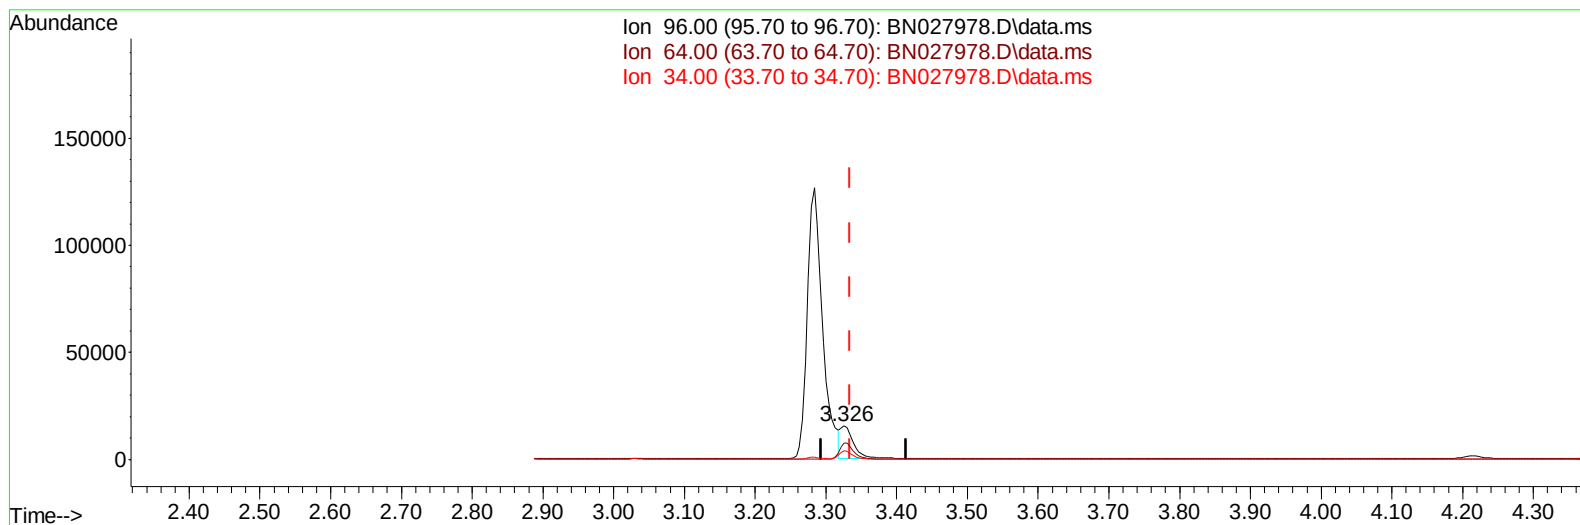

TIC: BN027978.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.326min (-0.008) 1.99 ng/ul m

response 19445

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.40	48.39#
34.00	43.80	25.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027978.D
 Acq On : 30 Sep 2023 02:05
 Operator : MA/JU
 Sample : 04497-20
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBP3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

Quant Time: Sep 30 02:50:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	7764	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	26615	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	16428	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	34919	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	23110	0.400	ng/ul	0.00
23) Perylene-d12	24.015	264	22663	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	19445m	1.988	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	11783	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	27519	0.390	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.364	88	56217	5.523	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027978.D
Acq On : 30 Sep 2023 02:05
Operator : MA/JU
Sample : 04497-20
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBBP3

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:50:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023

