

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027928.D
 Acq On : 28 Sep 2023 16:28
 Operator : MA/JU
 Sample : 04480-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ47

Quant Time: Sep 28 17:20:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	2637	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	10195	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	6852	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	14774	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	13298	0.400	ng/ul	# 0.00
23) Perylene-d12	24.015	264	12701	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	24753	7.452	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	11076	0.717	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	28058	0.691	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	1465	0.424	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027928.D
Acq On : 28 Sep 2023 16:28
Operator : MA/JU
Sample : 04480-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ47

Quant Time: Sep 28 17:20:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

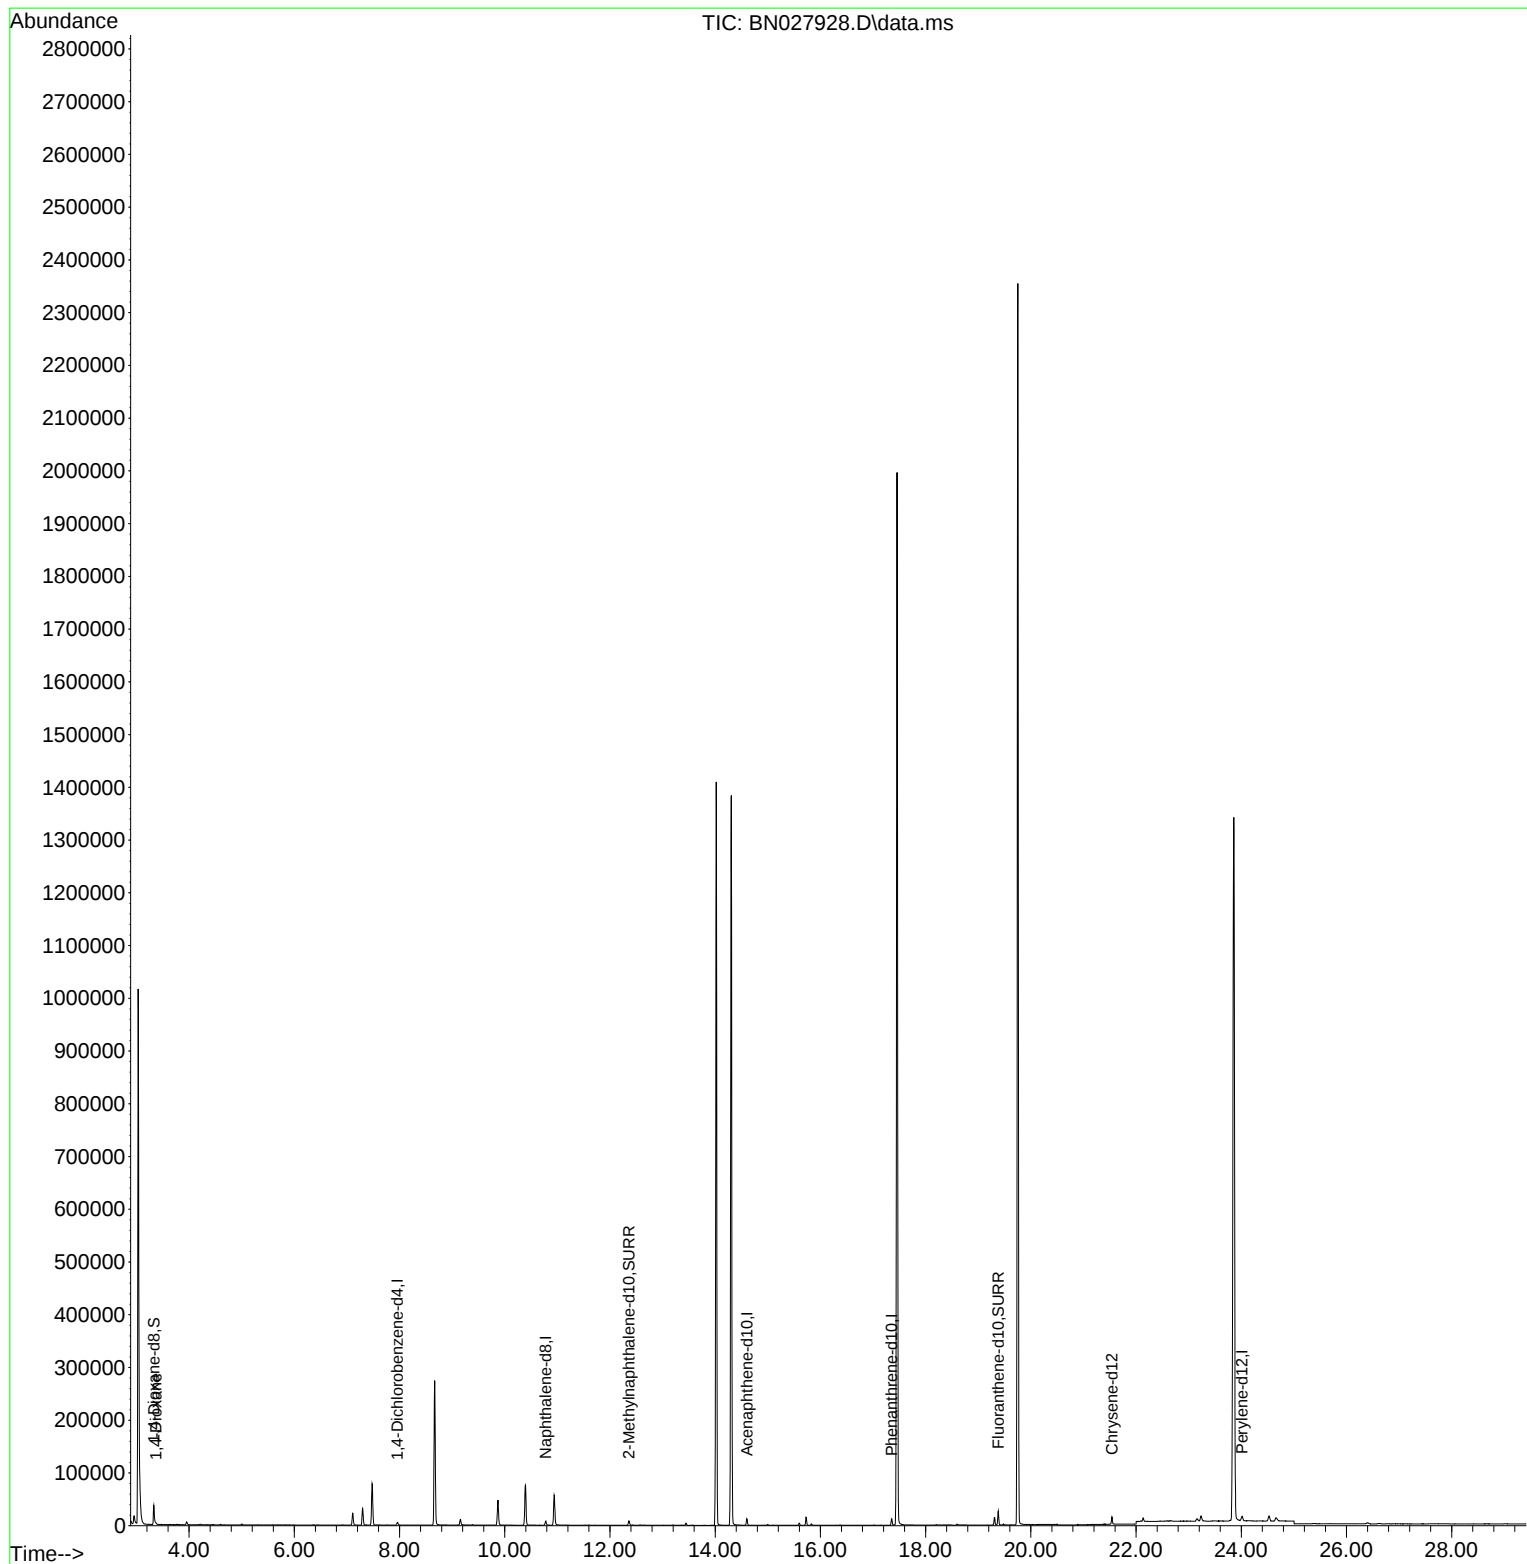

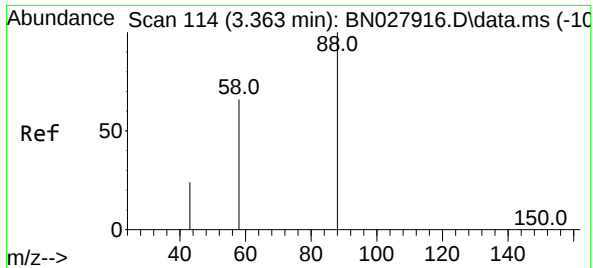

#2
 1,4-Dioxane
 Concen: 0.424 ng/ul
 RT: 3.368 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN027928.D
 Acq: 28 Sep 2023 16:28

Instrument :
 BNA_N
 ClientSampleId :
 BBJ47

Tgt Ion:	88	Resp:	1465
Ion	Ratio	Lower	Upper
88	100		
43	60.0	39.6	59.4#
58	48.9	48.3	72.5

