

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027959.D
 Acq On : 29 Sep 2023 13:56
 Operator : MA/JU
 Sample : 04472-22
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYP5

Quant Time: Sep 29 16:07:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	6418	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	25060	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	14722	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.363	188	32238	0.400	ng/ul	0.00
17) Chrysene-d12	21.551	240	23181	0.400	ng/ul	0.01
23) Perylene-d12	24.036	264	22113	0.400	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	19577	2.422	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	12717	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.390	212	26412	0.373	ng/ul	0.00
Target Compounds						
8) 1-Methylnaphthalene	12.660	142	1073	0.023	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027959.D
Acq On : 29 Sep 2023 13:56
Operator : MA/JU
Sample : 04472-22
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZYP5

Quant Time: Sep 29 16:07:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

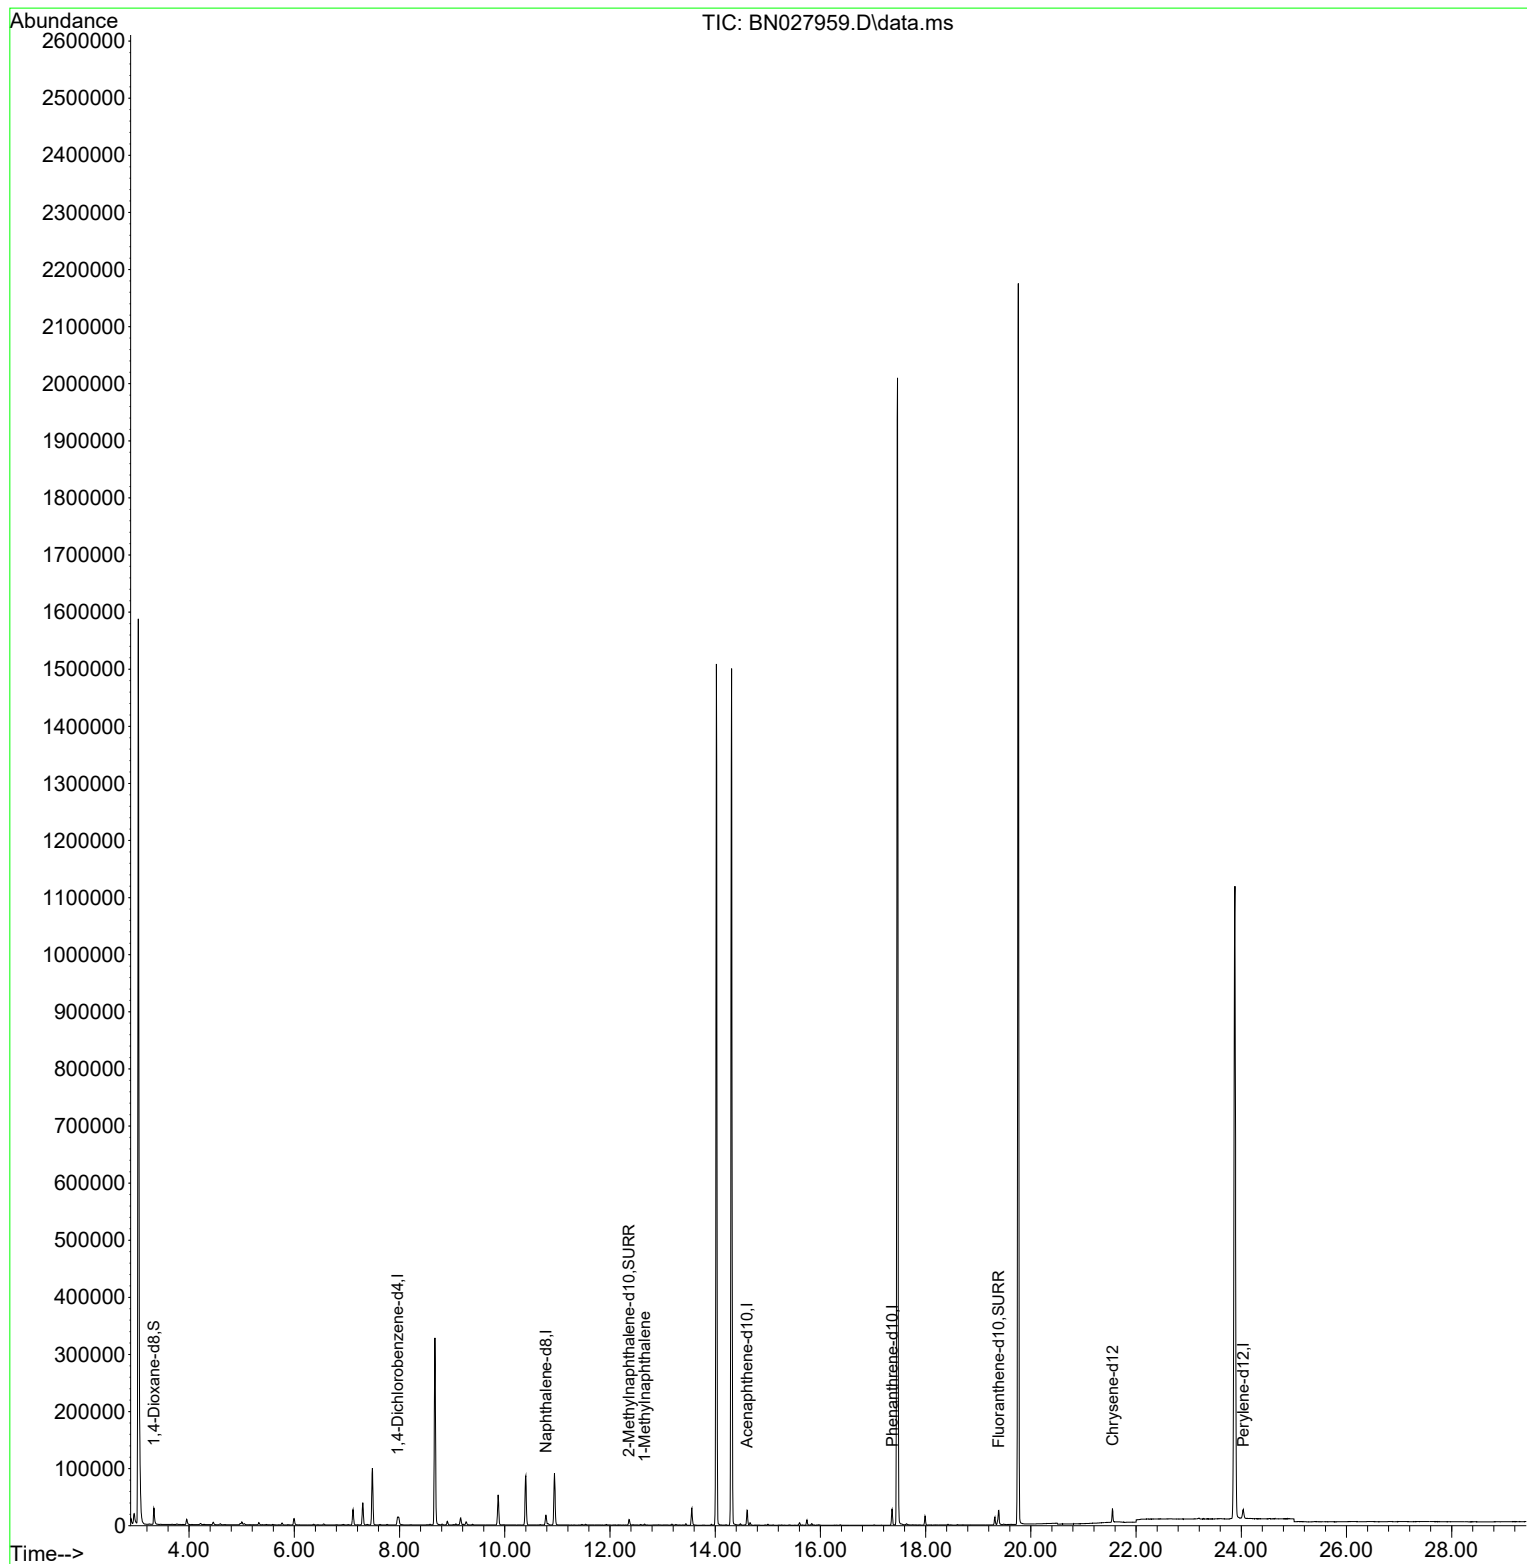

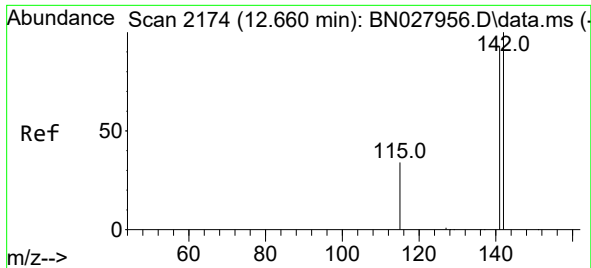

#8
 1-Methylnaphthalene
 Concen: 0.023 ng/ul
 RT: 12.660 min Scan# 2174
 Delta R.T. 0.006 min
 Lab File: BN027959.D
 Acq: 29 Sep 2023 13:56

Instrument :
 BNA_N
 ClientSampleId :
 EZYP5

Tgt Ion:142 Resp: 1073
 Ion Ratio Lower Upper
 142 100
 141 92.8 72.8 109.2

