

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027960.D
 Acq On : 29 Sep 2023 14:33
 Operator : MA/JU
 Sample : 04497-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ38

Quant Time: Sep 29 16:07:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	7308	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	26602	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	15742	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.362	188	32831	0.400	ng/ul	0.00
17) Chrysene-d12	21.551	240	22630	0.400	ng/ul	0.01
23) Perylene-d12	24.032	264	22149	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	14456	1.570	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	9059	0.225	ng/ul	0.00
18) Fluoranthene-d10	19.390	212	19017	0.275	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	1762	0.184	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027960.D
Acq On : 29 Sep 2023 14:33
Operator : MA/JU
Sample : 04497-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ38

Quant Time: Sep 29 16:07:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

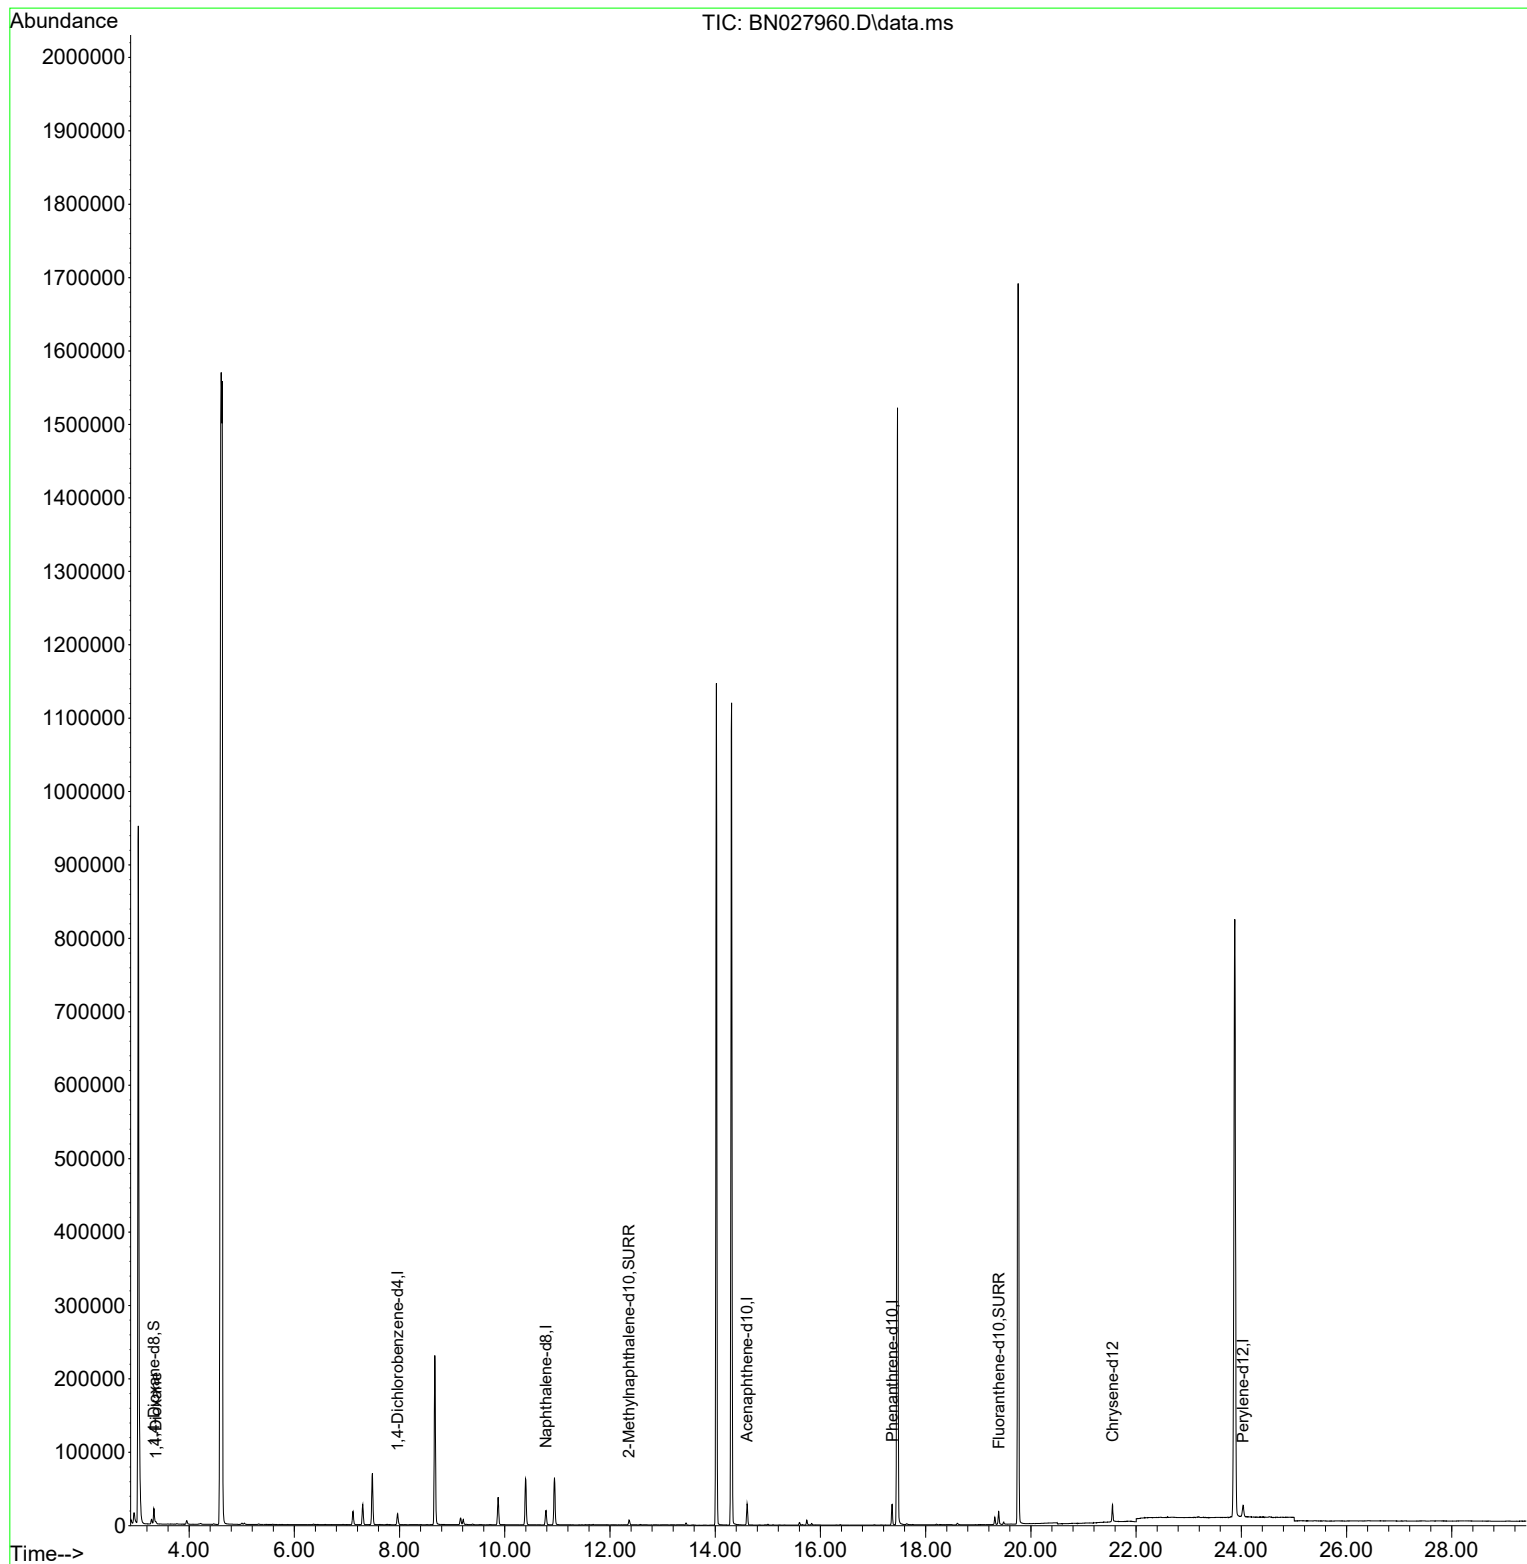

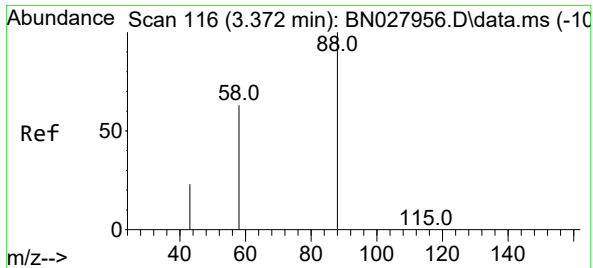

#2
1,4-Dioxane
Concen: 0.184 ng/ul
RT: 3.368 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN027960.D
Acq: 29 Sep 2023 14:33

Instrument :
BNA_N
ClientSampleId :
BBJ38

Tgt Ion: 88 Resp: 1762
Ion Ratio Lower Upper
88 100
43 67.6 39.6 59.4#
58 63.0 48.3 72.5

