

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027962.D
 Acq On : 29 Sep 2023 15:45
 Operator : MA/JU
 Sample : 04497-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJC4

Quant Time: Sep 29 18:22:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	7175	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	26027	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	15480	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	32412	0.400	ng/ul	0.00
17) Chrysene-d12	21.548	240	22251	0.400	ng/ul	0.01
23) Perylene-d12	24.026	264	22242	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	16767	1.855	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	10639	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	23345	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.372	88	768	0.082	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027962.D
Acq On : 29 Sep 2023 15:45
Operator : MA/JU
Sample : 04497-07
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJC4

Quant Time: Sep 29 18:22:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

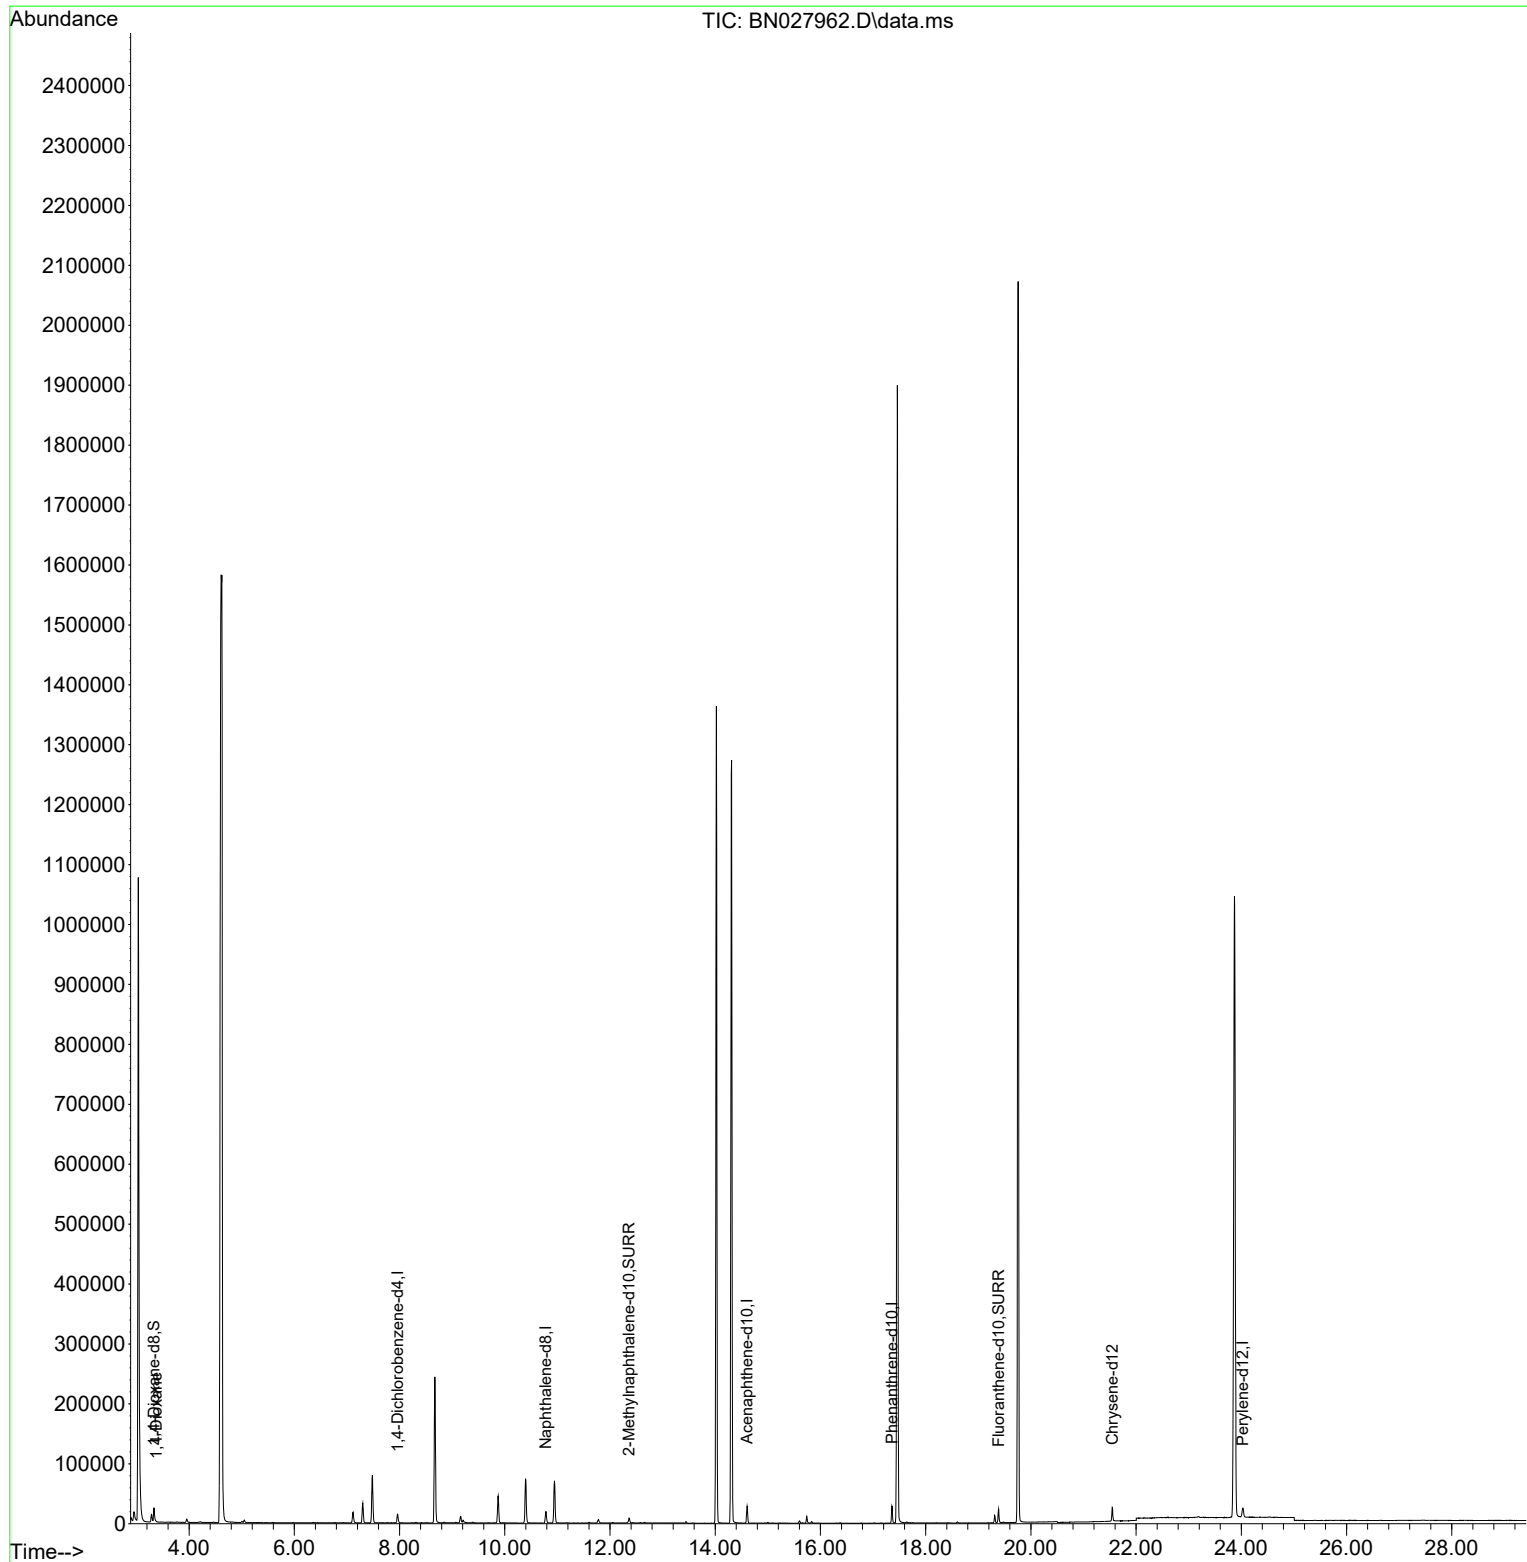

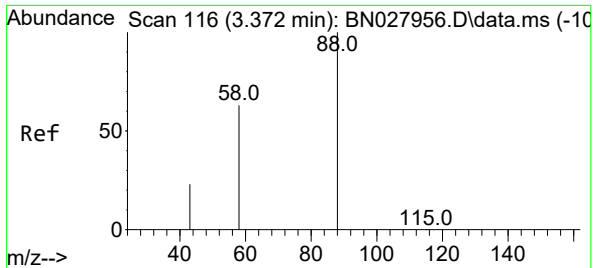

#2
1,4-Dioxane
Concen: 0.082 ng/ul
RT: 3.372 min Scan# 116
Delta R.T. 0.004 min
Lab File: BN027962.D
Acq: 29 Sep 2023 15:45

Instrument :
BNA_N
ClientSampleId :
BBJC4

Tgt Ion:	88	Resp:	768
Ion	Ratio	Lower	Upper
88	100		
43	74.0	39.6	59.4#
58	34.9	48.3	72.5#

