

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027965.D
 Acq On : 29 Sep 2023 17:34
 Operator : MA/JU
 Sample : 04497-10
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHQ2

Quant Time: Sep 29 18:22:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	7688	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	27972	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	16683	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	34307	0.400	ng/ul	0.00
17) Chrysene-d12	21.548	240	22345	0.400	ng/ul	0.01
23) Perylene-d12	24.027	264	23497	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	15565	1.607	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	11194	0.264	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	22194	0.325	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	6917	0.686	ng/ul#	90
19) Fluoranthene	19.418	202	2160	0.024	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027965.D
Acq On : 29 Sep 2023 17:34
Operator : MA/JU
Sample : 04497-10
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHQ2

Quant Time: Sep 29 18:22:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration




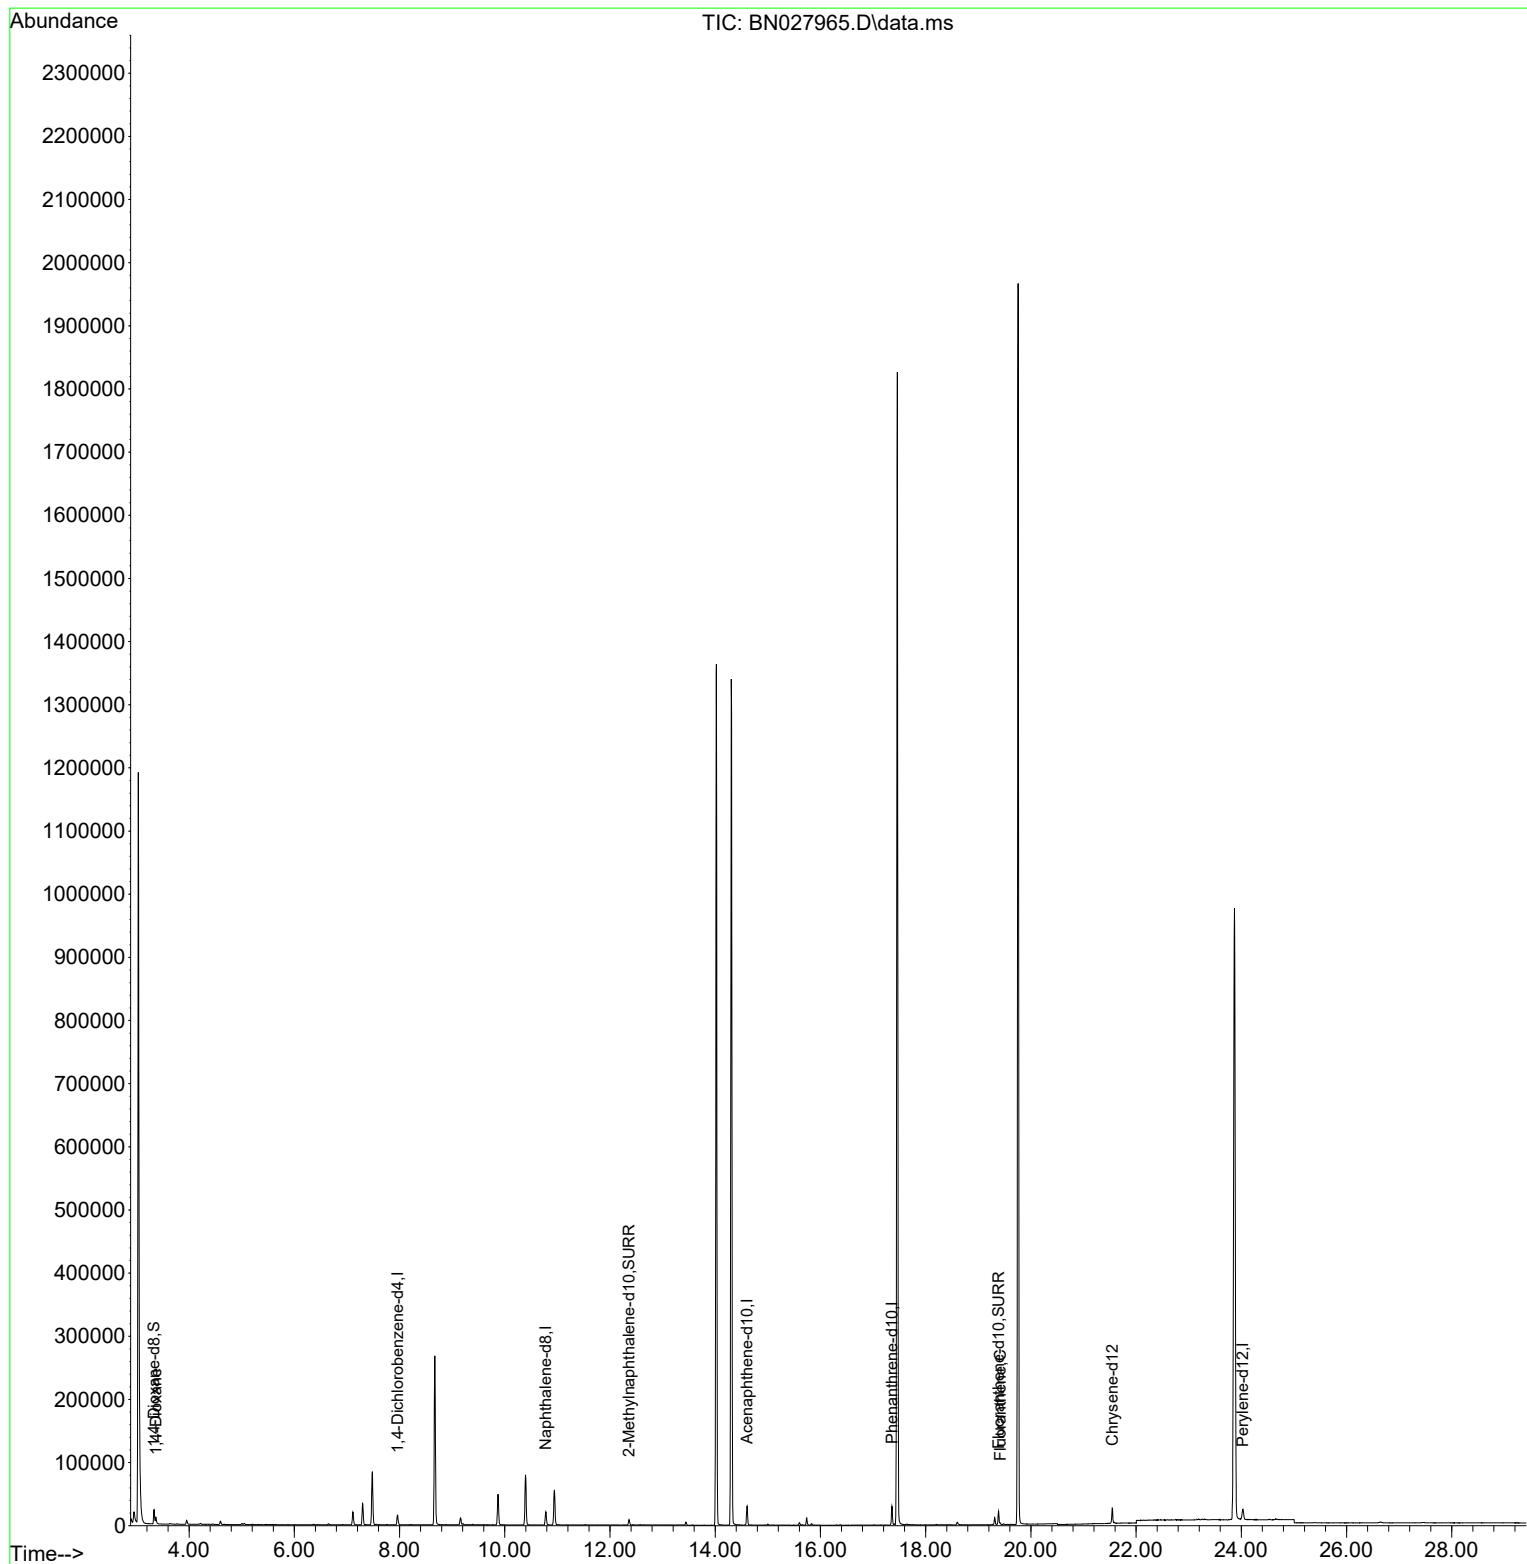


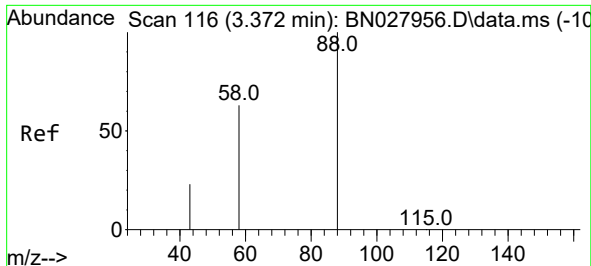

#2
1,4-Dioxane
Concen: 0.686 ng/ul
RT: 3.368 min Scan# 116
Delta R.T. 0.000 min
Lab File: BN027965.D
Acq: 29 Sep 2023 17:34

Instrument :
BNA_N
ClientSampleId :
BBHQ2

Tgt Ion: 88 Resp: 6917
Ion Ratio Lower Upper
88 100
43 35.4 39.6 59.4#
58 61.3 48.3 72.5

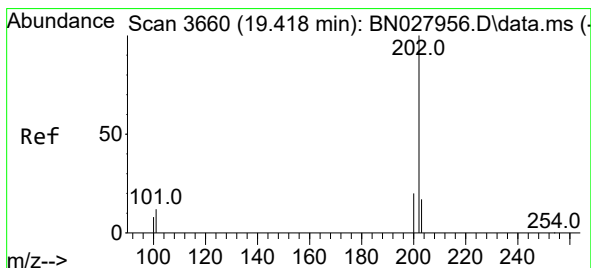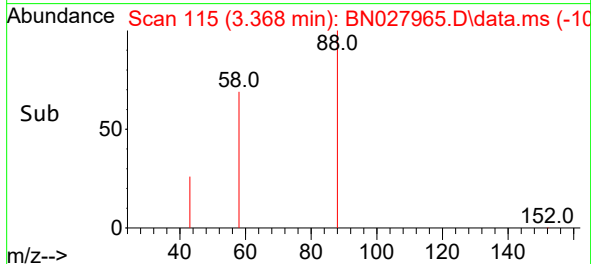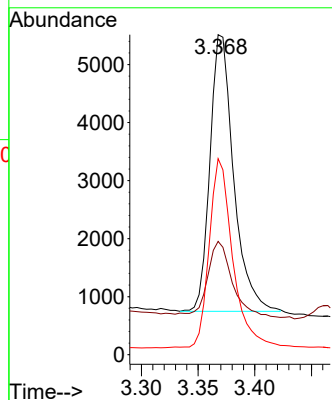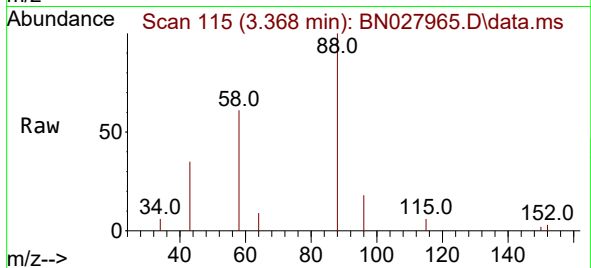

#19
Fluoranthene
Concen: 0.024 ng/ul
RT: 19.418 min Scan# 3660
Delta R.T. 0.009 min
Lab File: BN027965.D
Acq: 29 Sep 2023 17:34

Tgt Ion: 202 Resp: 2160
Ion Ratio Lower Upper
202 100
101 17.7 9.3 13.9#
100 12.0 7.0 10.4#

