

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
 Data File : BN027978.D
 Acq On : 30 Sep 2023 02:05
 Operator : MA/JU
 Sample : 04497-20
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBP3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

Quant Time: Sep 30 02:50:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	7764	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	26615	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	16428	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	34919	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	23110	0.400	ng/ul	0.00
23) Perylene-d12	24.015	264	22663	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	19445m	1.988	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	11783	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	27519	0.390	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.364	88	56217	5.523	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092823\
Data File : BN027978.D
Acq On : 30 Sep 2023 02:05
Operator : MA/JU
Sample : 04497-20
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BBBP3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/30/2023
Supervised By :mohammad ahmed 09/30/2023


Quant Time: Sep 30 02:50:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

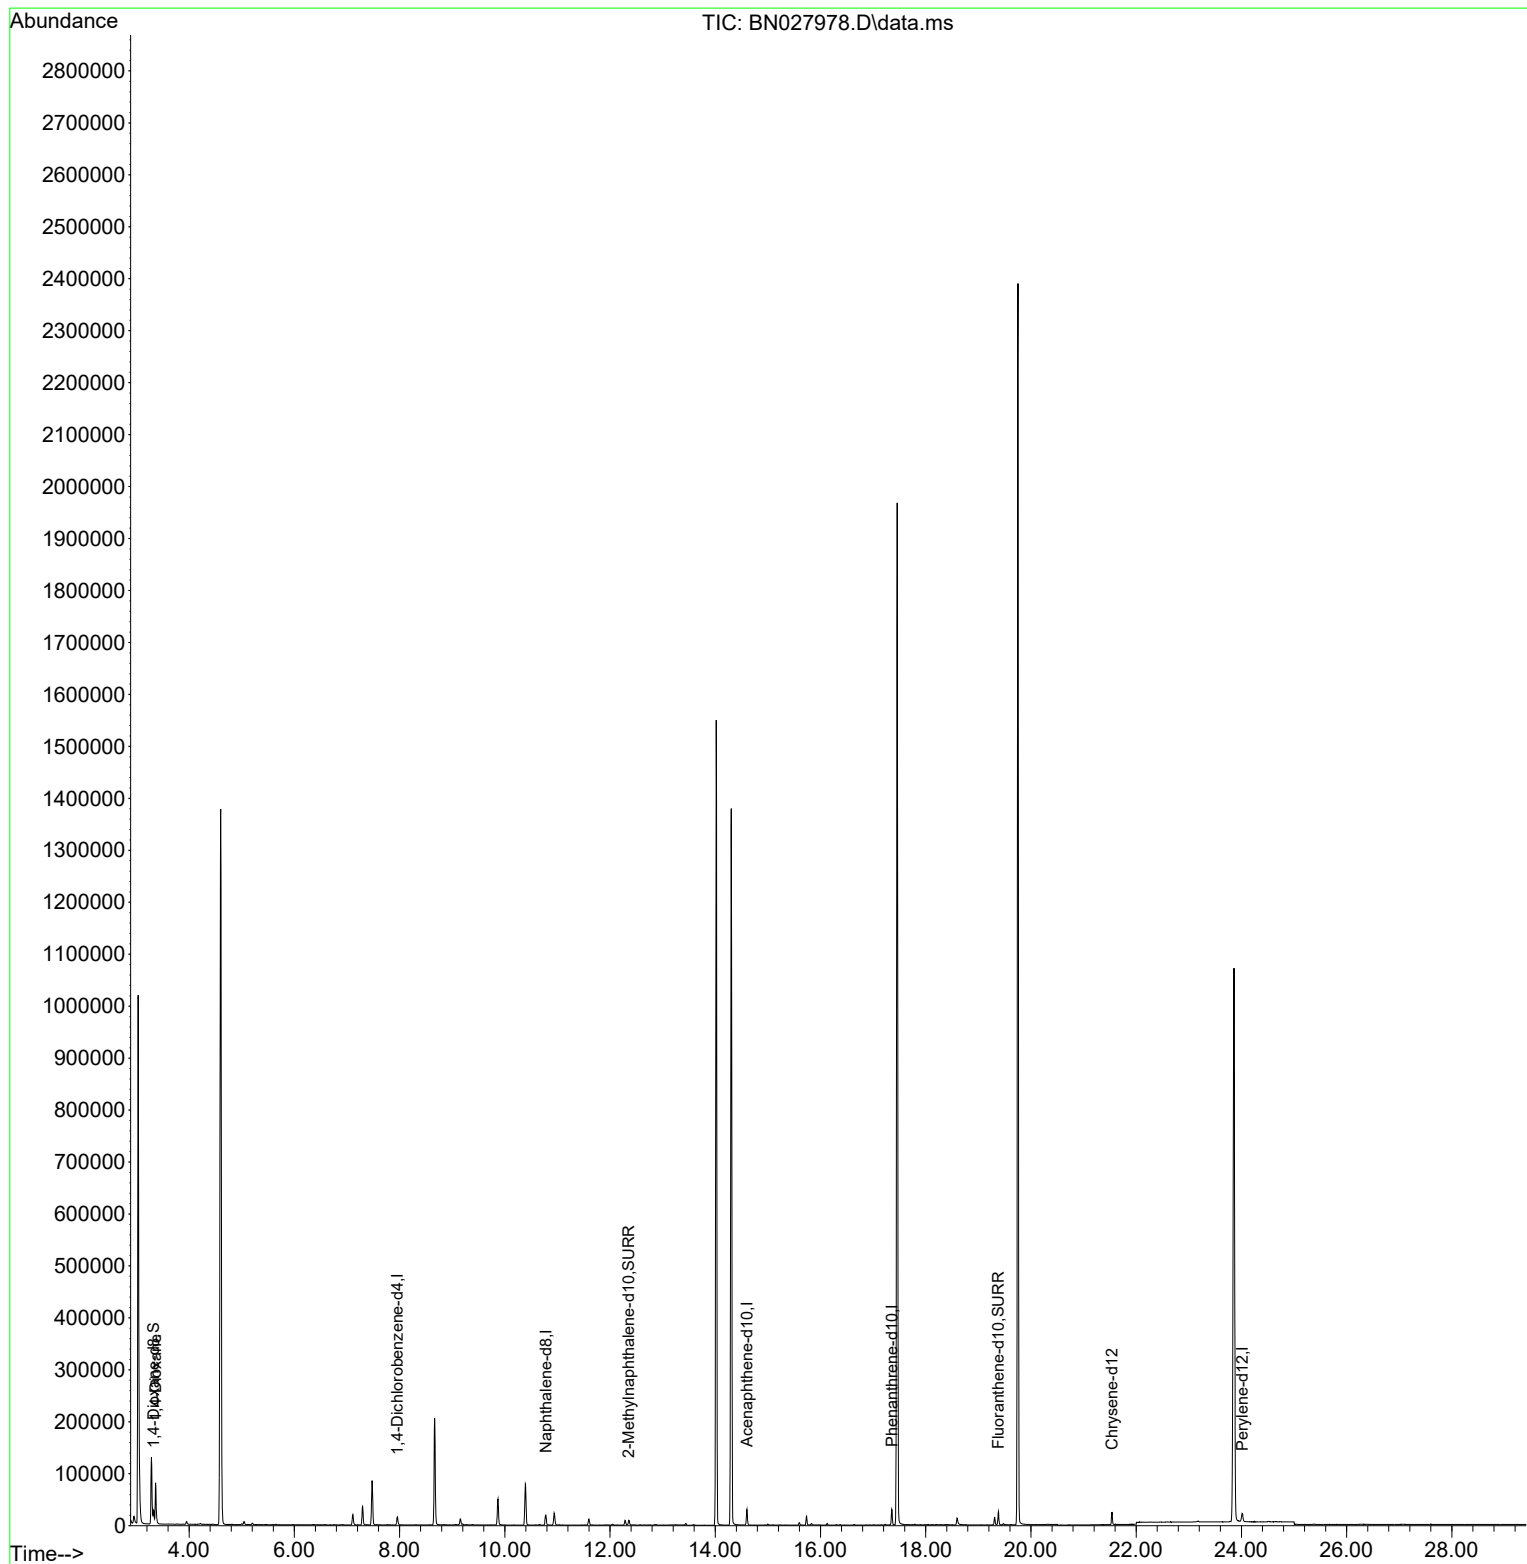

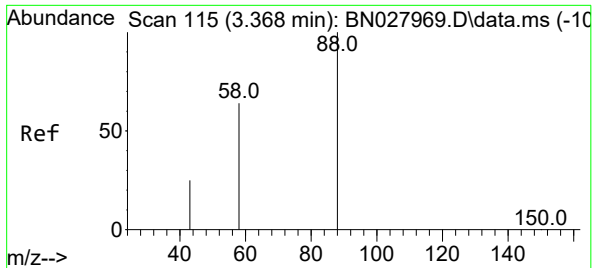

#2
 1,4-Dioxane
 Concen: 5.523 ng/ul
 RT: 3.364 min Scan# 11
 Delta R.T. -0.004 min
 Lab File: BN027978.D
 Acq: 30 Sep 2023 02:05

Instrument :
 BNA_N
 ClientSampleId :
 BBBP3

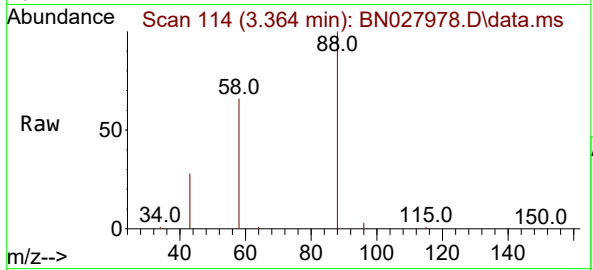

Tgt Ion: 88 Resp: 5621

Ion	Ratio	Lower	Upper
88	100		
43	28.3	39.6	59.4
58	66.1	48.3	72.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/30/2023
 Supervised By :mohammad ahmed 09/30/2023

