

Data File : BN007894.D
Acq On : 30 Sep 2019 13:30
Operator : JU
Sample : PB123466BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB123466BL

Quant Time: Oct 01 06:47:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	8402	0.40	ng	0.00
7) Naphthalene-d8	10.46	136	31323	0.40	ng	-0.01
13) Acenaphthene-d10	14.32	164	17562	0.40	ng	0.00
19) Phenanthrene-d10	17.07	188	35254	0.40	ng	0.00
27) Chrysene-d12	21.25	240	28294	0.40	ng	-0.02
34) Perylene-d12	23.47	264	34234	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.31	112	7071	0.24	ng	0.00
5) Phenol-d6	6.87	99	8958	0.25	ng	0.00
8) Nitrobenzene-d5	8.83	82	7354	0.27	ng	0.00
11) 2-Methylnaphthalene-d10	12.05	152	15358	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.81	330	1290	0.13	ng	0.00
15) 2-Fluorobiphenyl	12.94	172	20182	0.28	ng	0.00
25) Fluoranthene-d10	19.10	212	29834	0.25	ng	-0.01
29) Terphenyl-d14	19.70	244	23659	0.34	ng	-0.01
Target Compounds						
3) n-Nitrosodimethylamine	3.01	42	2262	0.527	ng	Qvalue # 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN007894.D

Acq On : 30 Sep 2019 13:30

Operator : JU

Sample : PB123466BS

Misc :

ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB123466BL


Quant Time: Oct 01 06:47:17 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Sep 18 18:24:40 2019

Response via : Initial Calibration

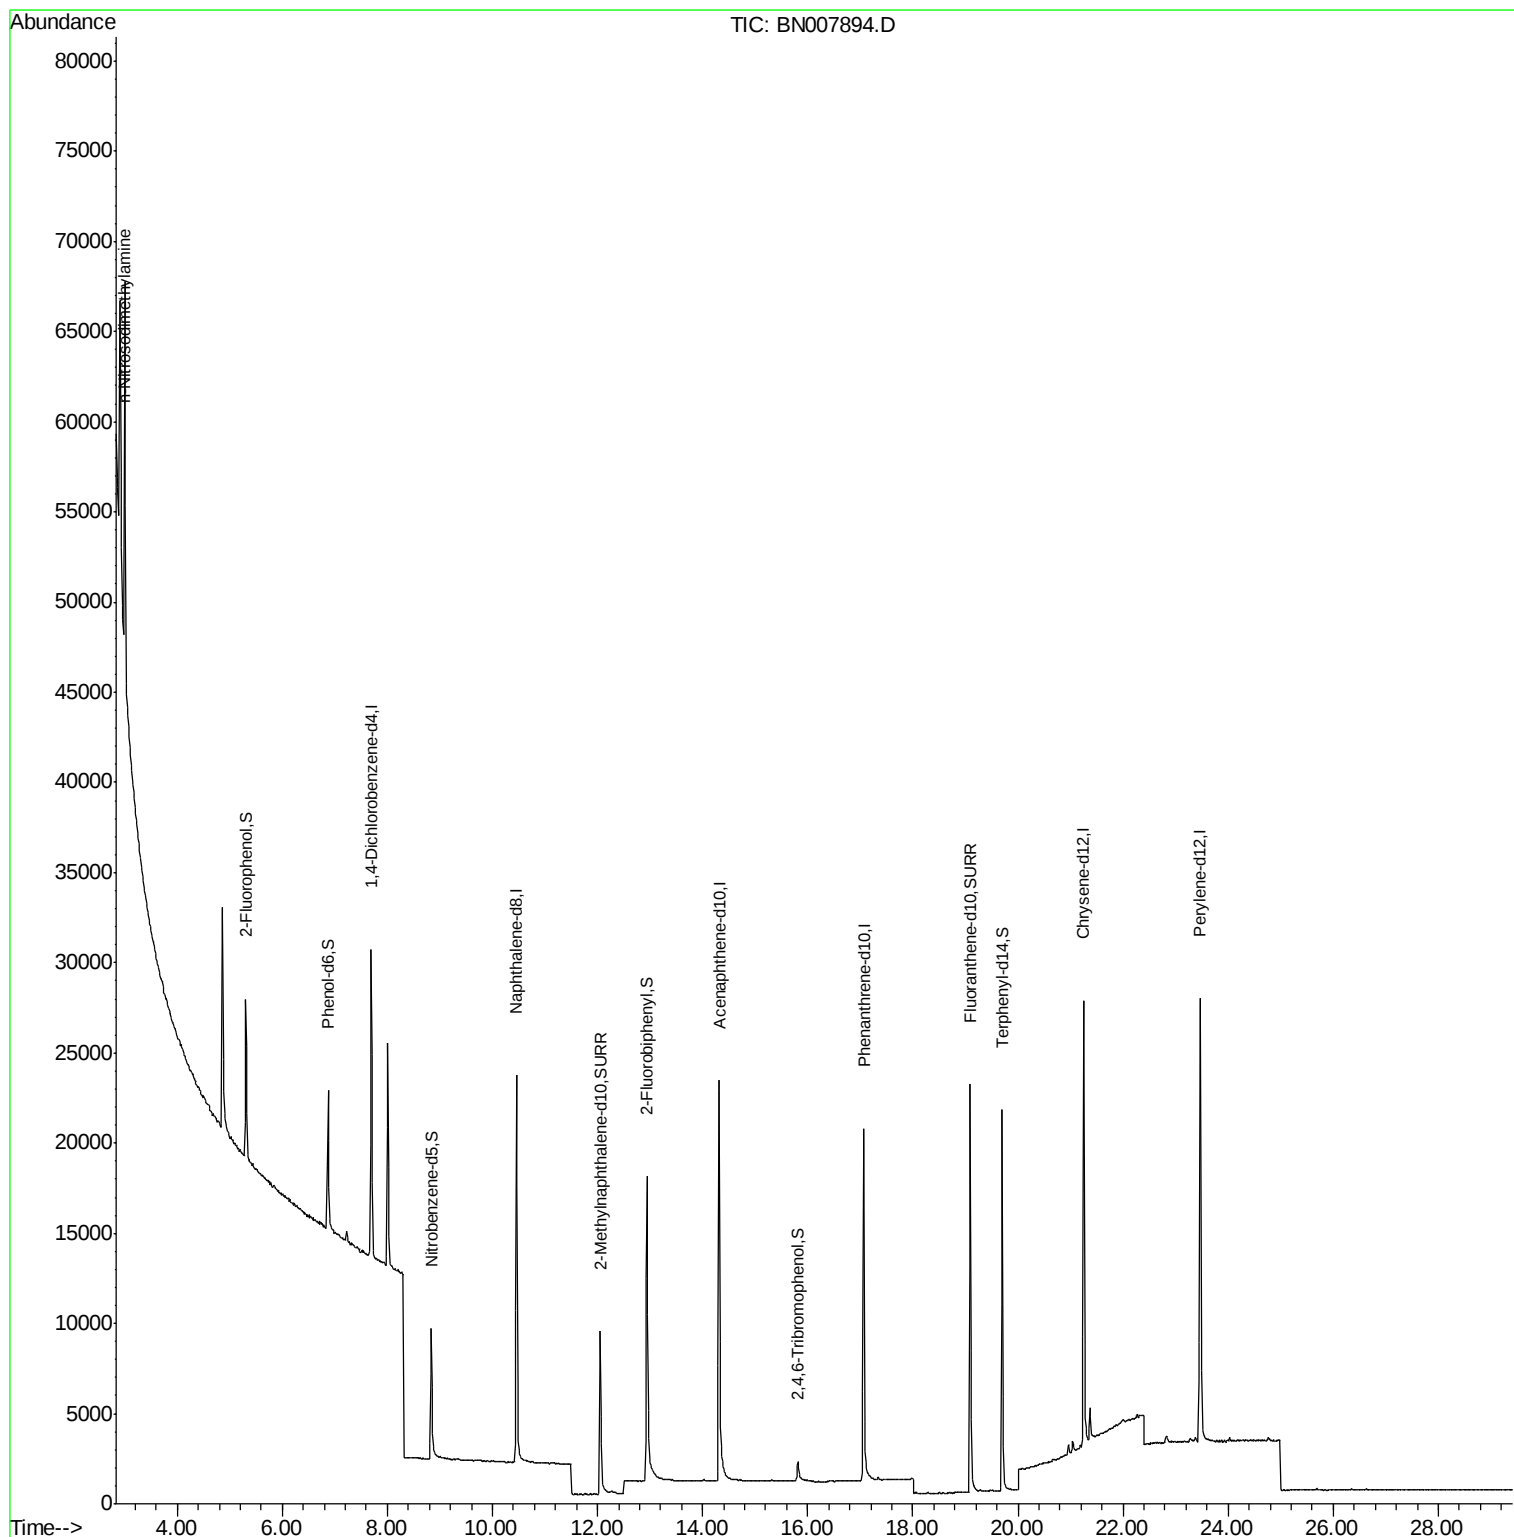



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.69 min Scan# 604

Delta R.T. -0.01 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30

Instrument :

BNA_N

ClientSampleId :

PB123466BL


Tgt Ion:152 Resp: 8402

Ion Ratio Lower Upper

152 100

150 153.2 125.6 188.4




115 62.2 53.3 79.9

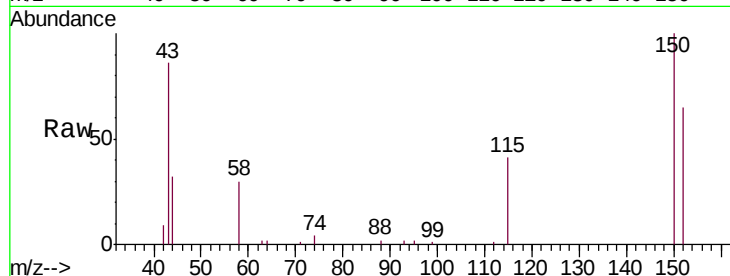

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

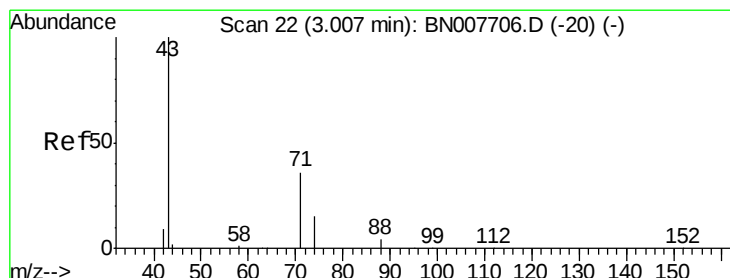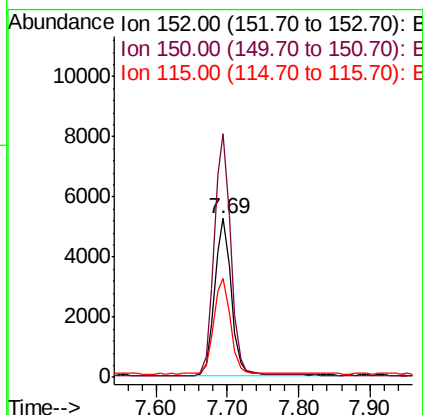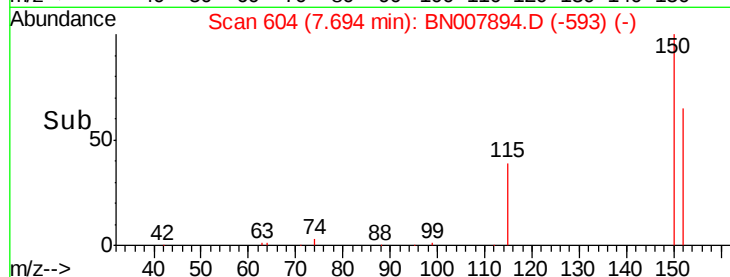

#3

n-Nitrosodimethylamine

Concen: 0.527 ng

RT: 3.01 min Scan# 22

Delta R.T. 0.00 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30


Tgt Ion: 42 Resp: 2262

Ion Ratio Lower Upper

42 100

74 104.2 87.9 131.9



44 28.5 29.4 44.0#

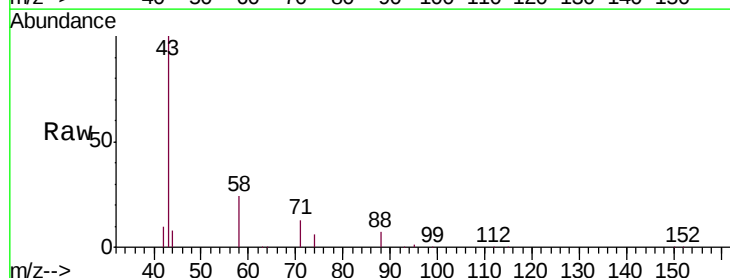

Abundance Ion 42.00 (41.70 to 42.70): BNC

Ion 74.00 (73.70 to 74.70): BNC

Ion 44.00 (43.70 to 44.70): BNC

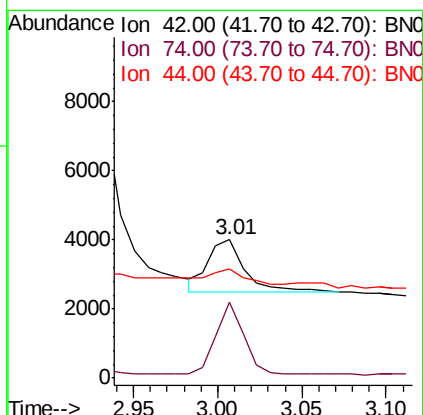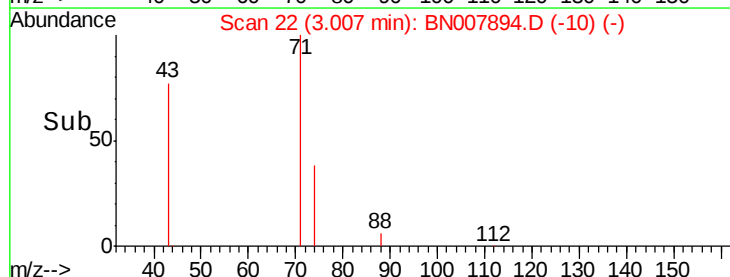



#4

2-Fluorophenol

Concen: 0.245 ng

RT: 5.31 min Scan# 308

Delta R.T. -0.01 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30

Instrument :

BNA_N

ClientSampleId :

PB123466BL


Tgt Ion: 112 Resp: 7071

Ion Ratio Lower Upper

112 100

64 59.4 46.6 70.0



63 29.7 23.1 34.7

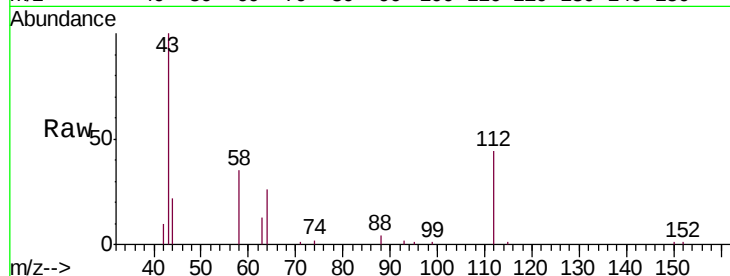

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

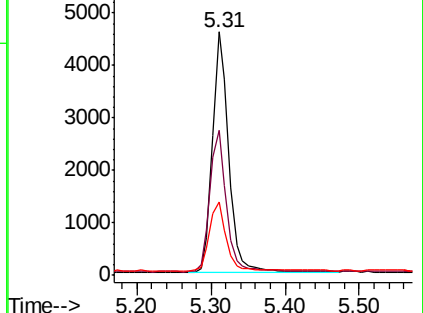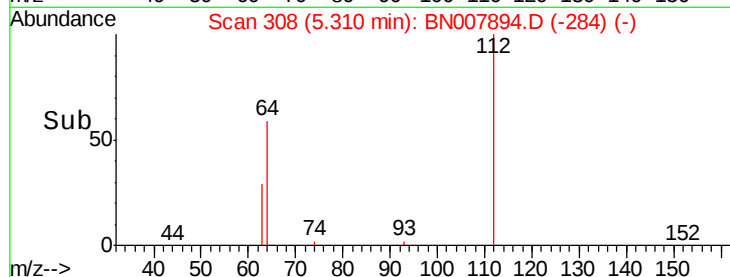

#5

Phenol-d6

Concen: 0.246 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30


Tgt Ion: 99 Resp: 8958

Ion Ratio Lower Upper

99 100

42 13.2 12.8 19.2



71 35.2 27.6 41.4

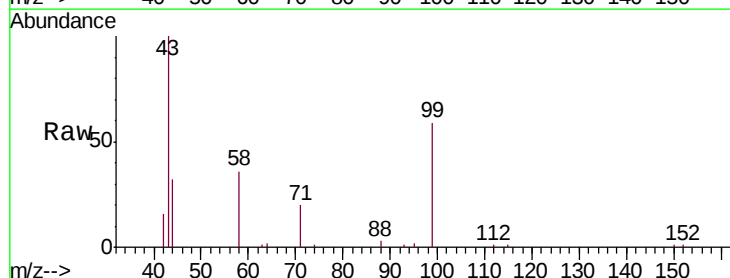

Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

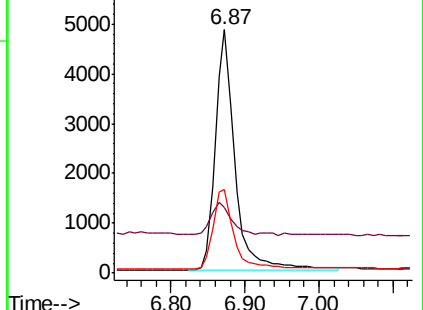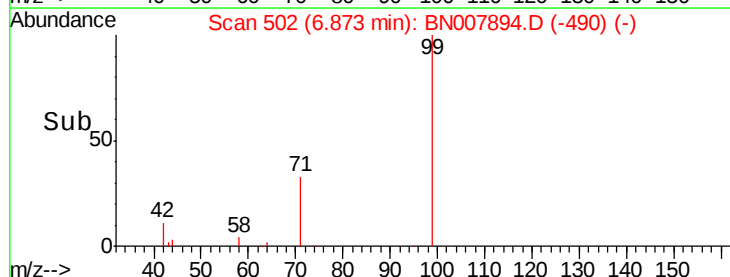



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.46 min Scan# 850

Delta R.T. -0.01 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30

Instrument :

BNA_N

ClientSampleId :

PB123466BL

Tgt Ion:136 Resp: 31323


Ion Ratio Lower Upper

136 100

137 11.2 9.2 13.8

54 7.4 5.8 8.8

68 7.8 6.5 9.7


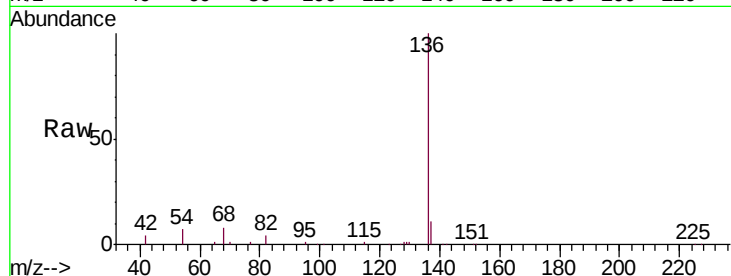


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BN0

Ion 68.00 (67.70 to 68.70): BN0

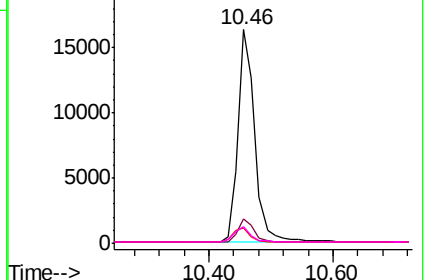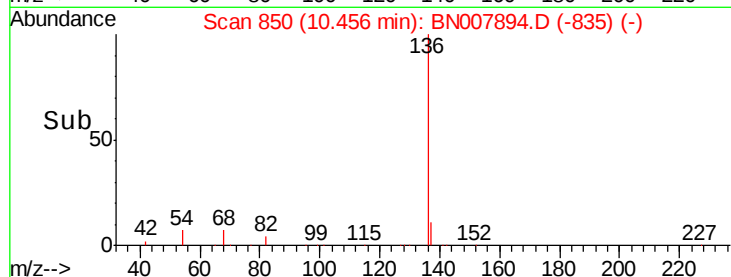

#8

Nitrobenzene-d5

Concen: 0.268 ng

RT: 8.83 min Scan# 722

Delta R.T. 0.00 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30


Tgt Ion: 82 Resp: 7354

Ion Ratio Lower Upper

82 100

128 38.4 24.5 36.7#



54 38.3 35.2 52.8

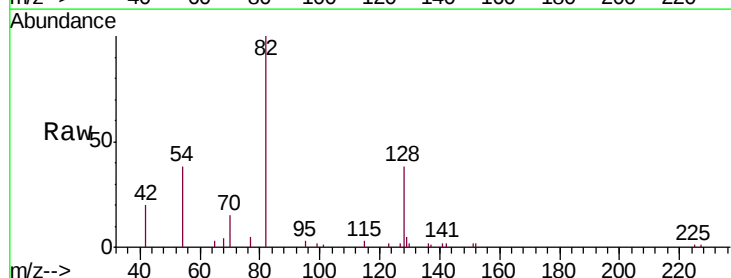

Abundance Ion 82.00 (81.70 to 82.70): BN0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BN0



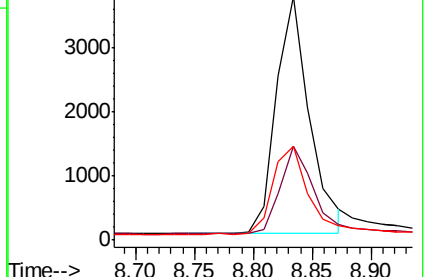
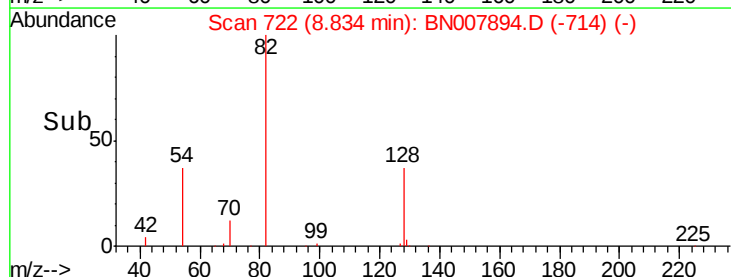




#11
 2-Methylnaphthalene-d10
 Concen: 0.291 ng
 RT: 12.05 min Scan# 1056
 Delta R.T. -0.01 min
 Lab File: BN007894.D
 Acq: 30 Sep 2019 13:30




Instrument :
 BNA_N
 ClientSampleId :
 PB123466BL


Tgt Ion:152 Resp: 15358
 Ion Ratio Lower Upper
 152 100
 151 19.4 15.4 23.2

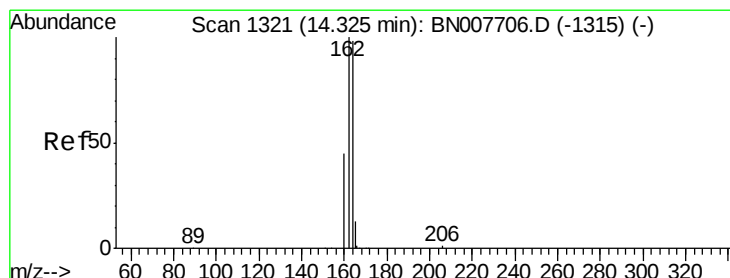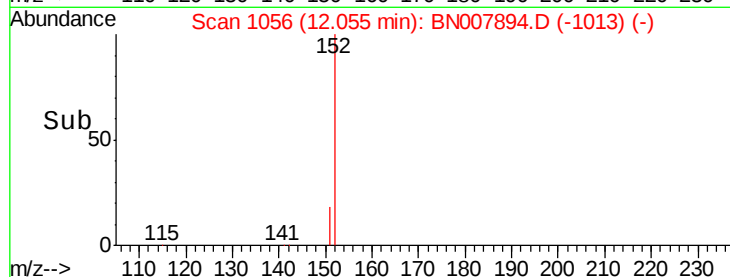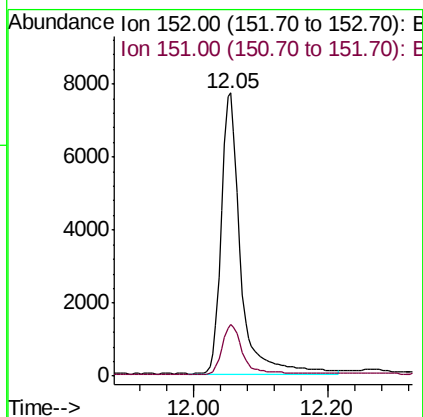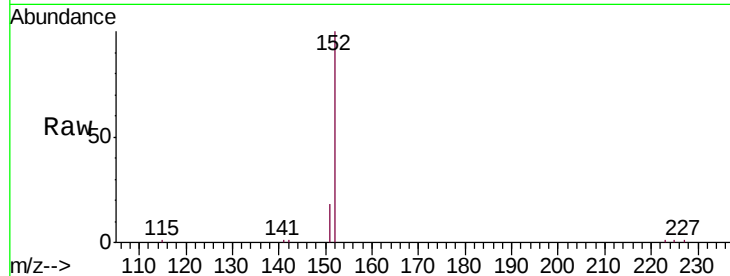

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.32 min Scan# 1320
 Delta R.T. -0.00 min
 Lab File: BN007894.D
 Acq: 30 Sep 2019 13:30

Tgt Ion:164 Resp: 17562
 Ion Ratio Lower Upper
 164 100
 162 99.6 81.7 122.5
 160 44.3 37.0 55.4

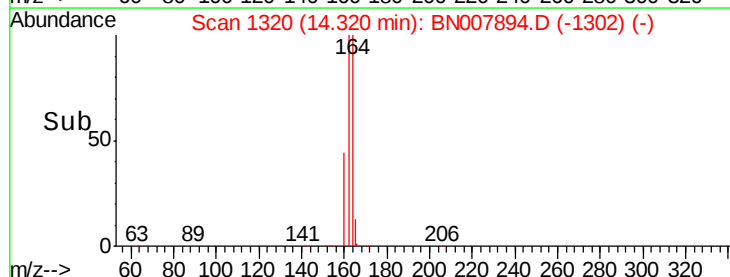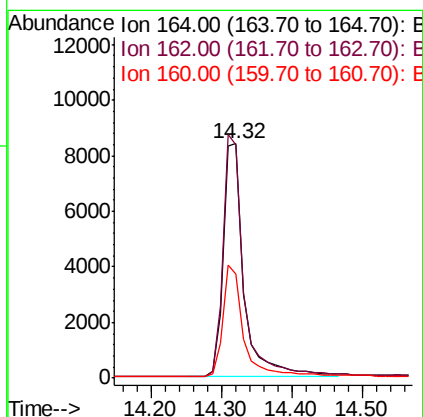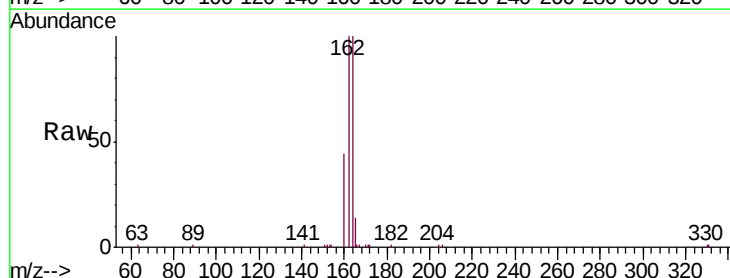


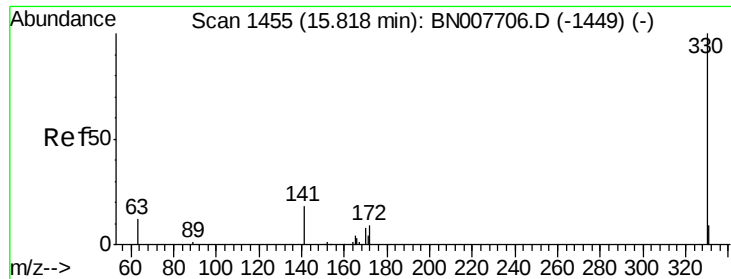




#14
2,4,6-Tribromophenol
Concen: 0.135 ng
RT: 15.81 min Scan# 1454
Delta R.T. -0.00 min
Lab File: BN007894.D
Acq: 30 Sep 2019 13:30

Instrument :
BNA_N
ClientSampleId :
PB123466BL

Tgt Ion: 330 Resp: 1290
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.4 28.7 43.1

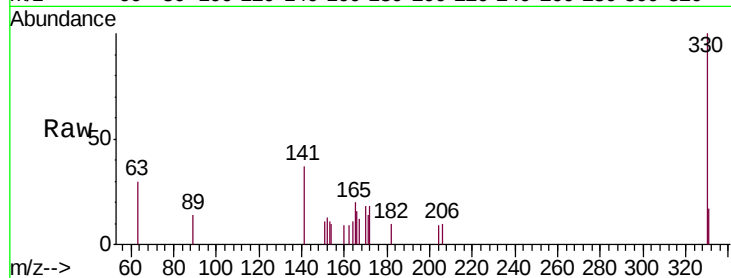


Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

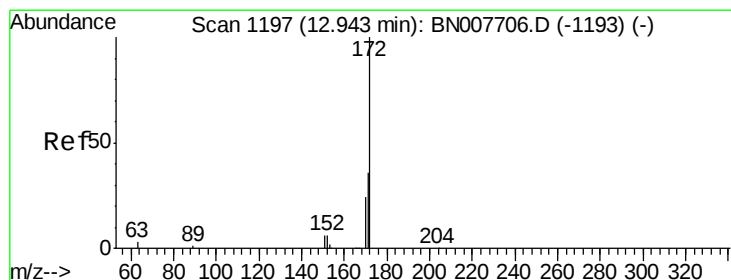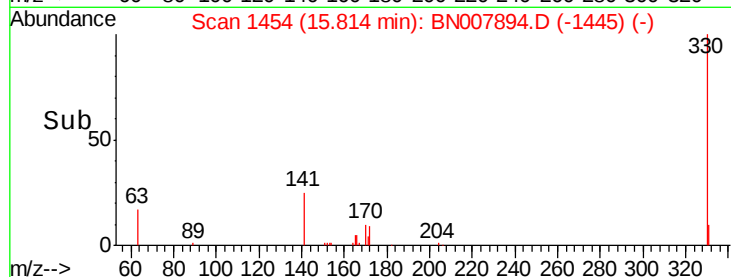
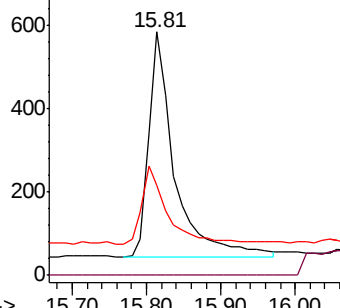



#15
2-Fluorobiphenyl
Concen: 0.279 ng
RT: 12.94 min Scan# 1196
Delta R.T. -0.00 min
Lab File: BN007894.D
Acq: 30 Sep 2019 13:30

Tgt Ion: 172 Resp: 20182
Ion Ratio Lower Upper
172 100
171 34.8 28.8 43.2
170 23.1 19.5 29.3

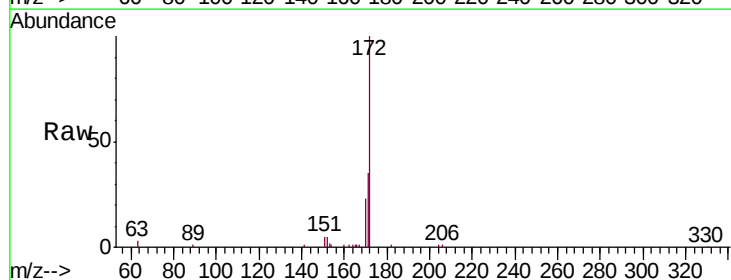

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

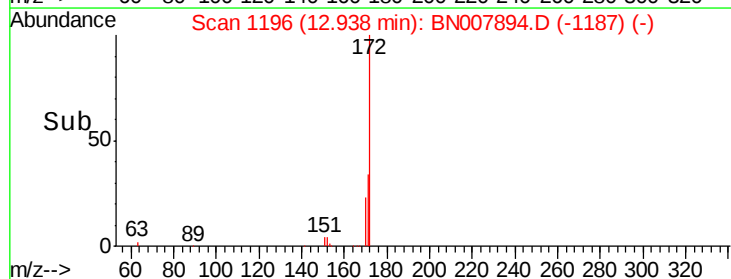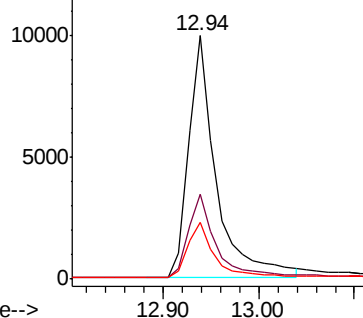

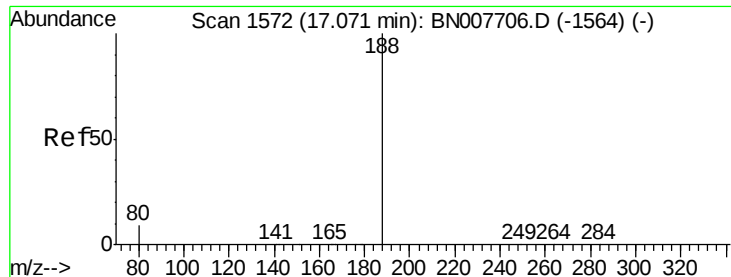

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.07 min Scan# 1571

Delta R.T. -0.00 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30

Instrument :

BNA_N

ClientSampleId :

PB123466BL


Tgt Ion:188 Resp: 35254

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 8.9 7.4 11.2

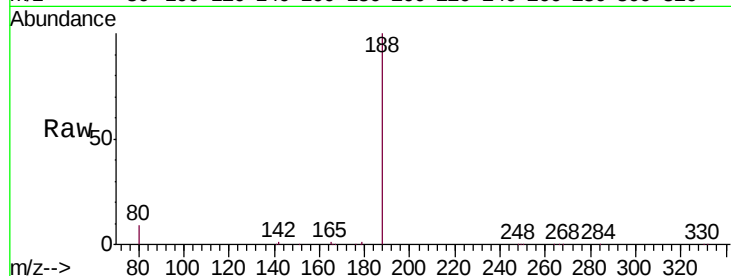

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

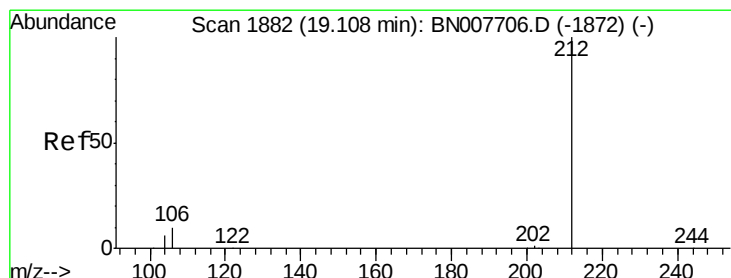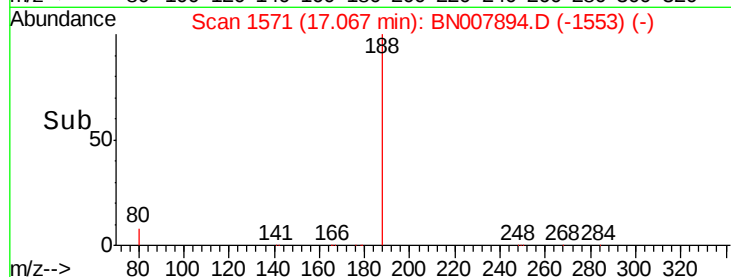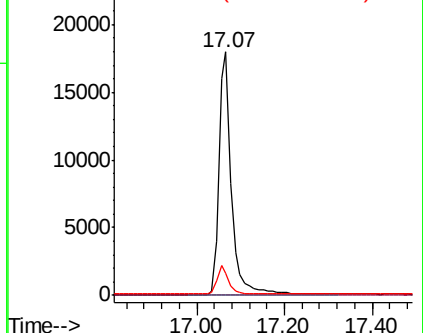

#25

Fluoranthene-d10

Concen: 0.251 ng

RT: 19.10 min Scan# 1878

Delta R.T. -0.01 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30


Tgt Ion:212 Resp: 29834

Ion Ratio Lower Upper

212 100

106 11.8 9.4 14.0



104 6.6 5.3 7.9

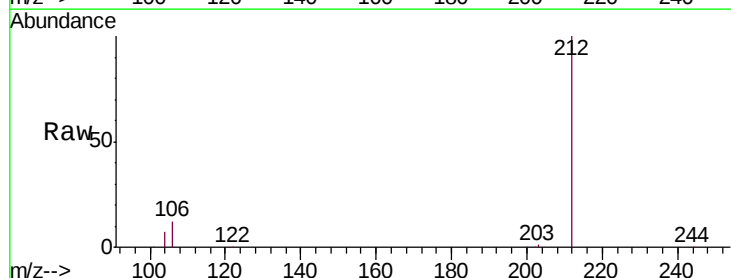


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

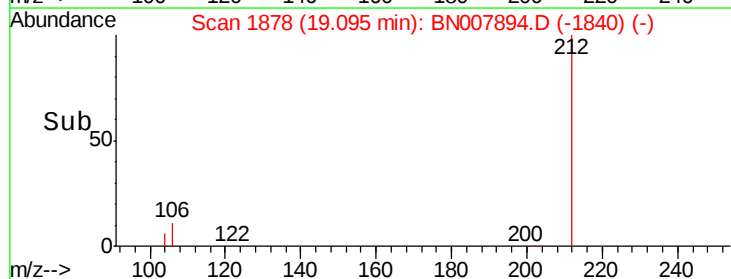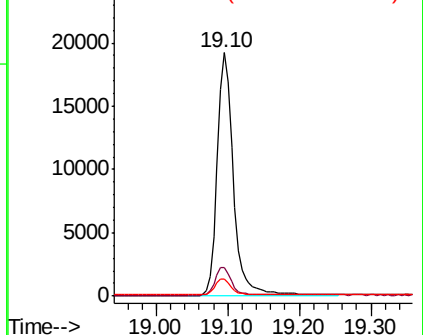

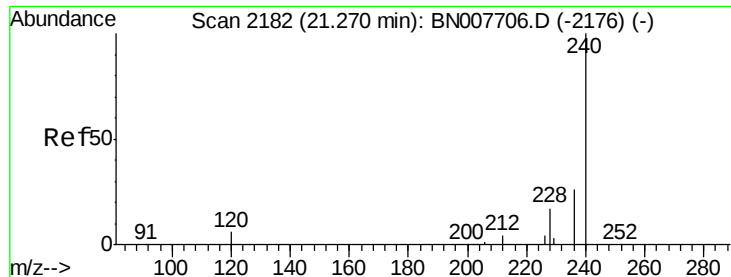

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.25 min Scan# 2179

Delta R.T. -0.02 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30

Instrument :

BNA_N

ClientSampleId :

PB123466BL


Tgt Ion:240 Resp: 28294

Ion Ratio Lower Upper

240 100

120 12.9 5.4 8.2#




236 27.1 21.0 31.4

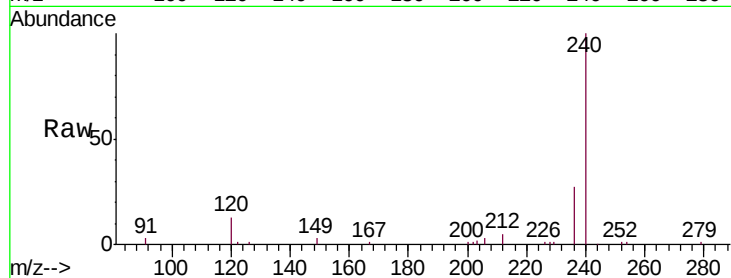

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

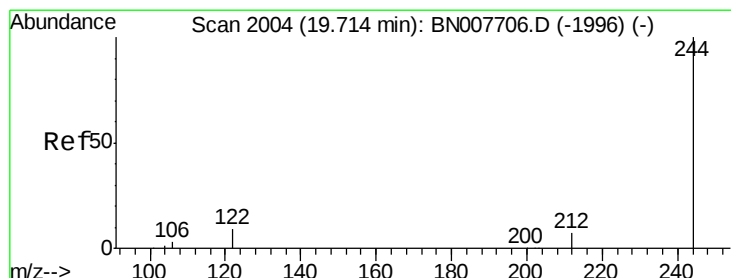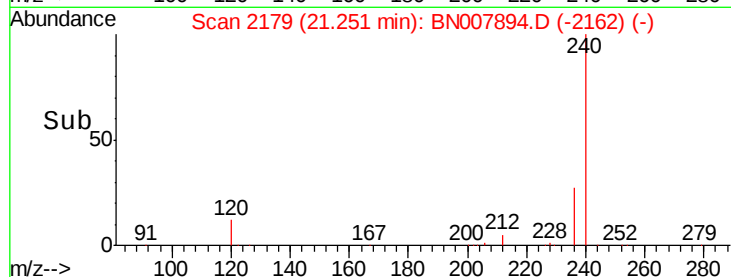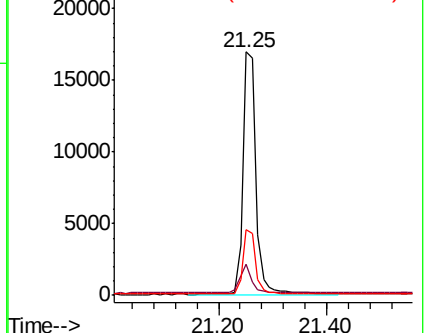

#29

Terphenyl-d14

Concen: 0.340 ng

RT: 19.70 min Scan# 2000

Delta R.T. -0.01 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30


Tgt Ion:244 Resp: 23659

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9



122 9.9 7.4 11.2



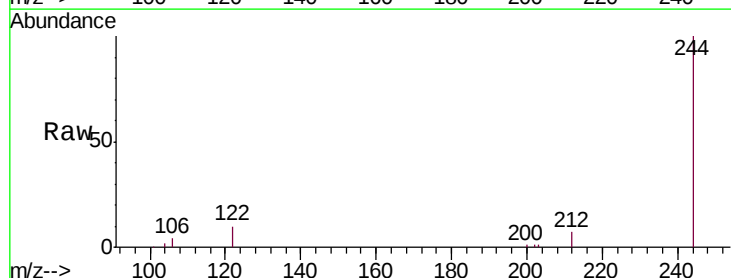


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

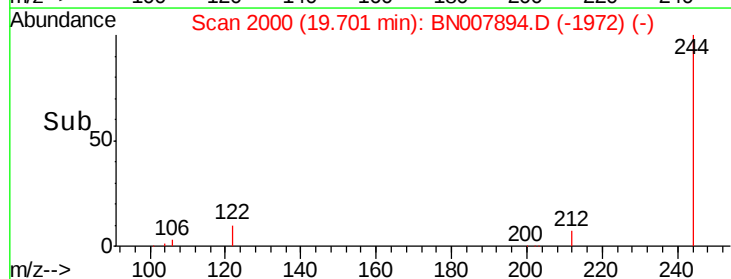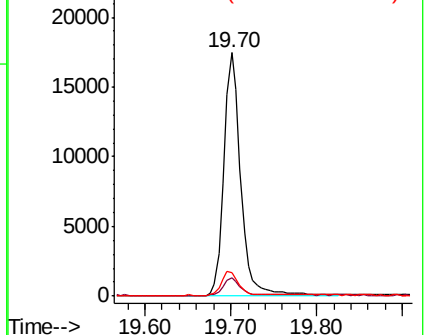

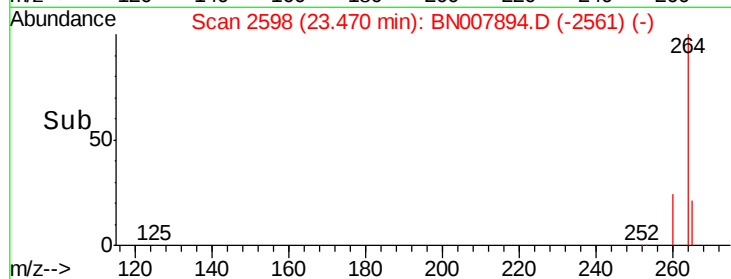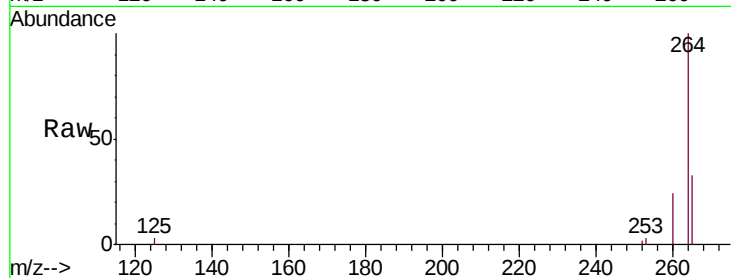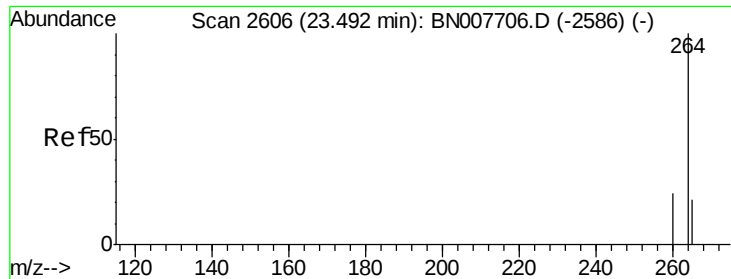

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.47 min Scan# 2598

Delta R.T. -0.02 min

Lab File: BN007894.D

Acq: 30 Sep 2019 13:30

Instrument :

BNA_N

ClientSampleId :

PB123466BL

Tgt Ion: 264 Resp: 34234

Ion Ratio Lower Upper

264 100

260 23.9 19.3 28.9

265 33.1 26.9 40.3

