
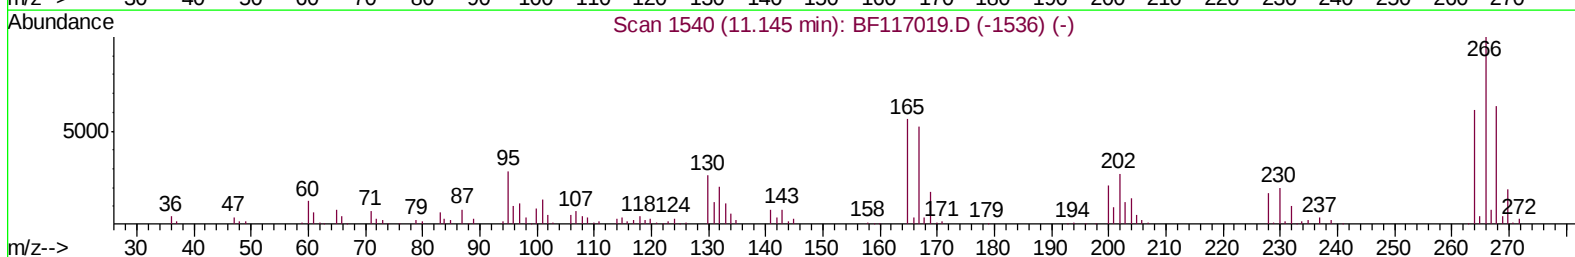
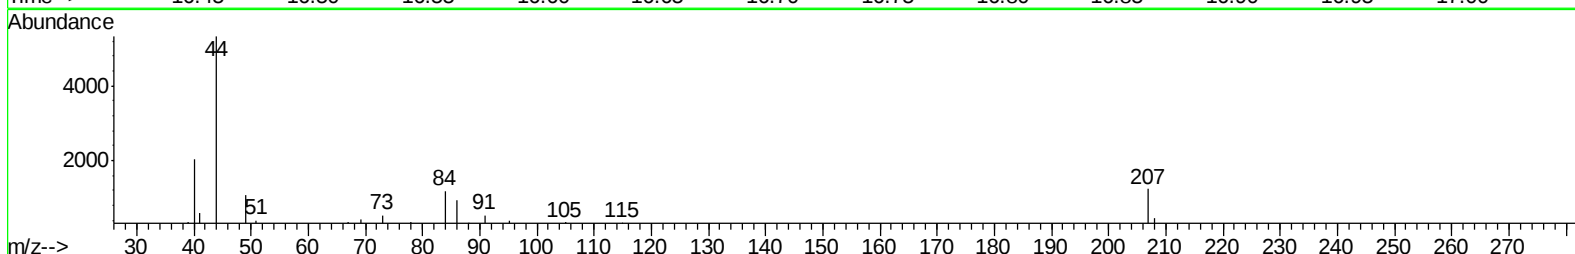


Data File : BN007908.D
Acq On : 30 Sep 2019 22:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 09:11:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

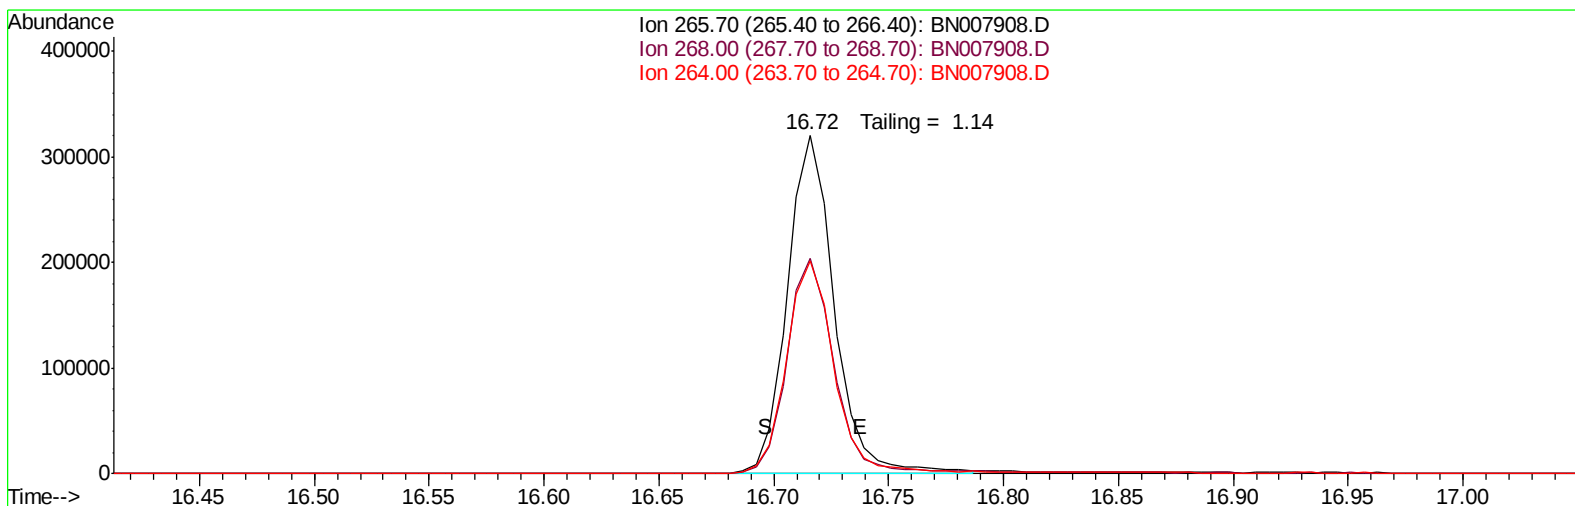

TIC: BN007908.D

(70) Pentachlorophenol (C)




11.145min (-11.145) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.10	0.00#
264.00	61.00	0.00#
0.00	0.00	0.00

Data File : BN007908.D
Acq On : 30 Sep 2019 22:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 09:11:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

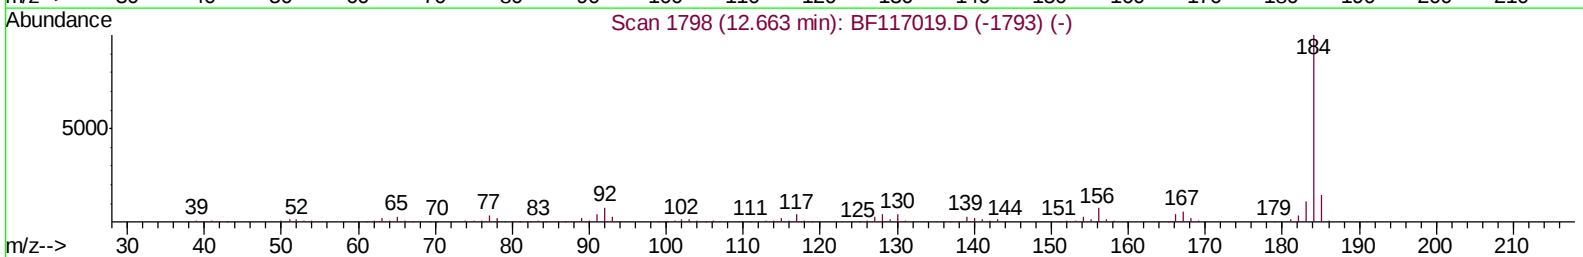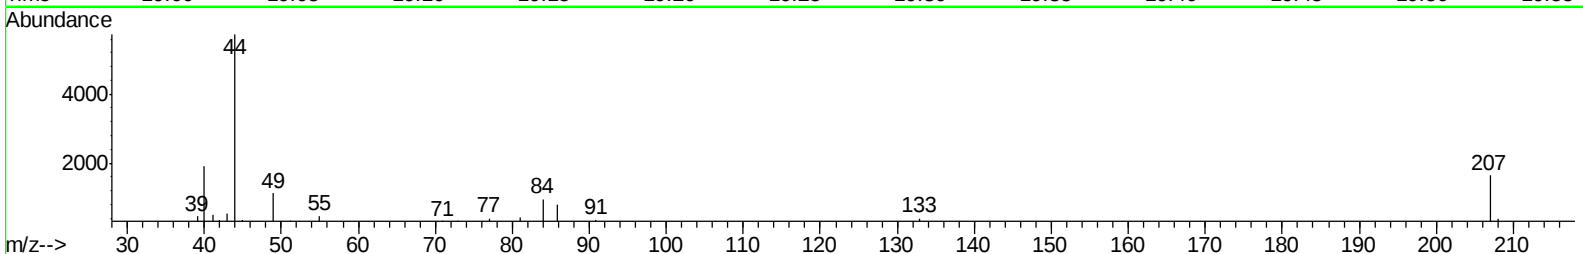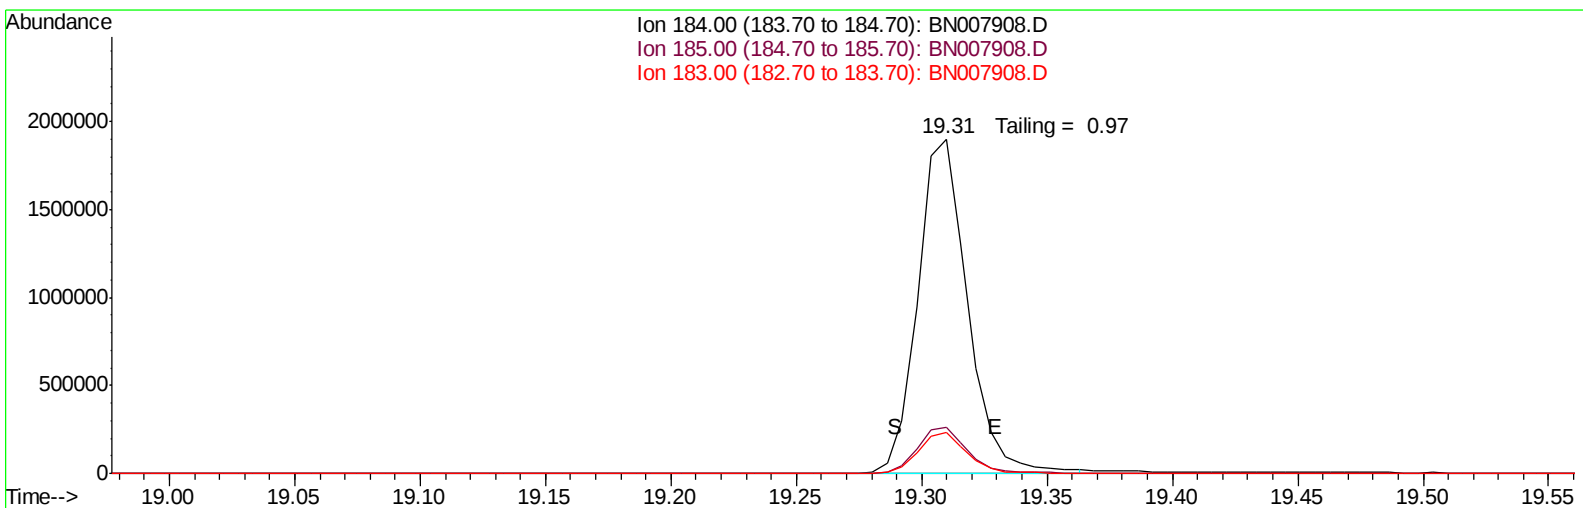

TIC: BN007908.D

(77) Benzidine

12.663min (-12.663) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.50	0.00#
183.00	11.20	0.00#
0.00	0.00	0.00