


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093019\
 Data File : BN007889.D
 Acq On : 30 Sep 2019 10:31
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

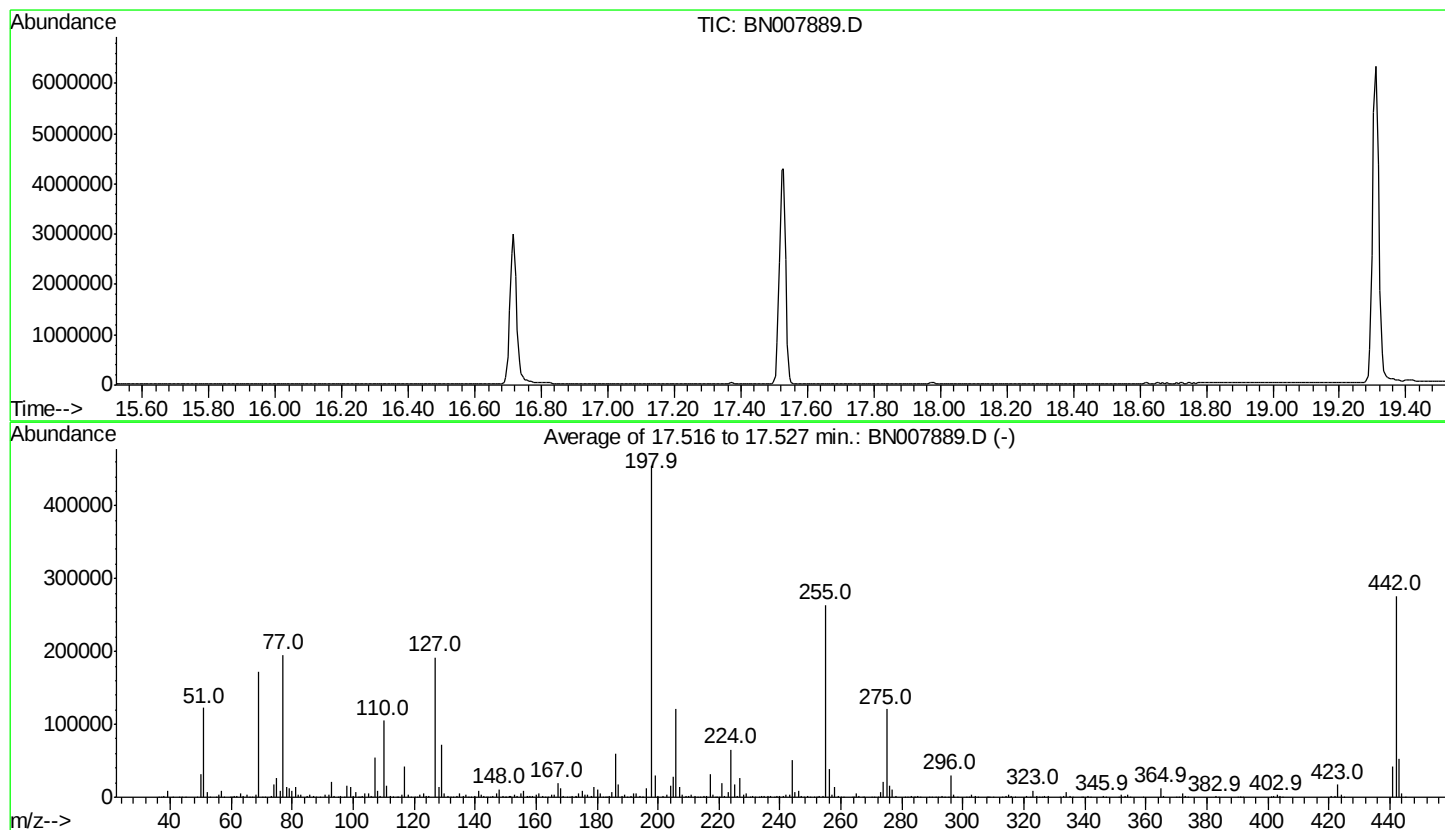

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	122488	PASS
68	69	0.00	2	1.9	3232	PASS
69	198	0.00	100	37.9	172650	PASS
70	69	0.00	2	0.5	914	PASS
127	198	10	80	42.1	191701	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	455082	PASS
199	198	5	9	6.7	30616	PASS
275	198	10	60	26.5	120824	PASS
365	198	1	100	2.8	12872	PASS
441	198	0.01	100	9.4	42954	PASS
442	198	50	100	60.7	276181	PASS
443	442	15	24	19.3	53285	PASS