

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093021\
 Data File : BN016586.D
 Acq On : 29 Sep 2021 22:07
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Sep 30 01:38:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN093021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 01:35:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	32242	0.400	ng	0.00
7) Naphthalene-d8	10.419	136	126767	0.400	ng	0.00
13) Acenaphthene-d10	14.281	164	64508	0.400	ng	0.00
19) Phenanthrene-d10	17.030	188	117824	0.400	ng	0.00
29) Chrysene-d12	21.238	240	116480	0.400	ng	0.00
35) Perylene-d12	23.498	264	123329	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	382676	4.770	ng	0.00
5) Phenol-d6	6.822	99	429262	5.327	ng	0.00
8) Nitrobenzene-d5	8.784	82	454372	6.751	ng	0.00
11) 2-Methylnaphthalene-d10	12.012	152	880899	4.886	ng	0.00
14) 2,4,6-Tribromophenol	15.778	330	175657	6.238	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	1241754	4.678	ng	0.00
27) Fluoranthene-d10	19.073	212	1606300	5.045	ng	0.00
31) Terphenyl-d14	19.688	244	1297139	5.169	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.253	88	68357	4.923	ng	# 73
3) n-Nitrosodimethylamine	3.576	42	122845	4.798	ng	98
6) bis(2-Chloroethyl)ether	7.089	93	390169	4.595	ng	100
9) Naphthalene	10.457	128	1622900	4.746	ng	99
10) Hexachlorobutadiene	10.749	225	308492	4.569	ng	# 100
12) 2-Methylnaphthalene	12.083	142	1010497	4.747	ng	100
16) Acenaphthylene	13.990	152	1497890	5.238	ng	100
17) Acenaphthene	14.345	154	934131	4.808	ng	97
18) Fluorene	15.334	166	1123457	4.746	ng	99
21) 4-Bromophenyl-phenylether	16.226	248	374739	5.379	ng	# 72
22) Hexachlorobenzene	16.336	284	408333	4.908	ng	99
23) Atrazine	16.506	200	315430	6.651	ng	100
25) Phenanthrene	17.066	178	1719761	4.852	ng	100
26) Anthracene	17.164	178	1616023	5.247	ng	100
28) Fluoranthene	19.108	202	1868510	4.823	ng	99
30) Pyrene	19.470	202	1961246	4.938	ng	100
32) Benzo(a)anthracene	21.227	228	1946491	5.391	ng	99
33) Chrysene	21.280	228	1900589	5.162	ng	99
36) Indeno(1,2,3-cd)pyrene	25.788	276	2416229	6.144	ng	99
37) Benzo(b)fluoranthene	22.820	252	2067638	5.021	ng	100
38) Benzo(k)fluoranthene	22.865	252	1952527	4.866	ng	# 96
39) Benzo(a)pyrene	23.399	252	1912352	5.063	ng	99
40) Dibenzo(a,h)anthracene	25.809	278	1995307	7.302	ng	97
41) Benzo(g,h,i)perylene	26.483	276	2127332	5.949	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093021\
Data File : BN016586.D
Acq On : 29 Sep 2021 22:07
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Sep 30 01:38:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN093021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 01:35:49 2021
Response via : Initial Calibration




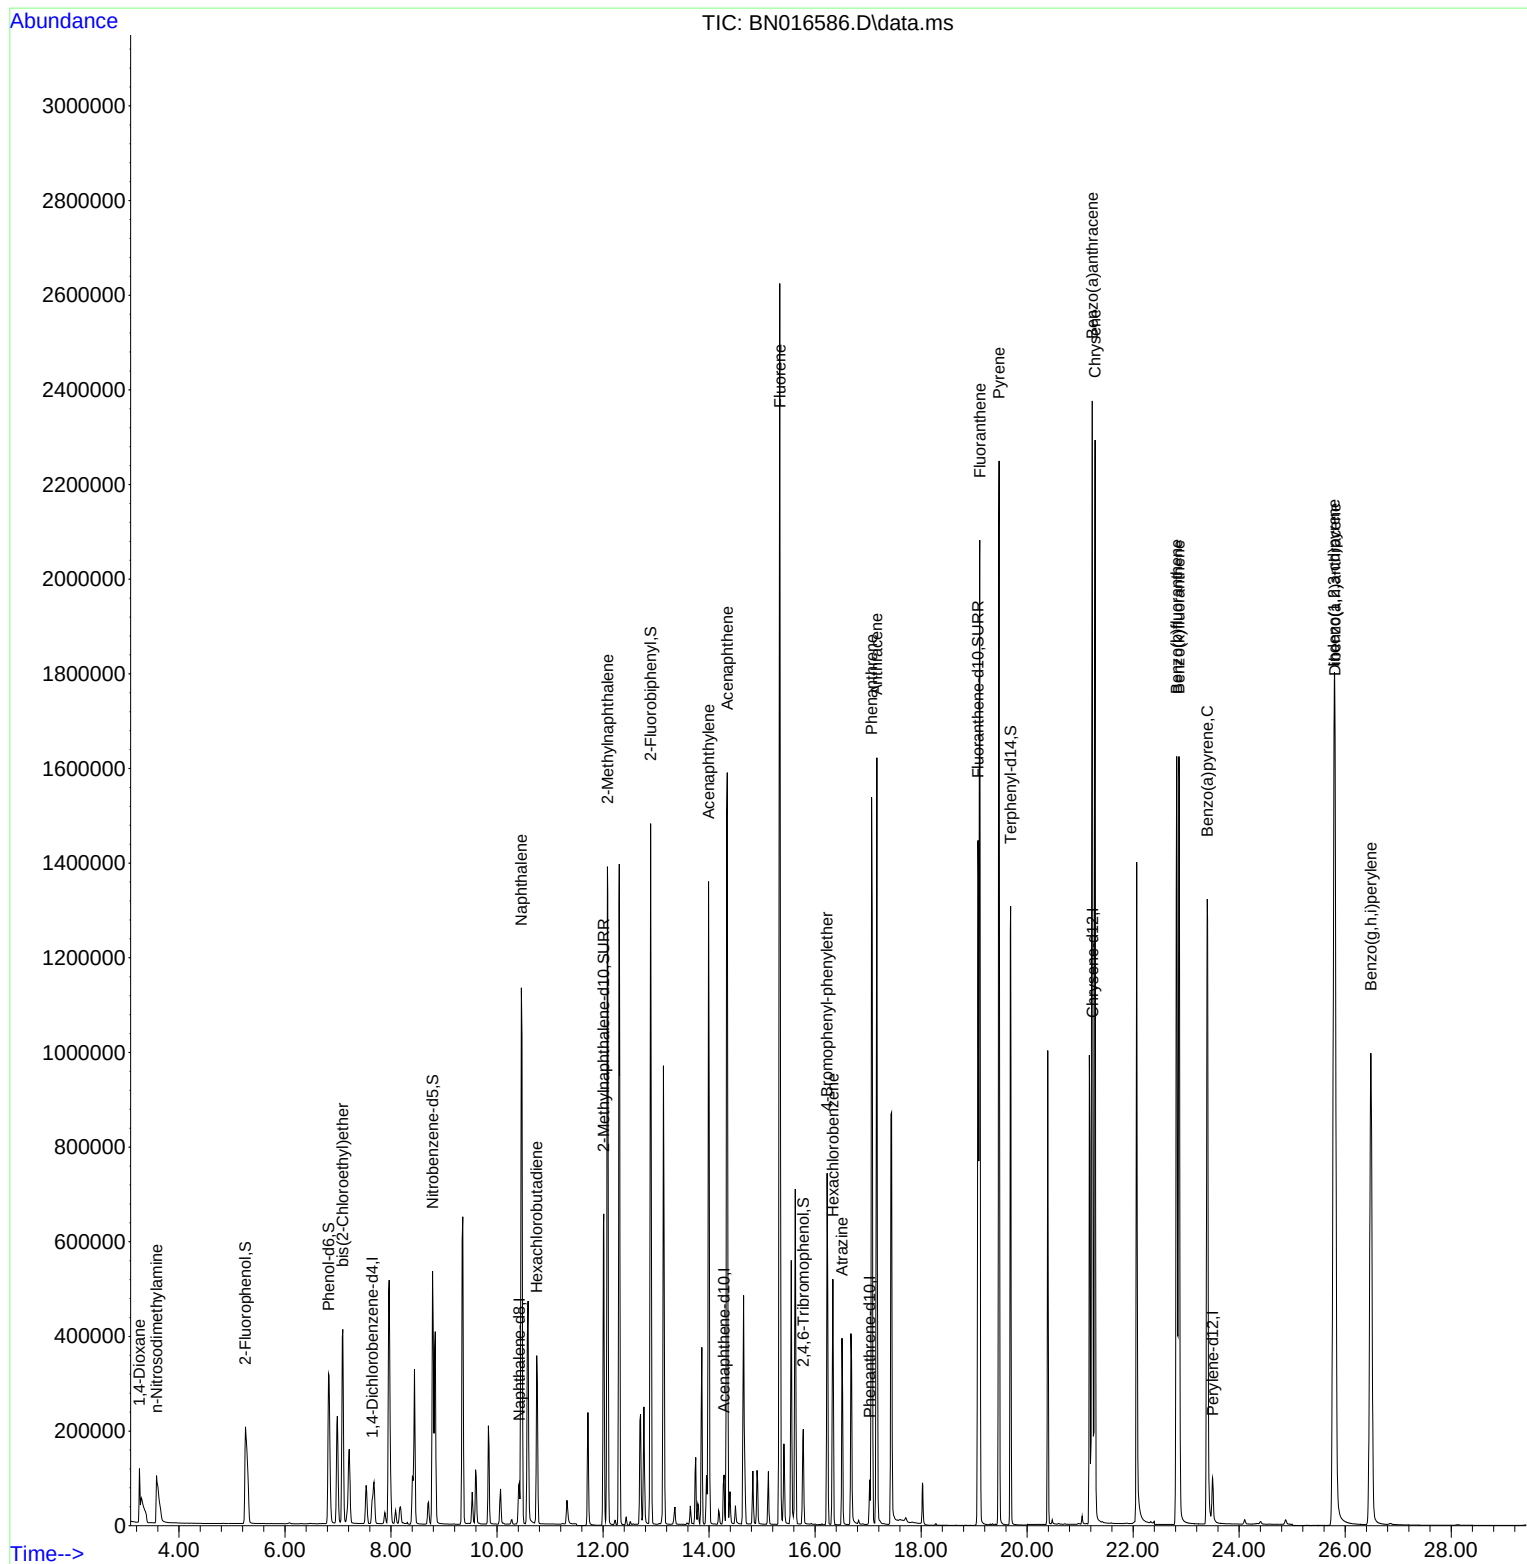




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.642 min Scan# 495
Delta R.T. -0.010 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampled :
SSTDICC5.0


Tgt Ion:152 Resp: 32242
Ion Ratio Lower Upper
152 100
150 158.5 123.3 184.9
115 60.2 46.2 69.2



#2
1,4-Dioxane
Concen: 4.923 ng
RT: 3.253 min Scan# 19
Delta R.T. -0.009 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion: 88 Resp: 68357
Ion Ratio Lower Upper
88 100
43 27.8 49.1 73.7#
58 74.0 52.0 78.0

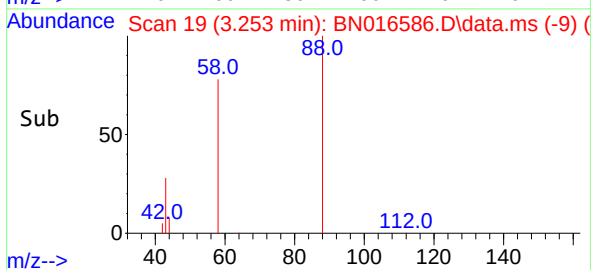







#3
n-Nitrosodimethylamine
Concen: 4.798 ng
RT: 3.576 min Scan# 54
Delta R.T. -0.009 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion: 42 Resp: 122845




Ion	Ratio	Lower	Upper
42	100		
74	152.6	123.7	185.5
44	6.4	6.3	9.5

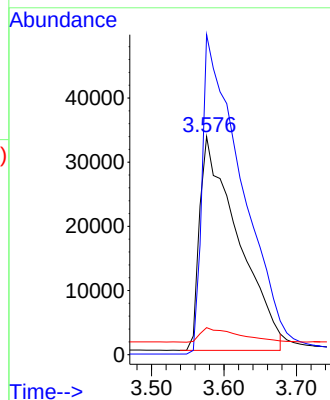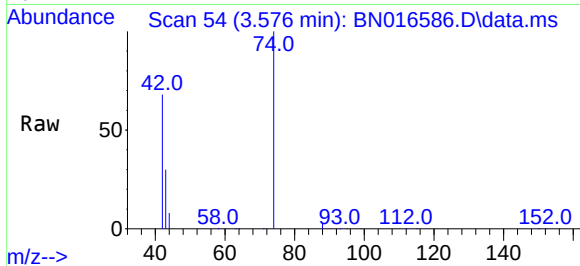


#4
2-Fluorophenol
Concen: 4.770 ng
RT: 5.254 min Scan# 236
Delta R.T. -0.009 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion: 112 Resp: 382676

Ion	Ratio	Lower	Upper
112	100		
64	54.3	43.4	65.2
63	27.3	21.8	32.8


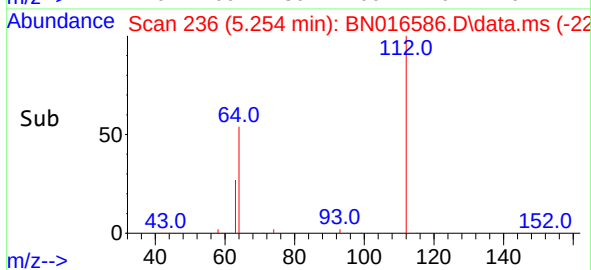
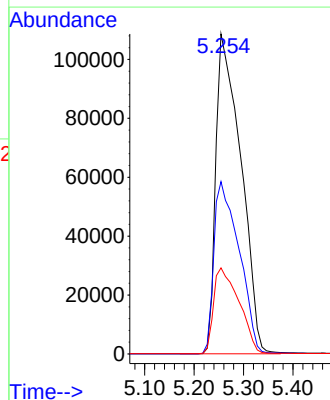
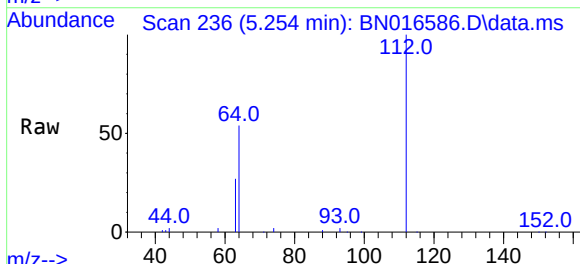




#5
Phenol-d6
Concen: 5.327 ng
RT: 6.822 min Scan# 406
Delta R.T. -0.009 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 429262
Ion Ratio Lower Upper
99 100
42 16.5 13.3 19.9
71 29.5 23.7 35.5



#6
bis(2-Chloroethyl)ether
Concen: 4.595 ng
RT: 7.089 min Scan# 435
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion: 93 Resp: 390169
Ion Ratio Lower Upper
93 100
63 73.7 59.1 88.7
95 32.7 26.3 39.5









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.419 min Scan# 734
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	126767
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	4.6	4.0	6.0
68	4.1	3.6	5.4

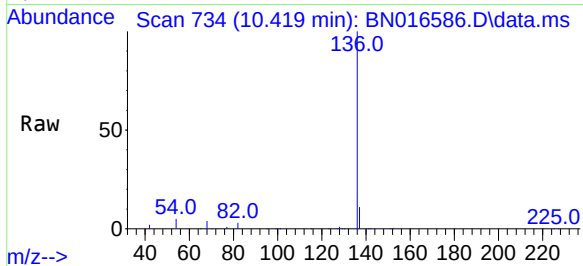

#8
Nitrobenzene-d5
Concen: 6.751 ng
RT: 8.784 min Scan# 605
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:	82	Resp:	454372
Ion	Ratio	Lower	Upper
82	100		
128	39.8	28.6	42.8
54	49.4	42.0	63.0


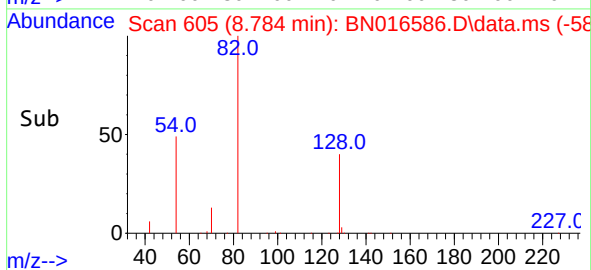

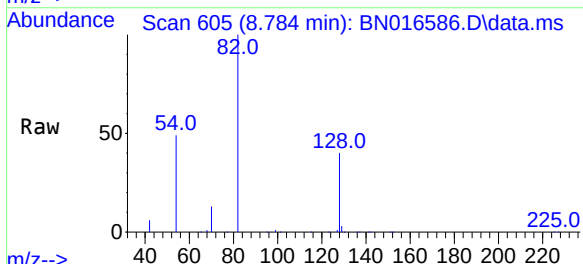




#9
Naphthalene
Concen: 4.746 ng
RT: 10.457 min Scan# 737
Delta R.T. -0.013 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1622900
Ion Ratio Lower Upper
128 100
129 11.1 8.8 13.2
127 13.0 10.1 15.1



#10
Hexachlorobutadiene
Concen: 4.569 ng
RT: 10.749 min Scan# 760
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:225 Resp: 308492
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.2 76.8


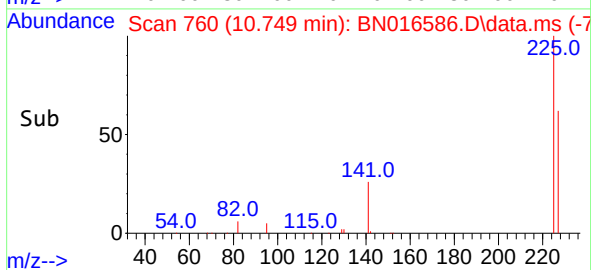




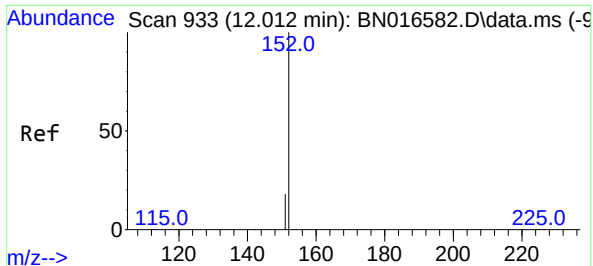

#11
2-Methylnaphthalene-d10
Concen: 4.886 ng
RT: 12.012 min Scan# 933
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 880899
Ion Ratio Lower Upper
152 100
151 20.1 16.3 24.5

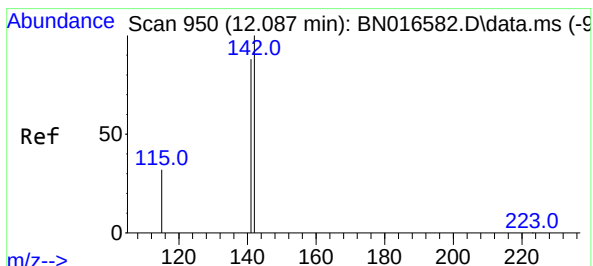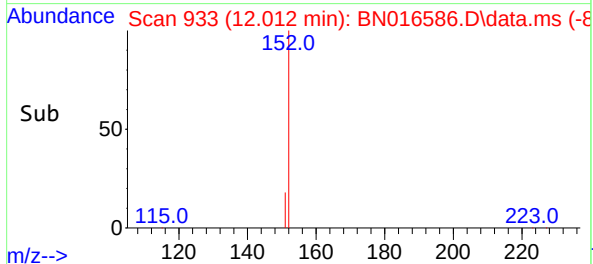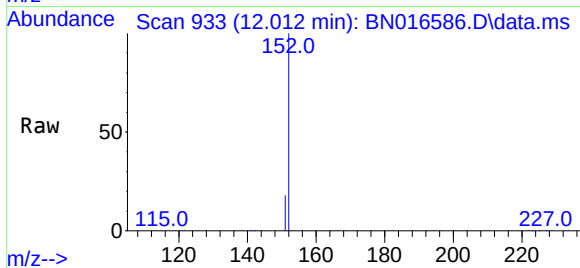

#12
2-Methylnaphthalene
Concen: 4.747 ng
RT: 12.083 min Scan# 949
Delta R.T. -0.004 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:142 Resp: 1010497
Ion Ratio Lower Upper
142 100
141 87.5 70.2 105.4
115 32.7 26.1 39.1


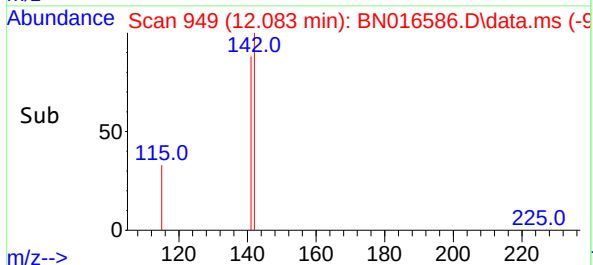

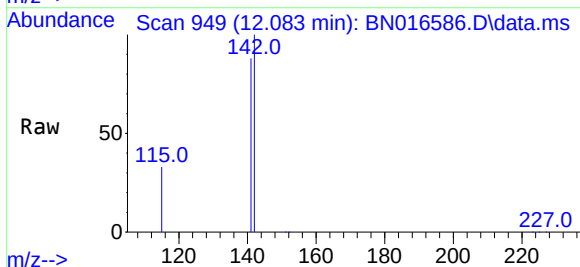




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.281 min Scan# 1184
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 64508
Ion Ratio Lower Upper
164 100
162 99.0 79.8 119.6
160 43.5 35.7 53.5



#14
2,4,6-Tribromophenol
Concen: 6.238 ng
RT: 15.778 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:330 Resp: 175657
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 31.6 25.4 38.2

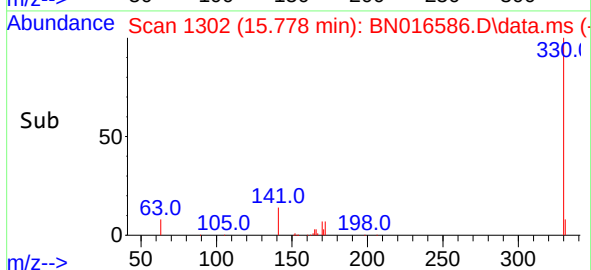







#15
2-Fluorobiphenyl
Concen: 4.678 ng
RT: 12.898 min Scan# 1075
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:172 Resp: 1241754




Ion	Ratio	Lower	Upper
172	100		
171	34.0	27.6	41.4
170	22.6	18.7	28.1




#16
Acenaphthylene
Concen: 5.238 ng
RT: 13.990 min Scan# 1161
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:152 Resp: 1497890

Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.4	23.2
153	13.1	10.4	15.6







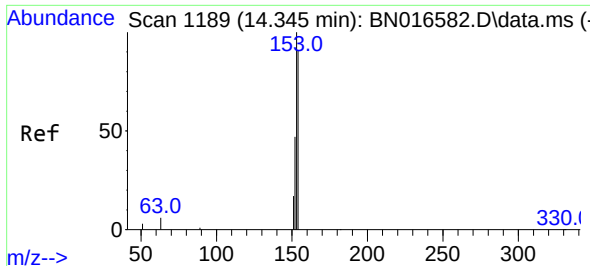

#17
Acenaphthene
Concen: 4.808 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 934131
Ion Ratio Lower Upper
154 100
153 110.4 90.5 135.7
152 52.8 44.5 66.7

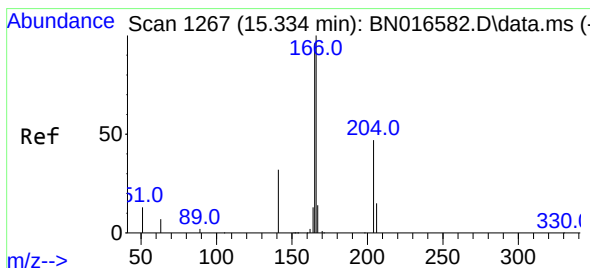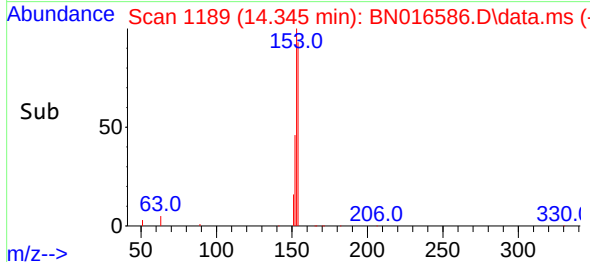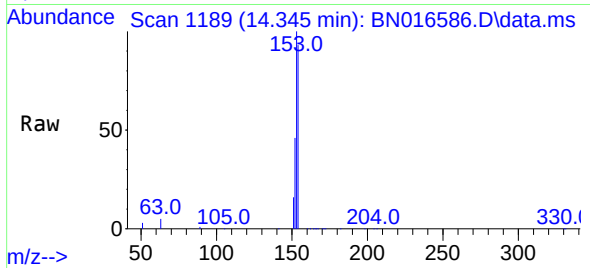

#18
Fluorene
Concen: 4.746 ng
RT: 15.334 min Scan# 1267
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:166 Resp: 1123457
Ion Ratio Lower Upper
166 100
165 96.1 78.1 117.1
167 13.6 10.7 16.1


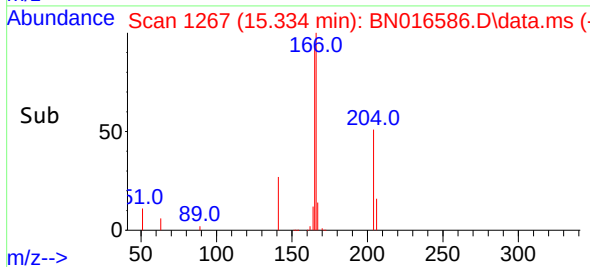

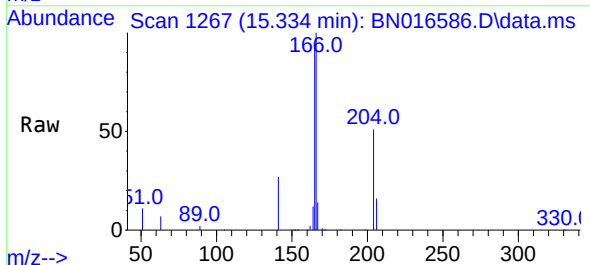


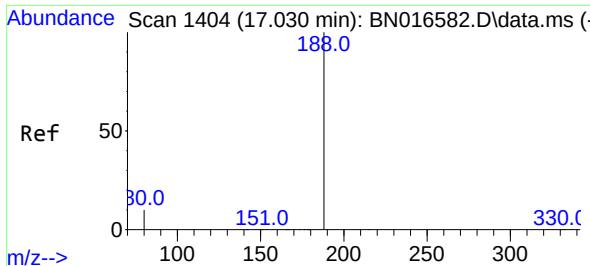

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.030 min Scan# 1404
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 117824
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.7 8.1 12.1

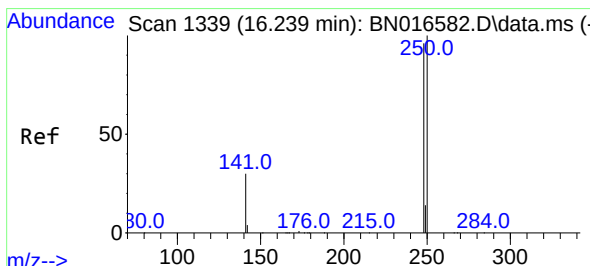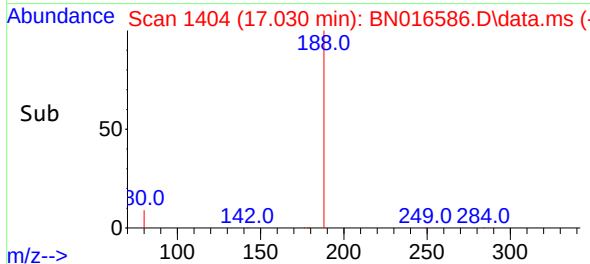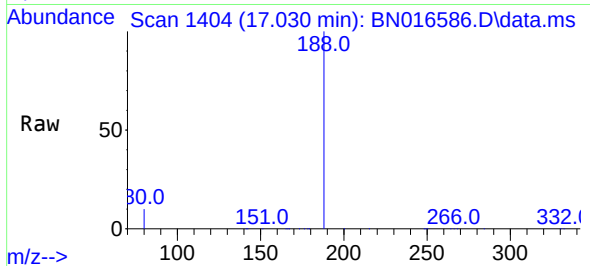

#21
4-Bromophenyl-phenylether
Concen: 5.379 ng
RT: 16.226 min Scan# 1338
Delta R.T. -0.012 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:248 Resp: 374739
Ion Ratio Lower Upper
248 100
250 91.6 83.7 125.5
141 75.9 25.3 37.9#


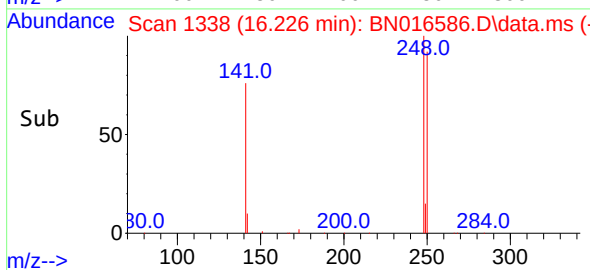

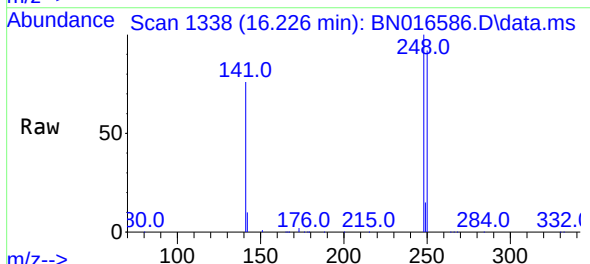




#22
Hexachlorobenzene
Concen: 4.908 ng
RT: 16.336 min Scan# 1347
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 408333
Ion Ratio Lower Upper
284 100
142 32.8 26.7 40.1
249 29.5 23.4 35.2



#23
Atrazine
Concen: 6.651 ng
RT: 16.506 min Scan# 1361
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:200 Resp: 315430
Ion Ratio Lower Upper
200 100
173 31.0 25.0 37.6
215 46.2 37.1 55.7


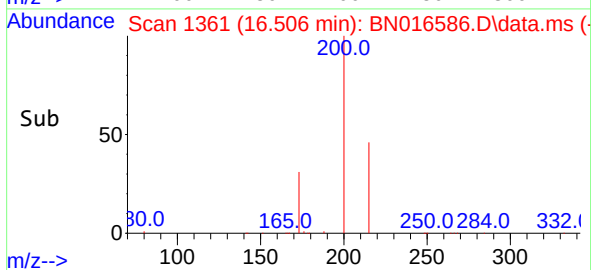




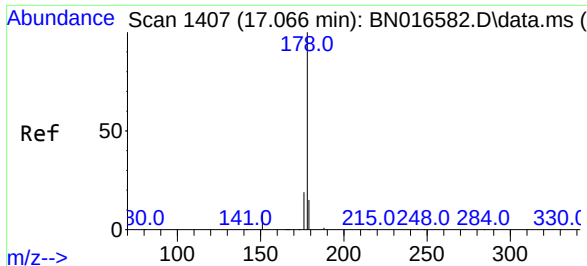

#25
Phenanthrene
Concen: 4.852 ng
RT: 17.066 min Scan# 1407
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 1719761
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.6
179 15.5 12.2 18.2

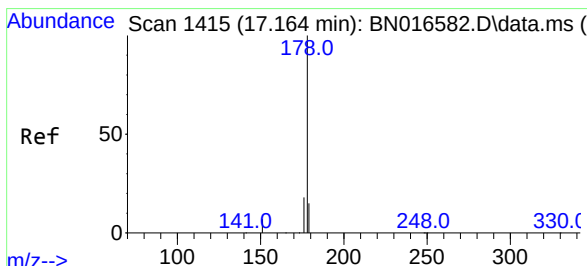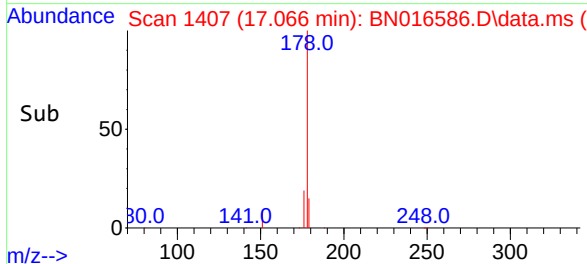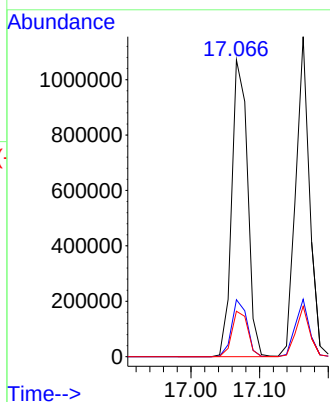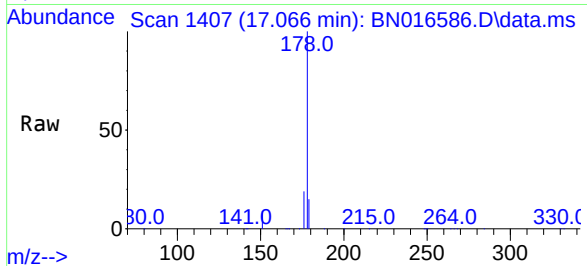

#26
Anthracene
Concen: 5.247 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:178 Resp: 1616023
Ion Ratio Lower Upper
178 100
176 18.2 14.6 22.0
179 15.4 12.3 18.5


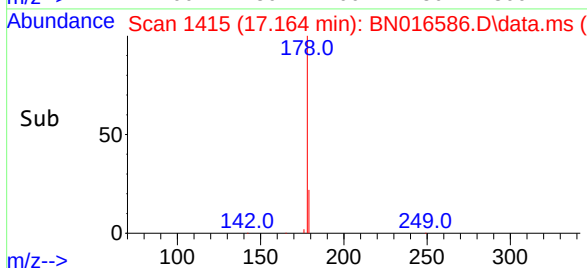
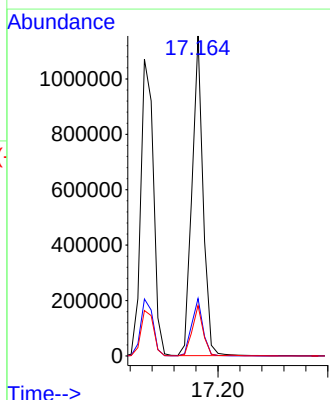
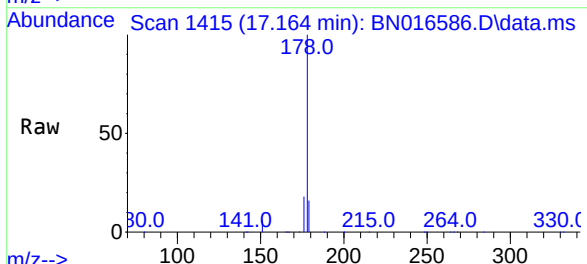




#27
Fluoranthene-d10
Concen: 5.045 ng
RT: 19.073 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 1606300
Ion Ratio Lower Upper
212 100
106 14.0 11.0 16.6
104 7.7 6.0 9.0

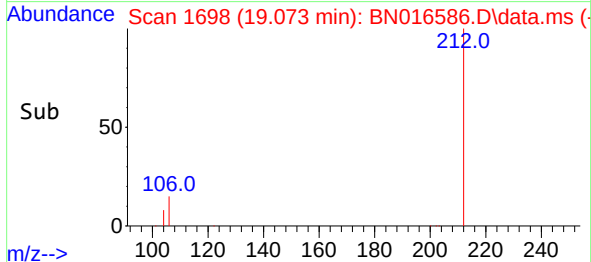

#28
Fluoranthene
Concen: 4.823 ng
RT: 19.108 min Scan# 1705
Delta R.T. 0.005 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:202 Resp: 1868510
Ion Ratio Lower Upper
202 100
101 11.6 9.1 13.7
203 17.6 13.8 20.8


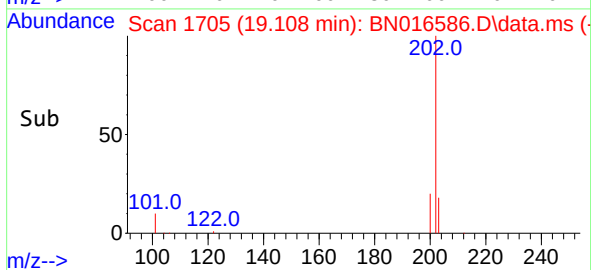






#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.238 min Scan# 2002
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 116480
Ion Ratio Lower Upper
240 100
120 14.1 11.6 17.4
236 26.9 21.6 32.4

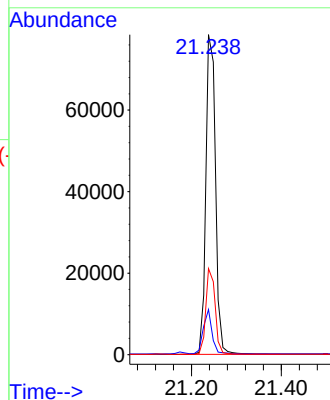

#30
Pyrene
Concen: 4.938 ng
RT: 19.470 min Scan# 1778
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:202 Resp: 1961246
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.8 13.9 20.9


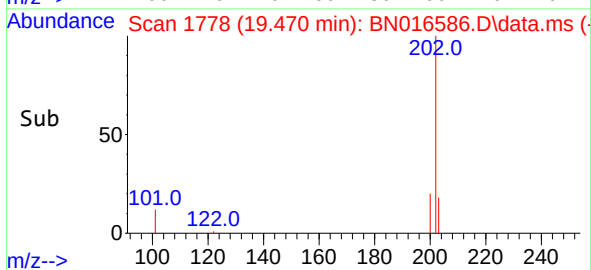
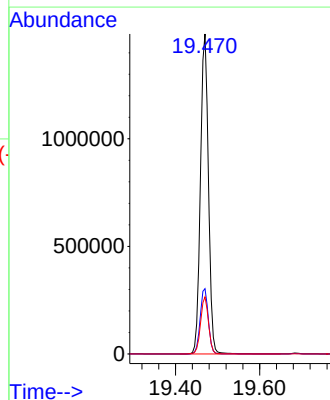





#31
Terphenyl-d14
Concen: 5.169 ng
RT: 19.688 min Scan# 1822
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:244 Resp: 1297139
Ion Ratio Lower Upper
244 100
212 7.3 5.8 8.8
122 12.1 9.2 13.8

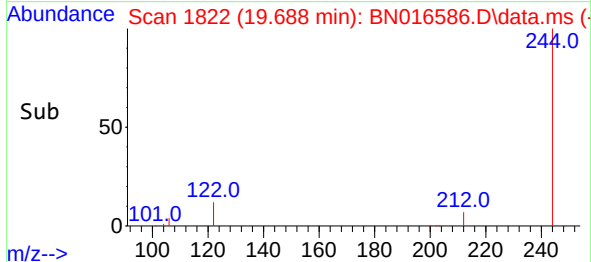

#32
Benzo(a)anthracene
Concen: 5.391 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:228 Resp: 1946491
Ion Ratio Lower Upper
228 100
226 26.4 21.4 32.0
229 20.1 15.6 23.4



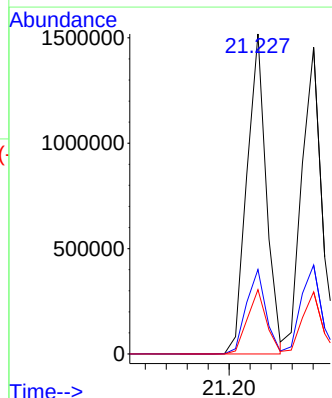



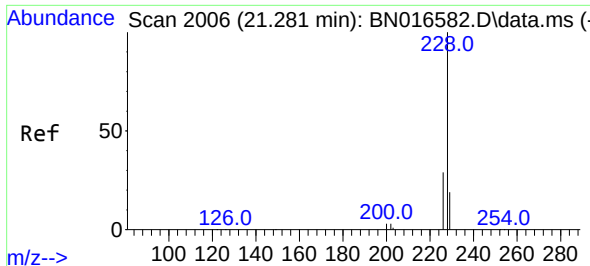

#33
Chrysene
Concen: 5.162 ng
RT: 21.280 min Scan# 2006
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 1900589
Ion Ratio Lower Upper
228 100
226 29.0 23.4 35.0
229 20.2 15.7 23.5

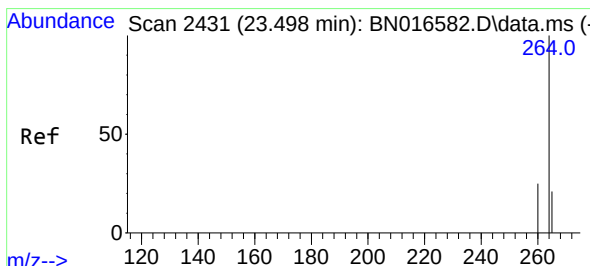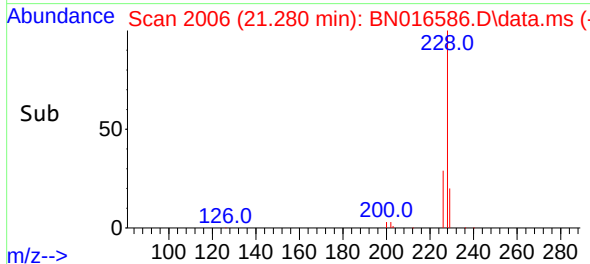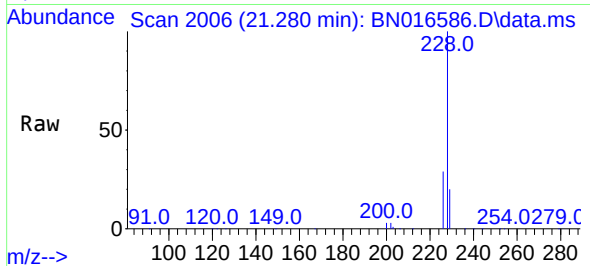

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.498 min Scan# 2431
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:264 Resp: 123329
Ion Ratio Lower Upper
264 100
260 24.5 19.7 29.5
265 23.2 18.9 28.3


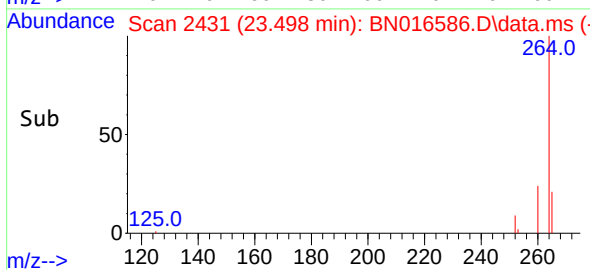

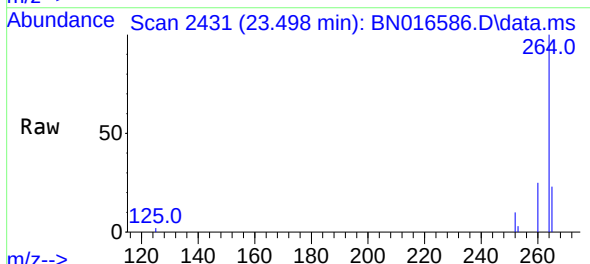




#36
Indeno(1,2,3-cd)pyrene
Concen: 6.144 ng
RT: 25.788 min Scan# 3100
Delta R.T. 0.003 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:276 Resp: 2416229
Ion Ratio Lower Upper
276 100
138 25.4 21.1 31.7
277 25.1 20.0 30.0



#37
Benzo(b)fluoranthene
Concen: 5.021 ng
RT: 22.820 min Scan# 2233
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:252 Resp: 2067638
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.6
125 10.2 8.2 12.2









#38
Benzo(k)fluoranthene
Concen: 4.866 ng
RT: 22.865 min Scan# 2246
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 1952527
Ion Ratio Lower Upper
252 100
253 22.2 18.2 27.2
125 10.4 11.0 16.4#

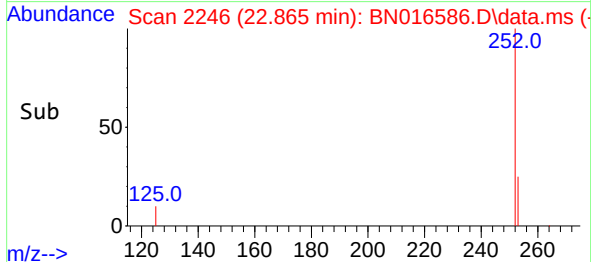

#39
Benzo(a)pyrene
Concen: 5.063 ng
RT: 23.399 min Scan# 2402
Delta R.T. -0.000 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:252 Resp: 1912352
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.6
125 11.2 9.2 13.8


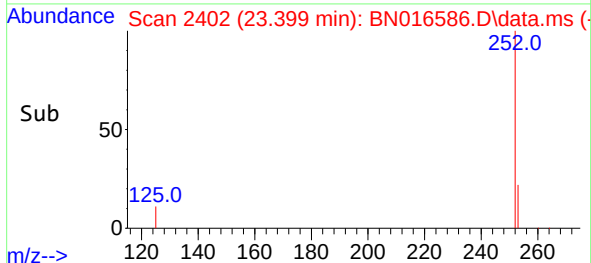
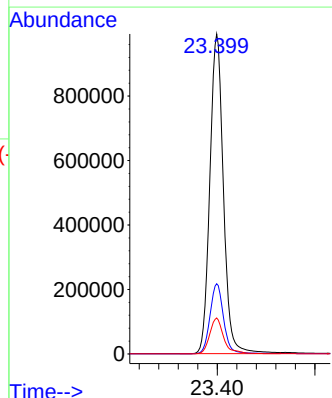
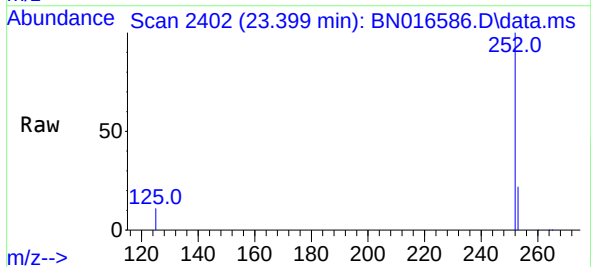




#40
Dibenzo(a,h)anthracene
Concen: 7.302 ng
RT: 25.809 min Scan# 3106
Delta R.T. 0.003 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:278 Resp: 1995307
Ion Ratio Lower Upper
278 100
139 16.5 15.6 23.4
279 23.7 19.0 28.4



#41
Benzo(g,h,i)perylene
Concen: 5.949 ng
RT: 26.483 min Scan# 3303
Delta R.T. 0.003 min
Lab File: BN016586.D
Acq: 29 Sep 2021 22:07

Tgt Ion:276 Resp: 2127332
Ion Ratio Lower Upper
276 100
277 23.9 19.0 28.6
138 21.7 17.5 26.3

