
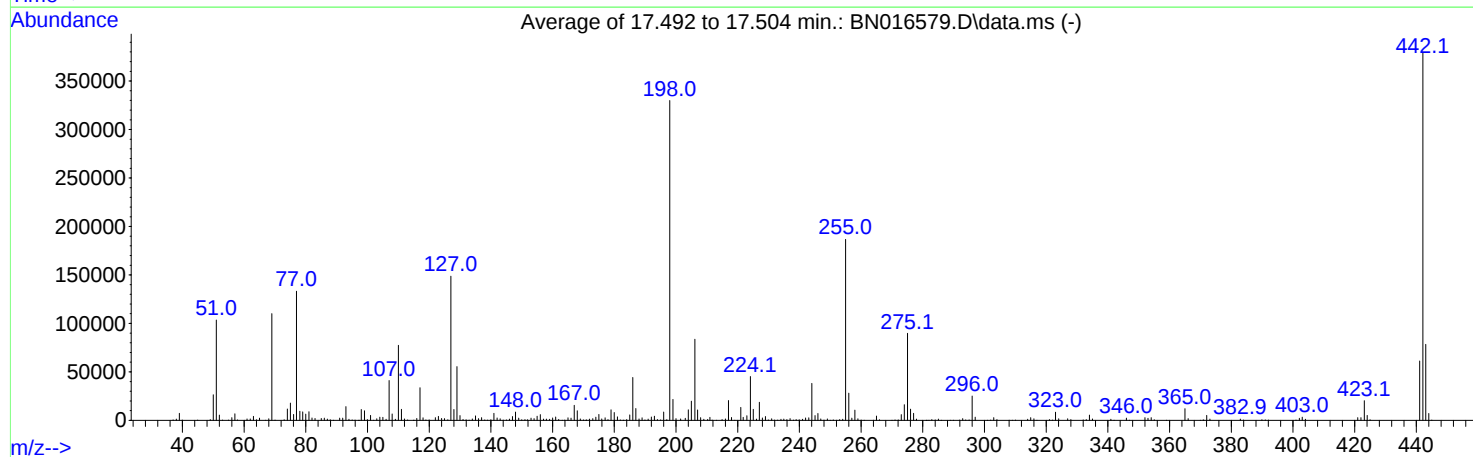


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093021\
 Data File : BN016579.D
 Acq On : 29 Sep 2021 17:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN093021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 30 02:08:37 2021

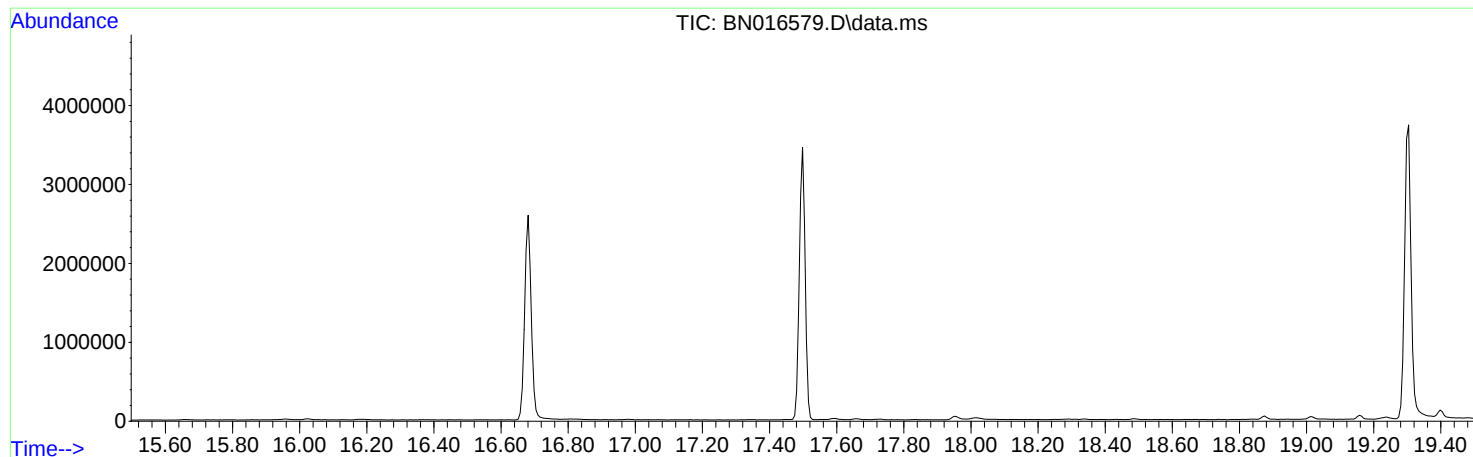




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	103501	PASS
68	69	0.00	2	1.6	1737	PASS
69	198	0.00	100	33.4	110025	PASS
70	69	0.00	2	0.3	383	PASS
127	198	10	80	45.1	148632	PASS
197	198	0.00	2	0.2	547	PASS
198	198	100	100	100.0	329856	PASS
199	198	5	9	6.6	21688	PASS
275	198	10	60	27.2	89717	PASS
365	198	1	100	3.6	11989	PASS
441	198	0.01	100	18.5	61165	PASS
442	442	50	100	100.0	379413	PASS
443	442	15	24	20.7	78365	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093021\
 Data File : BN016579.D
 Acq On : 29 Sep 2021 17:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 06:34:49 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 28 17:48:03 2021
 Response via : Initial Calibration

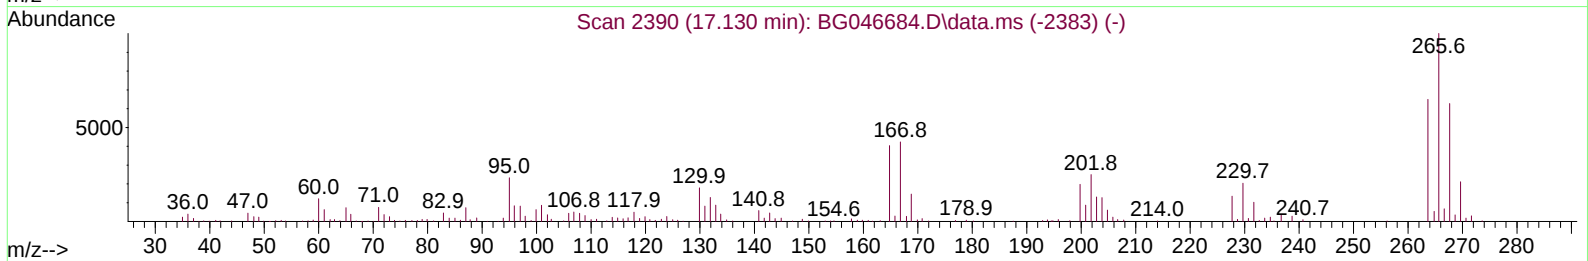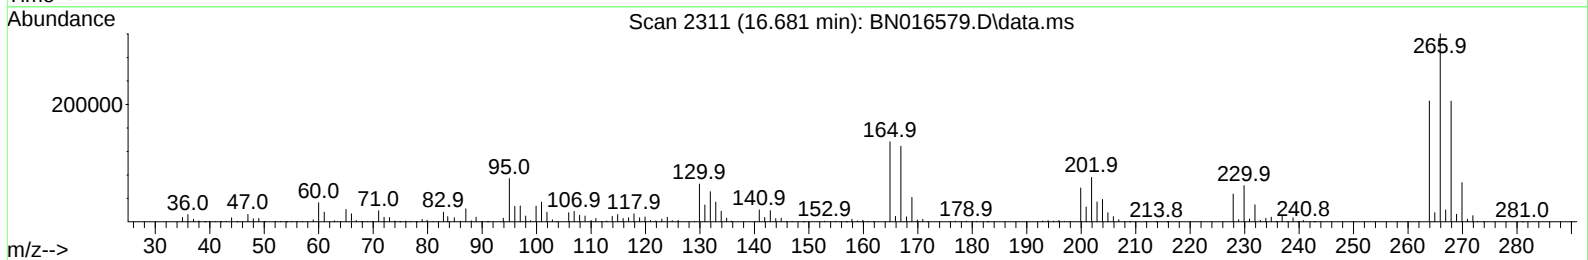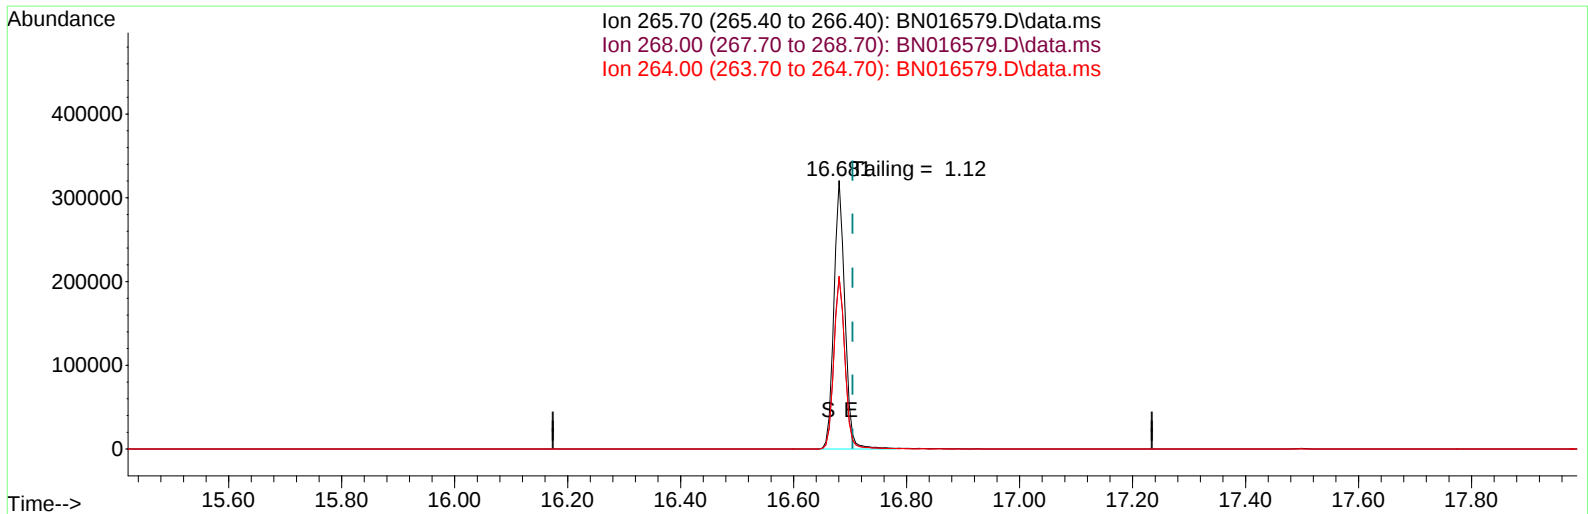

TIC: BN016579.D\data.ms

(70) Pentachlorophenol (C)

16.681min (-0.023) 27552.76 ng




response 434184

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	64.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093021\
Data File : BN016579.D
Acq On : 29 Sep 2021 17:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 30 06:34:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 28 17:48:03 2021
Response via : Initial Calibration

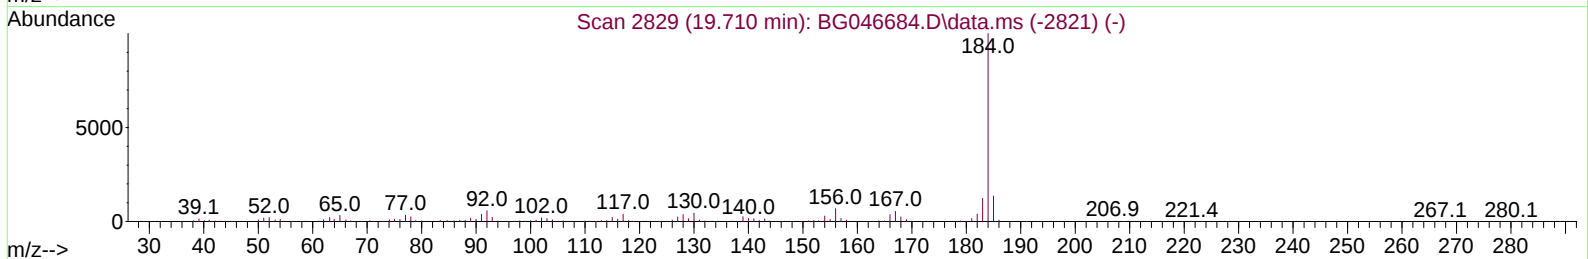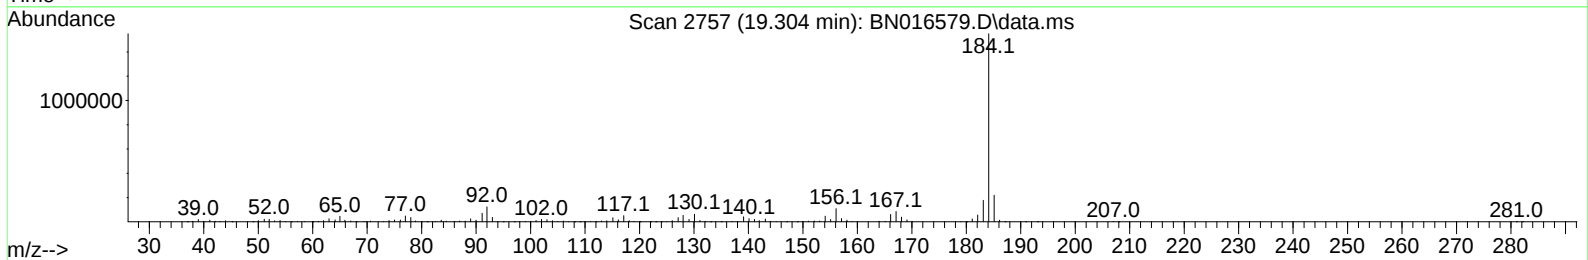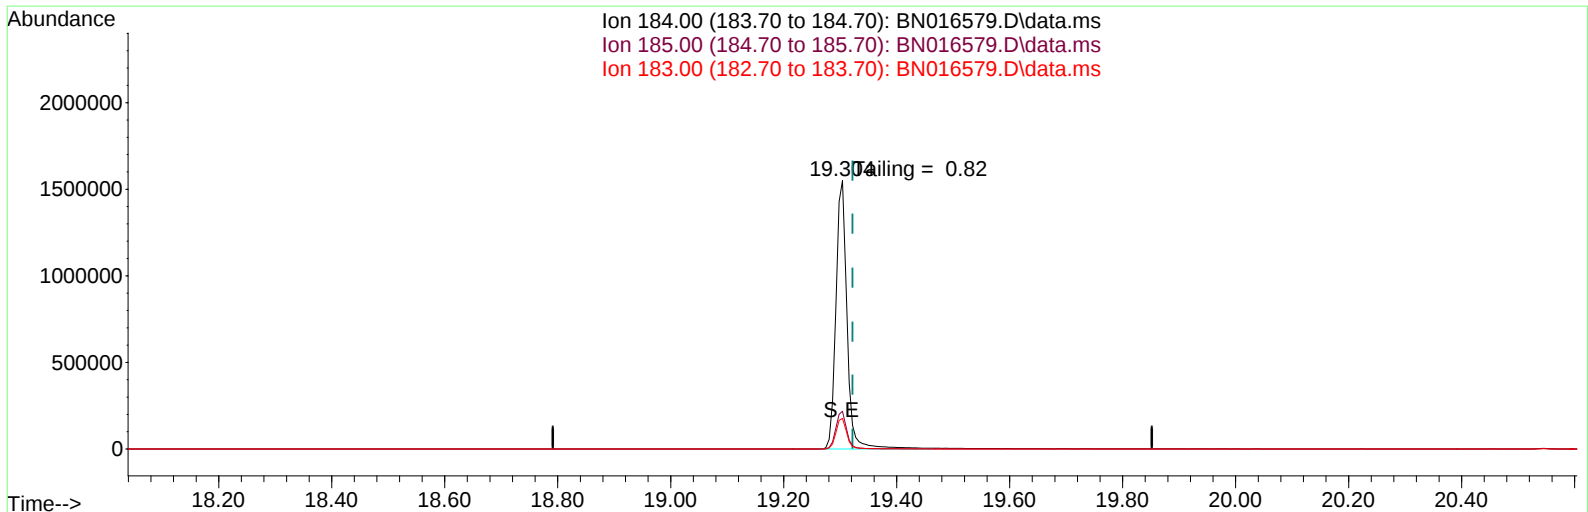

TIC: BN016579.D\data.ms

(77) Benzidine

19.304min (-0.018) 0.00 ng

response 2121026

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.11
183.00	13.20	11.41
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/30/2021	BNA_N	<u>BN016579.D</u>
Compound Name	Response	Retention Time
DDT	1027807	20.545
DDD	5508	20.157
DDE	0	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5508	1033315	0.53

Instrument :
BNA_N
ClientSampleId :
DFTPP