
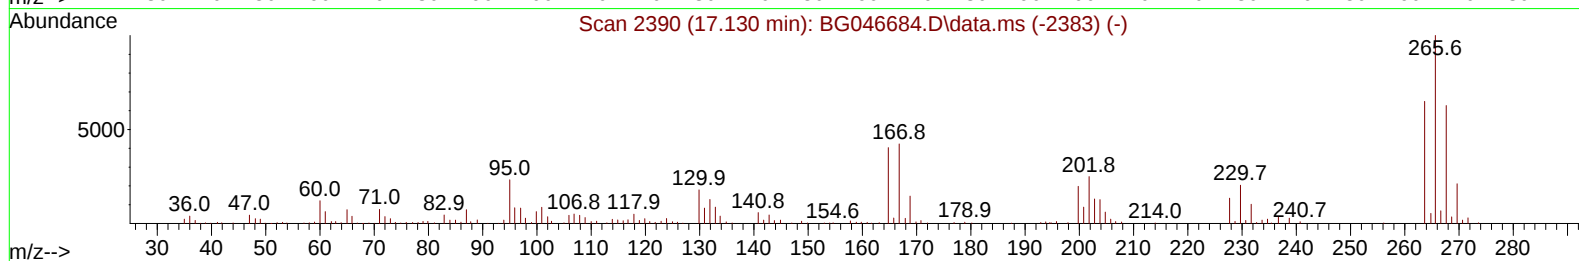
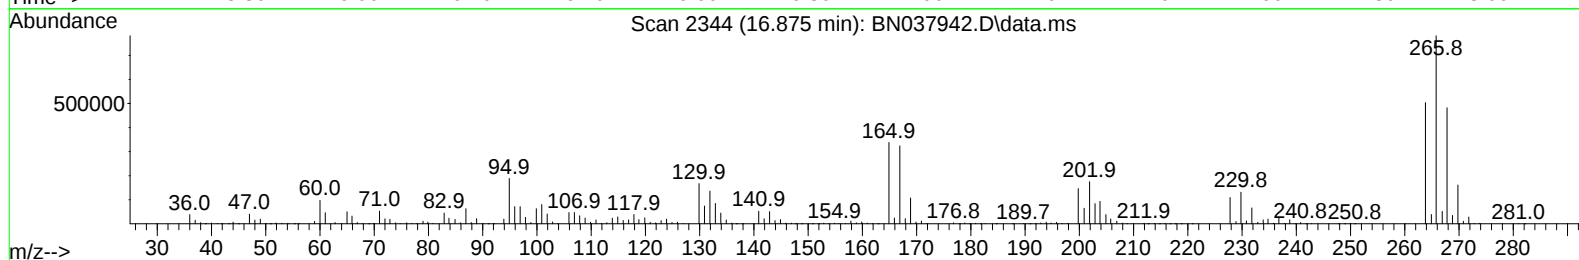


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037942.D
Acq On : 30 Sep 2025 11:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 13:14:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

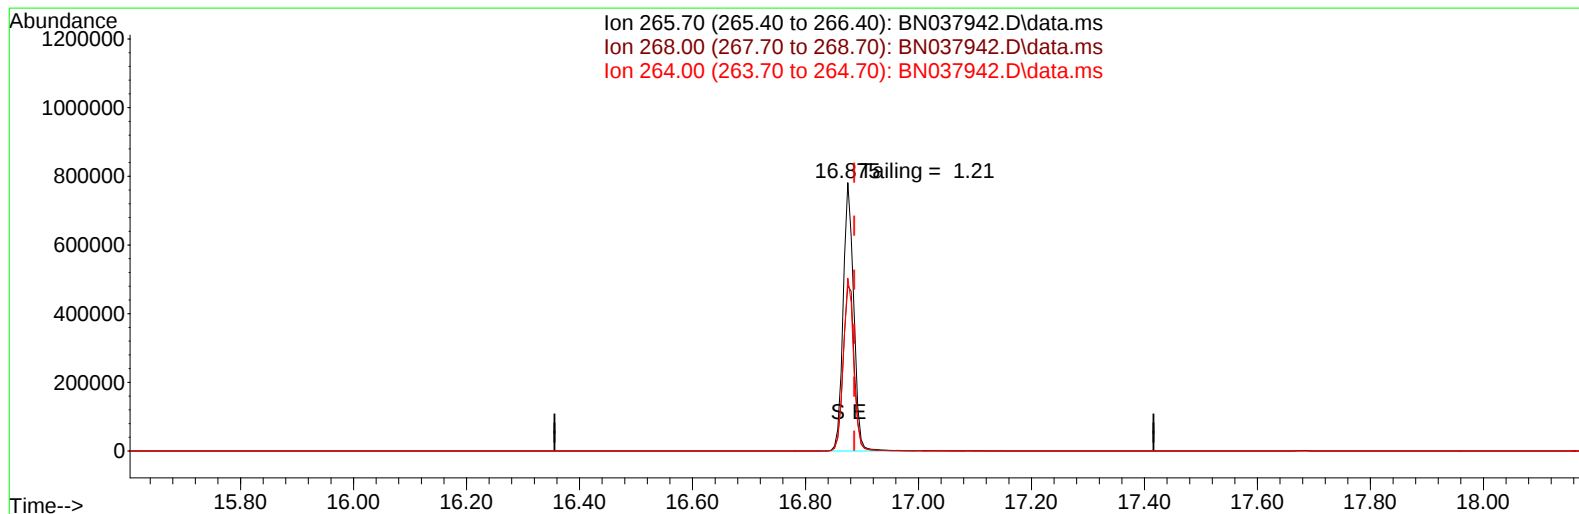

TIC: BN037942.D\data.ms

(70) Pentachlorophenol (C)




16.875min (-0.011) 31430.20 ng

response 1011044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.70
264.00	61.60	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037942.D
Acq On : 30 Sep 2025 11:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 13:14:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

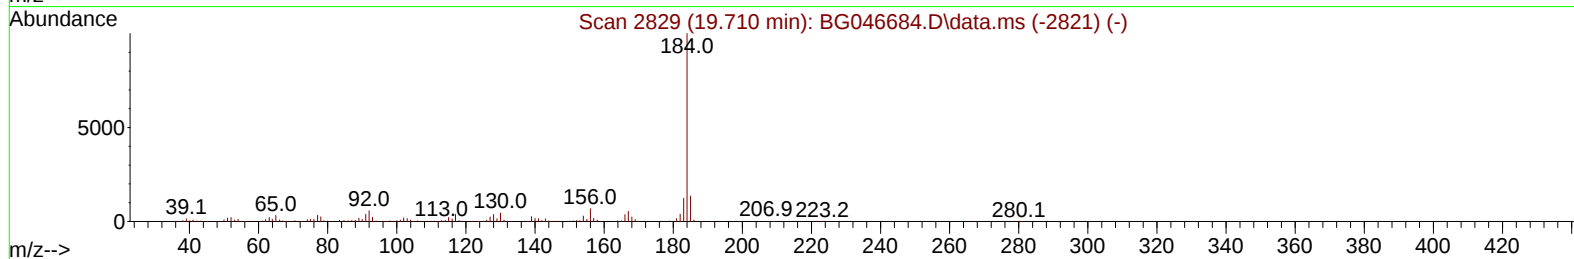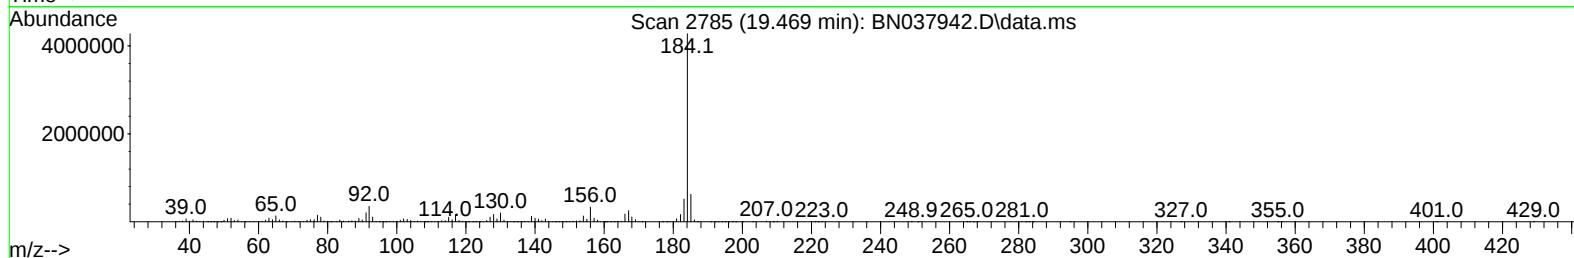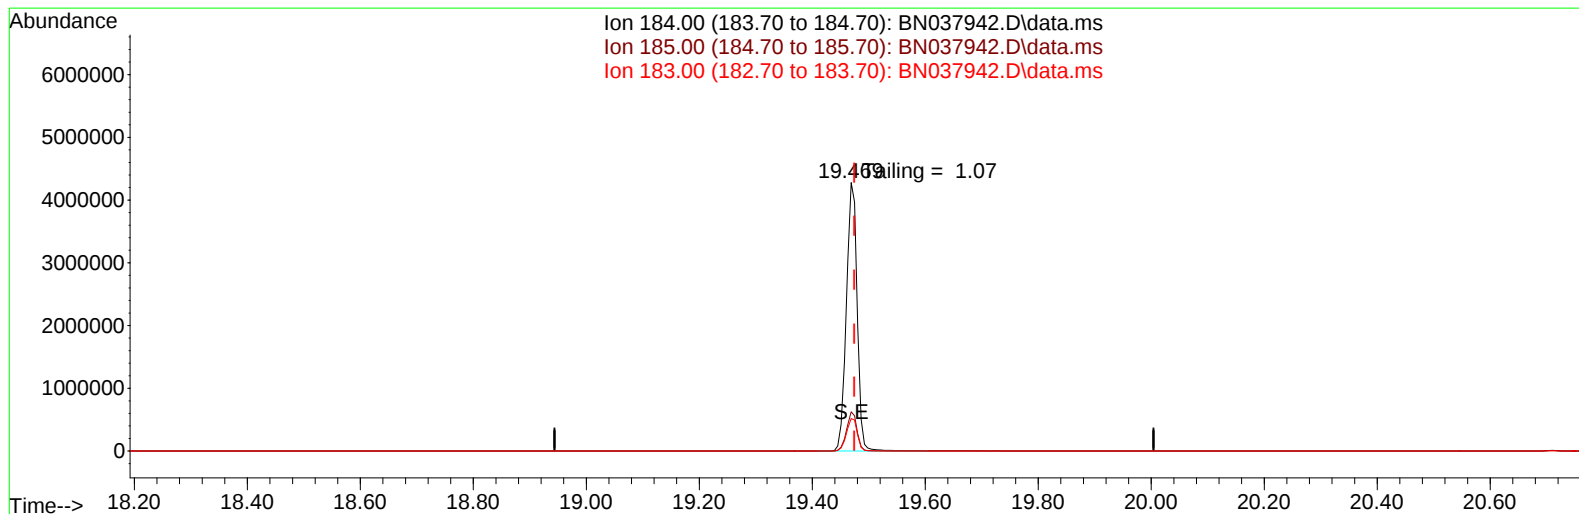

TIC: BN037942.D\data.ms

(77) Benzidine

19.469min (-0.005) 0.00 ng

response 5670270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.12
0.00	0.00	0.00