
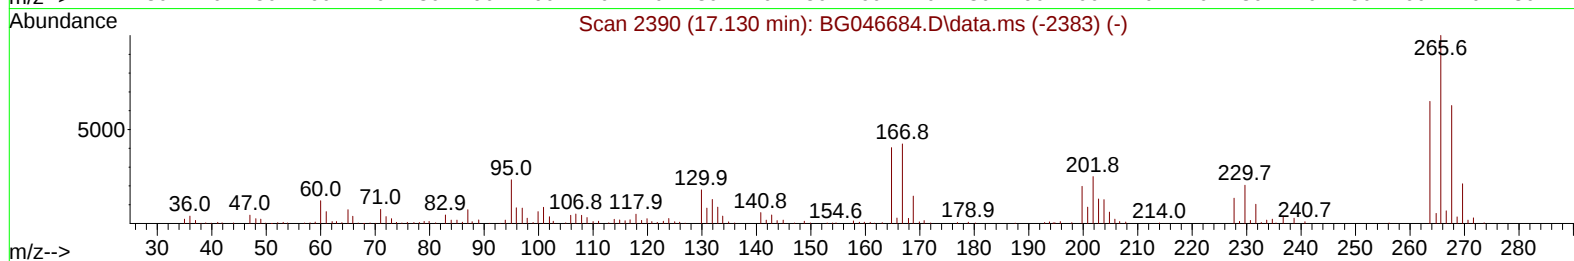
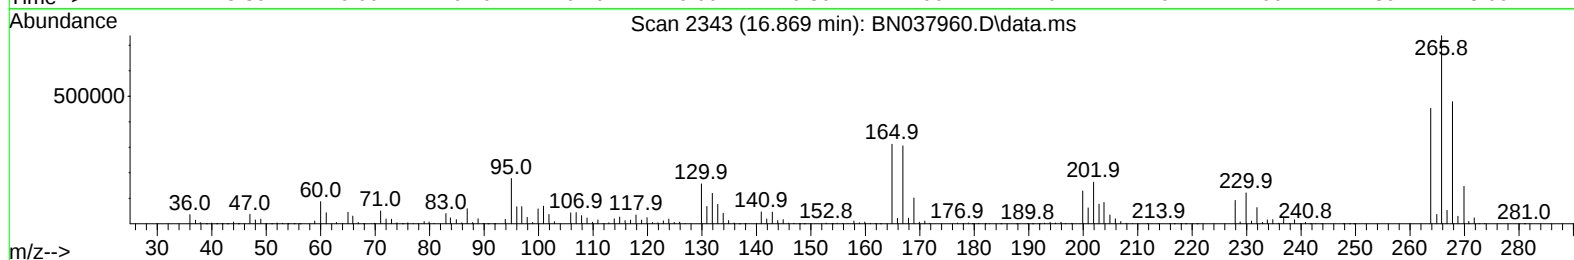


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037960.D
Acq On : 01 Oct 2025 00:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 01:44:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

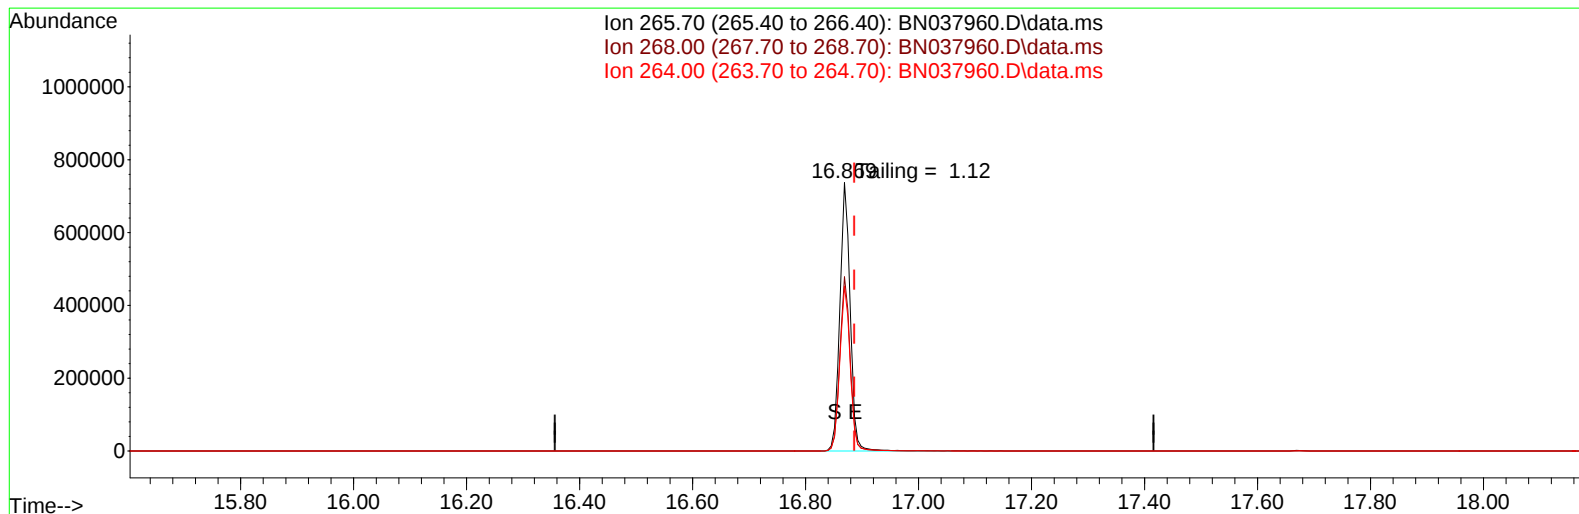

TIC: BN037960.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.017) 27797.15 ng

response 931043

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093025\
Data File : BN037960.D
Acq On : 01 Oct 2025 00:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 01:44:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

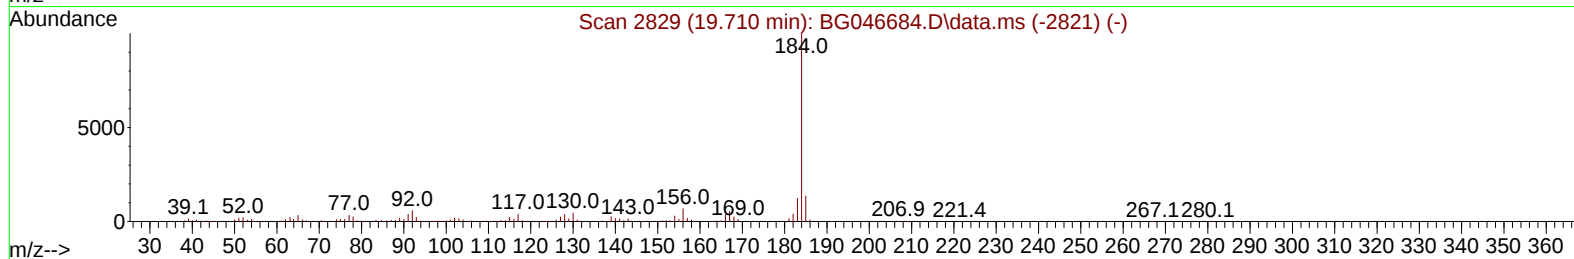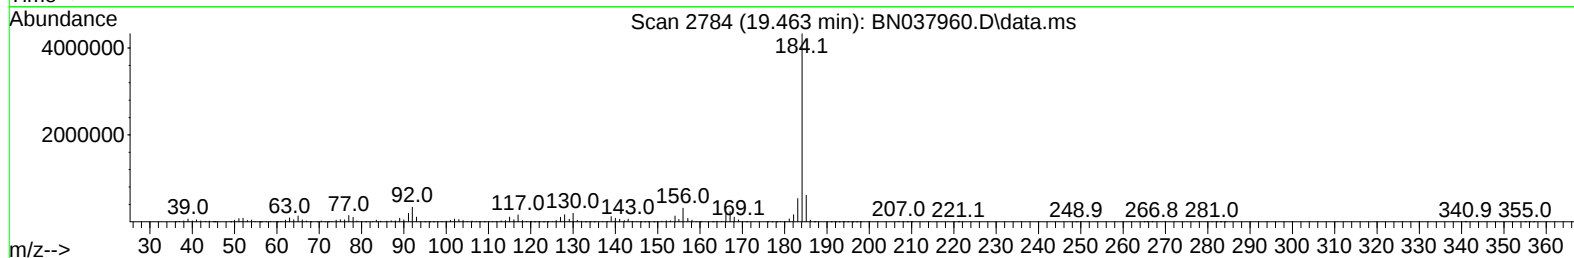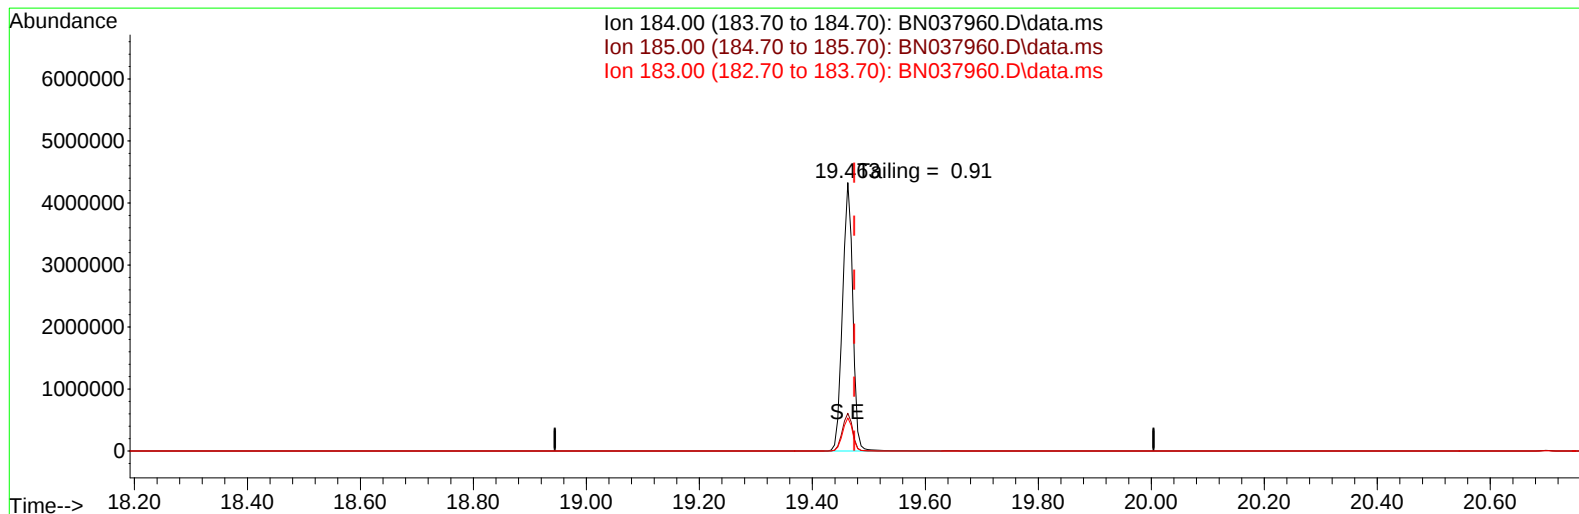

TIC: BN037960.D\data.ms

(77) Benzidine**19.463min (-0.011) 0.00 ng****response 5415438**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.37
0.00	0.00	0.00