

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100118\
 Data File : BN002885.D
 Acq On : 01 Oct 2018 18:33
 Operator : MJ/SJ
 Sample : J5117-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 02 02:29:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 02 02:29:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1487	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.40	136	6185	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	3747	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	762460	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.44	264	7213	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	4564	0.51	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
9) Fluorene	15.27	166	1297	0.094	ng/ul#	20
23) Benzo(a)pyrene	23.29	252	2433	0.107	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100118\
Data File : BN002885.D
Acq On : 01 Oct 2018 18:33
Operator : MJ/SJ
Sample : J5117-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 02 02:29:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 02 02:29:03 2018
Response via : Initial Calibration




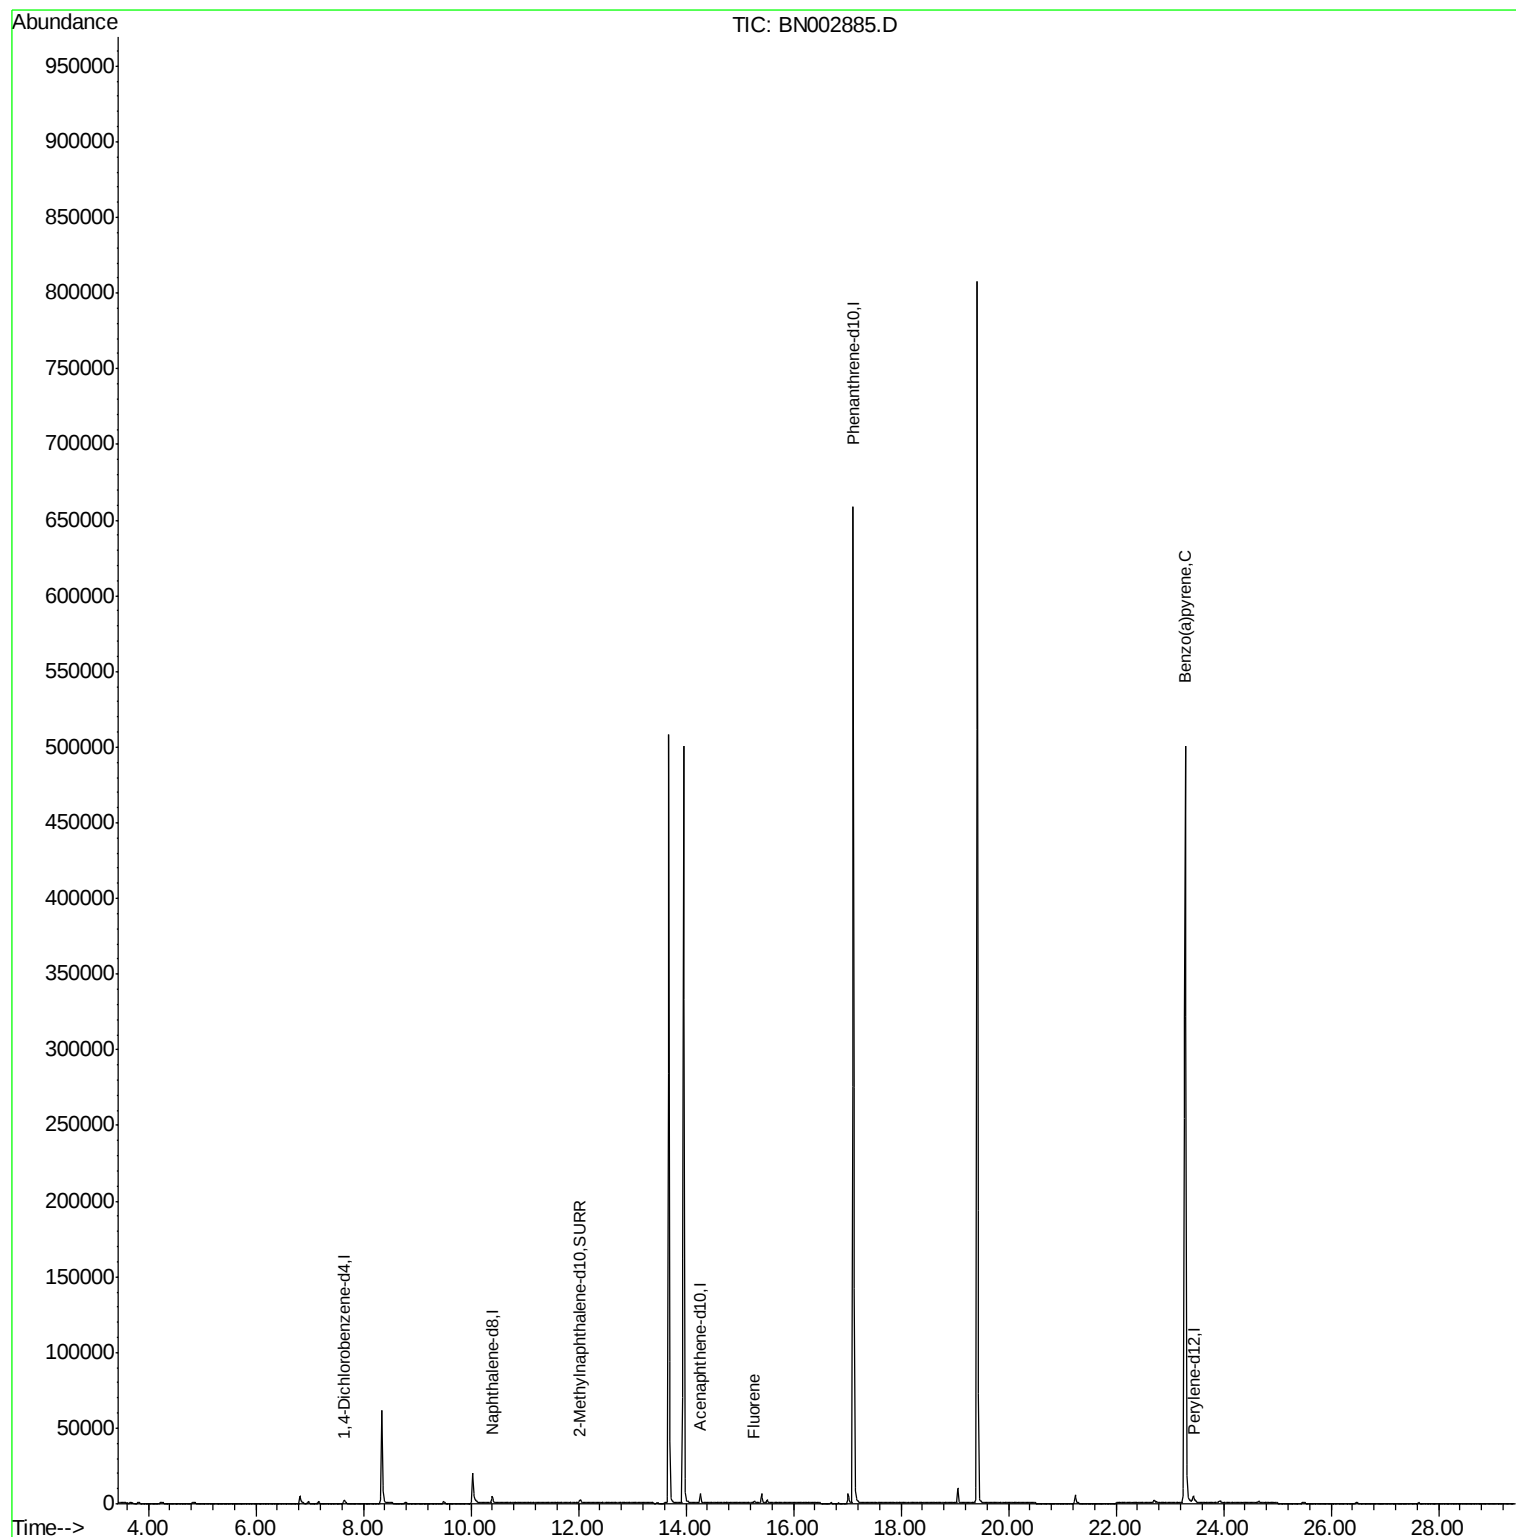


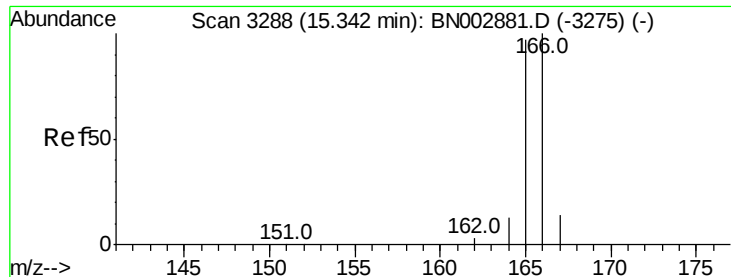

#9
Fluorene
 Concen: 0.094 ng/ul
 RT: 15.27 min Scan# 3272
 Delta R.T. -0.07 min
 Lab File: BN002885.D
 Acq: 01 Oct 2018 18:33

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 1297
 Ion Ratio Lower Upper
 166 100
 165 8.6 73.4 110.2#
 167 37.2 14.6 22.0#

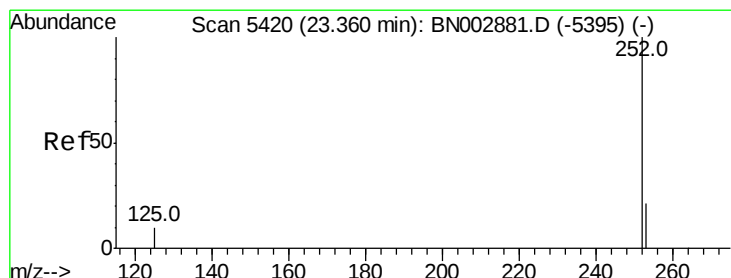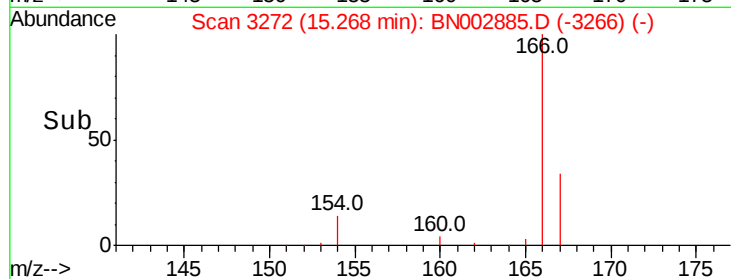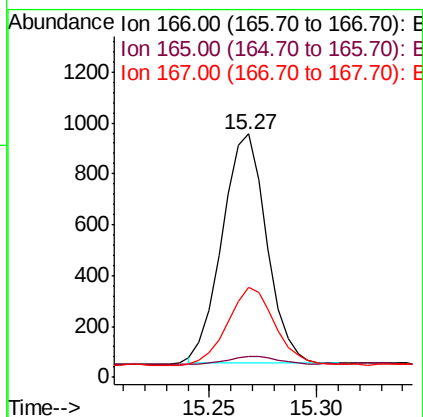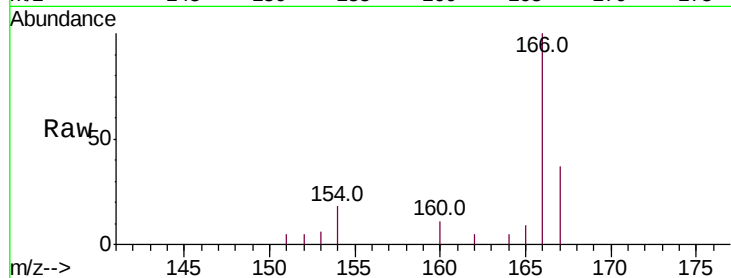

#23
Benzo(a)pyrene
 Concen: 0.107 ng/ul
 RT: 23.29 min Scan# 5395
 Delta R.T. -0.07 min
 Lab File: BN002885.D
 Acq: 01 Oct 2018 18:33

Tgt Ion:252 Resp: 2433
 Ion Ratio Lower Upper
 252 100
 253 40.8 16.0 24.0#
 125 37.8 12.0 18.0#

