

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100118\
 Data File : BN002886.D
 Acq On : 01 Oct 2018 19:08
 Operator : MJ/SJ
 Sample : J5117-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 02 02:29:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 02 02:29:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1310	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.40	136	5395	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	3241	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	618832	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.44	264	8369	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	3418	0.44	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.26	166	984	0.083	ng/ul#	22
23) Benzo(a)pyrene	23.29	252	2488	0.094	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100118\
Data File : BN002886.D
Acq On : 01 Oct 2018 19:08
Operator : MJ/SJ
Sample : J5117-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 02 02:29:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 02 02:29:03 2018
Response via : Initial Calibration




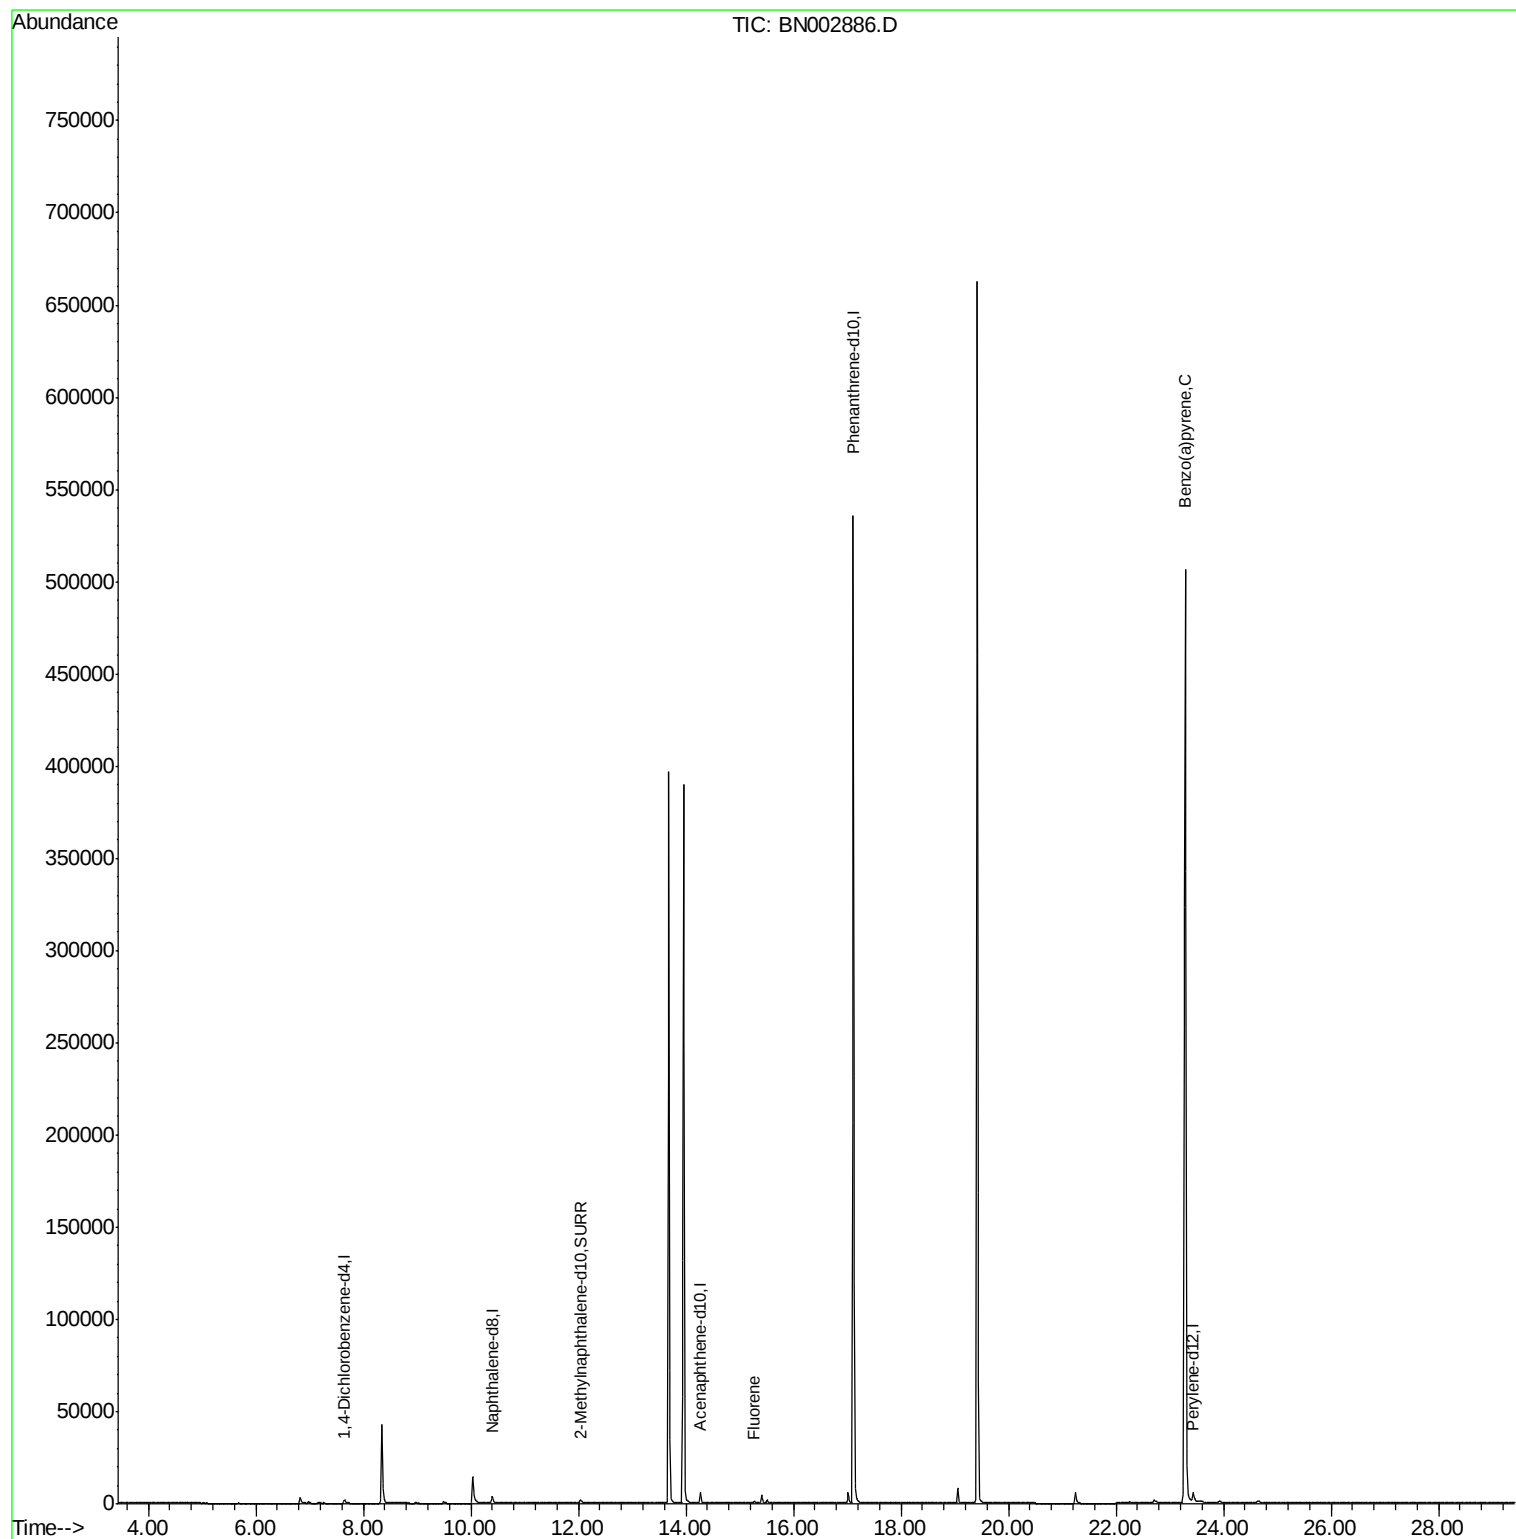


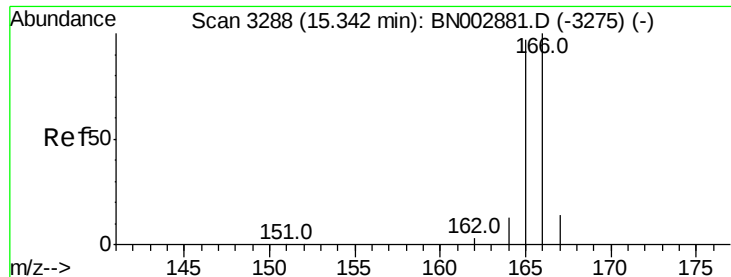

#9
Fluorene
Concen: 0.083 ng/ul
RT: 15.26 min Scan# 3271
Delta R.T. -0.08 min
Lab File: BN002886.D
Acq: 01 Oct 2018 19:08

Instrument :
BNA_N
ClientSampleId :

Tot Ion:166 Resp: 984
Ion Ratio Lower Upper
166 100
165 9.9 73.4 110.2#
167 34.4 14.6 22.0#

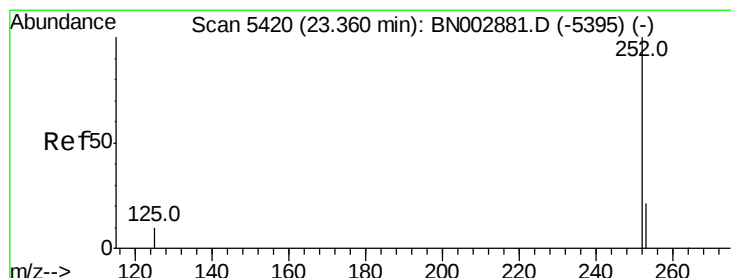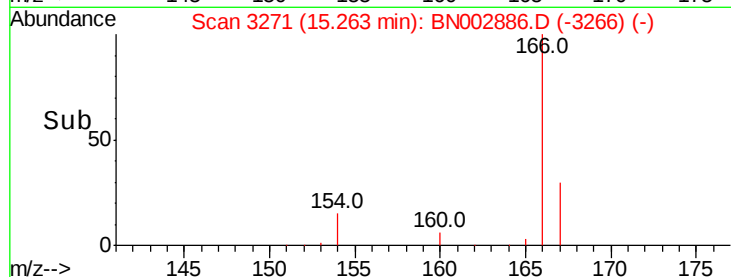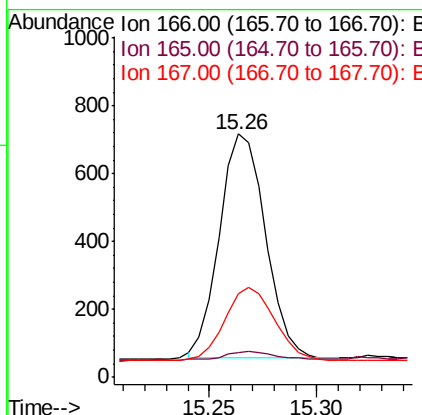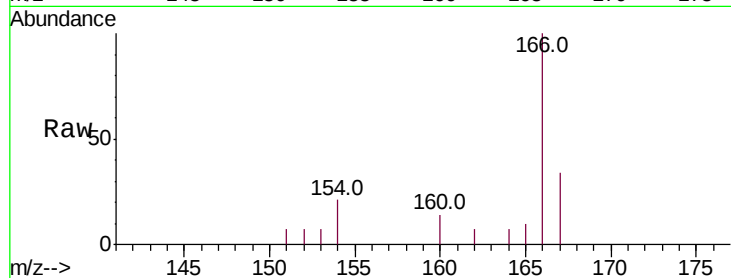

#23
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.29 min Scan# 5395
Delta R.T. -0.07 min
Lab File: BN002886.D
Acq: 01 Oct 2018 19:08

Tgt Ion:252 Resp: 2488
Ion Ratio Lower Upper
252 100
253 39.1 16.0 24.0#
125 35.6 12.0 18.0#

