


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
Data File : BN002883.D
Acq On : 01 Oct 2018 17:23
Operator : MJ/SJ
Sample : J5117-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC86

Manual Integrations
APPROVED

Sohil
10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:47:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 01 14:40:21 2018
Response via : Initial Calibration

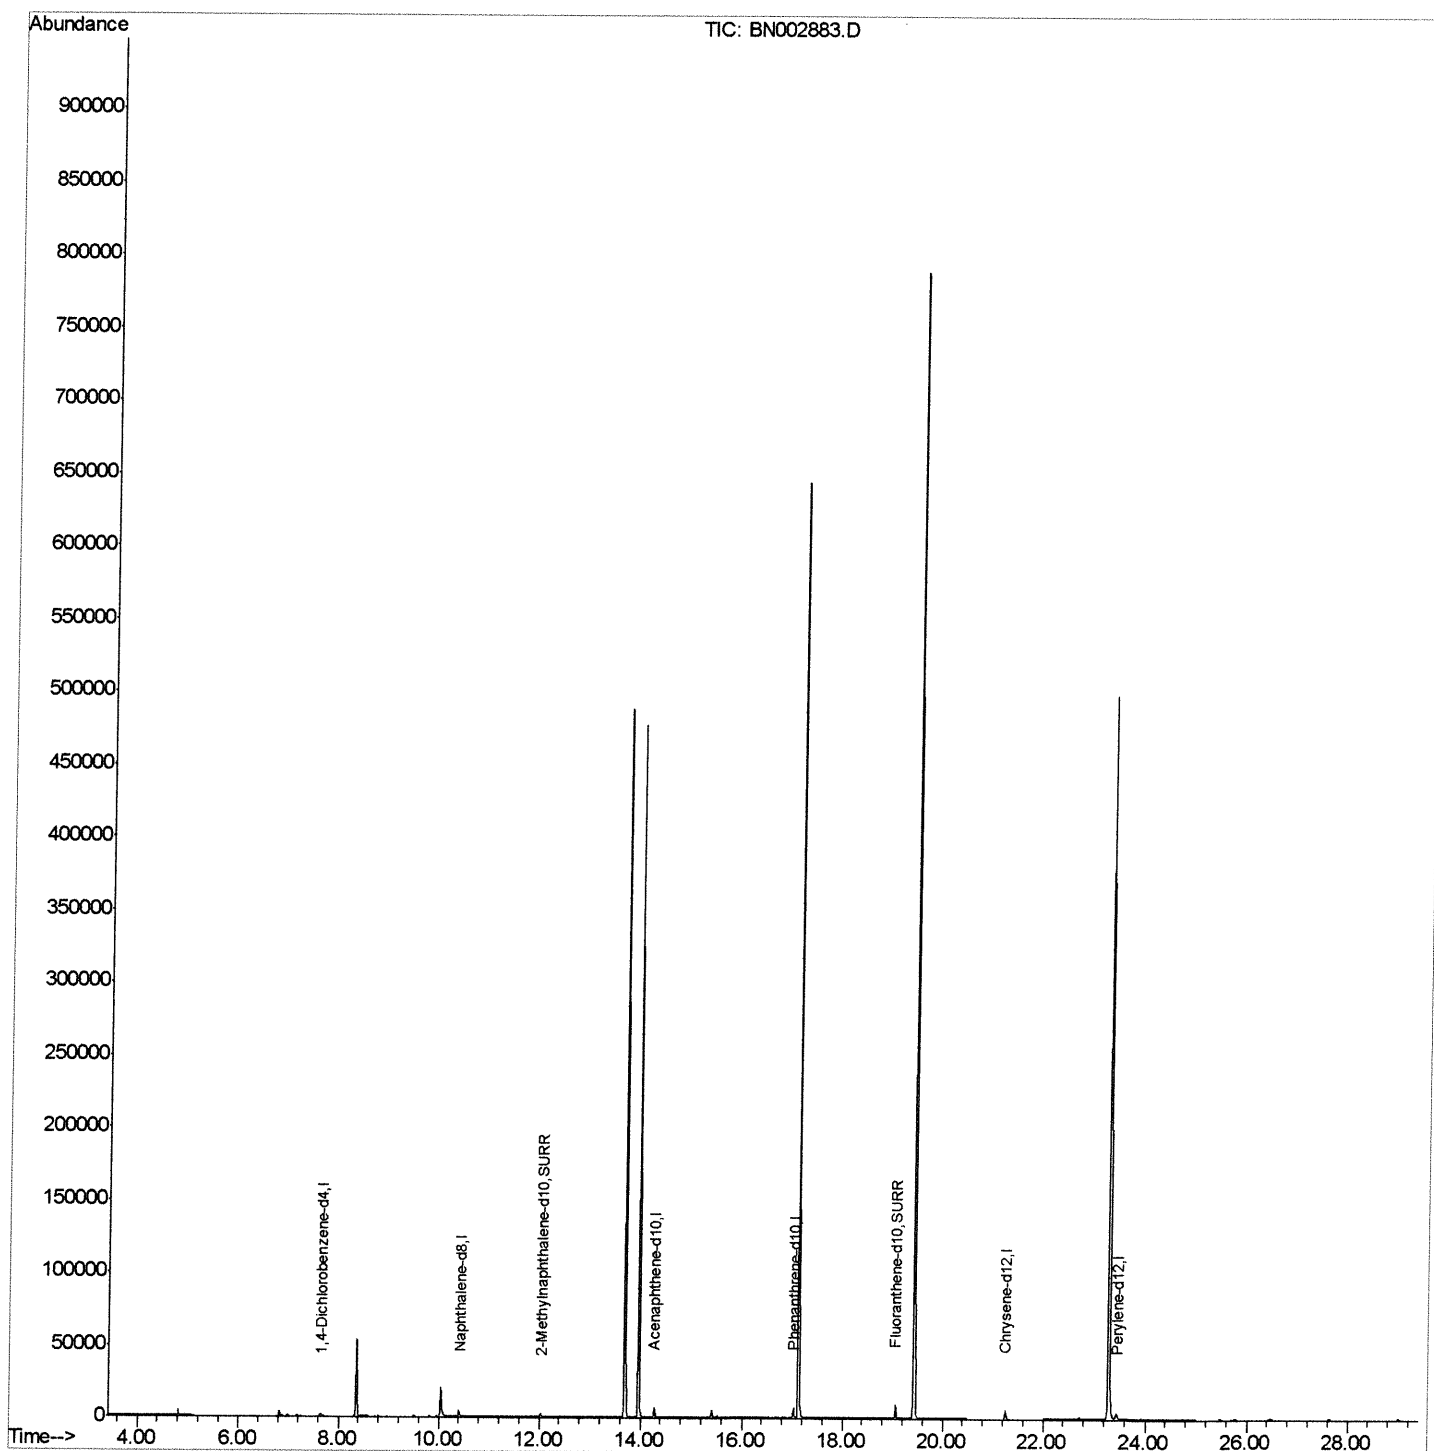

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
 Data File : BN002883.D
 Acq On : 01 Oct 2018 17:23
 Operator : MJ/SJ
 Sample : J5117-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC86

Manual Integrations
 APPROVED

Sohil
 10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:45:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 01 14:40:21 2018
 Response via : Initial Calibration

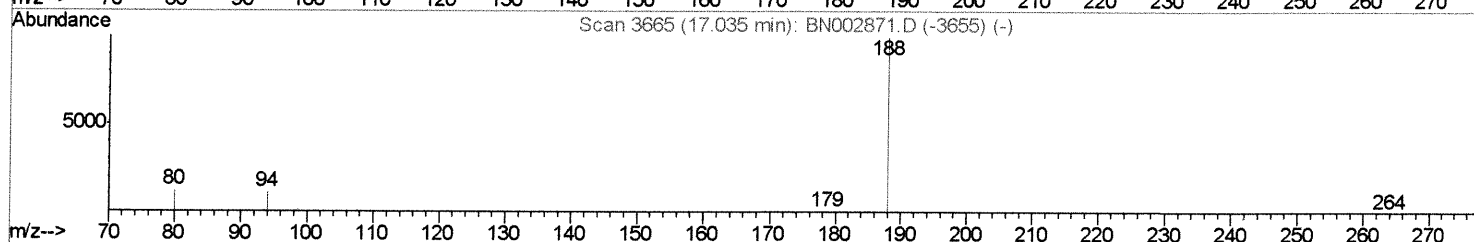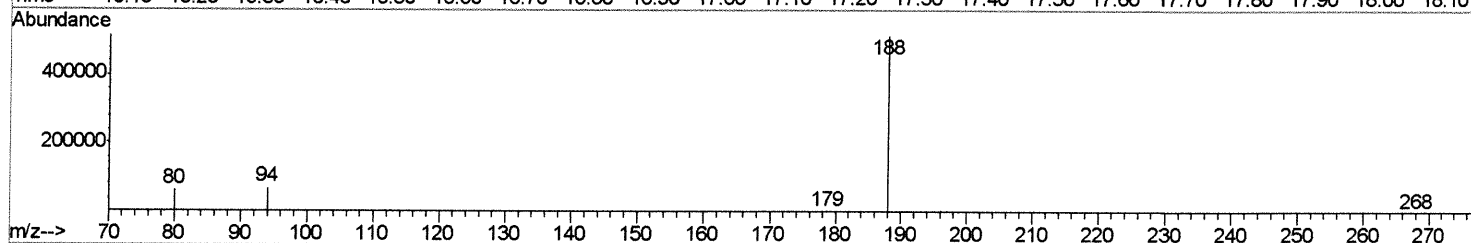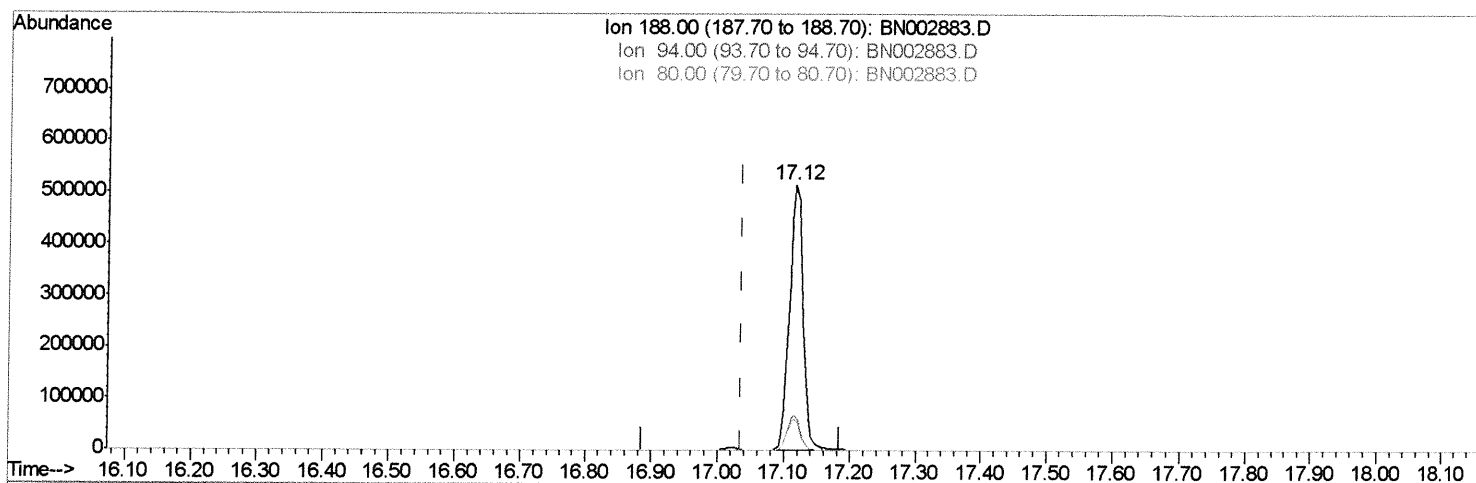

TIC: BN002883.D

(10) Phenanthrene-d10 (I)
 17.116min (+0.080) 0.40ng/ul
 response 738293

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.12
80.00	11.80	12.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
 Data File : BN002883.D
 Acq On : 01 Oct 2018 17:23
 Operator : MJ/SJ
 Sample : J5117-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC86

Manual Integrations
 APPROVED

Sohil
 10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:45:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 01 14:40:21 2018
 Response via : Initial Calibration

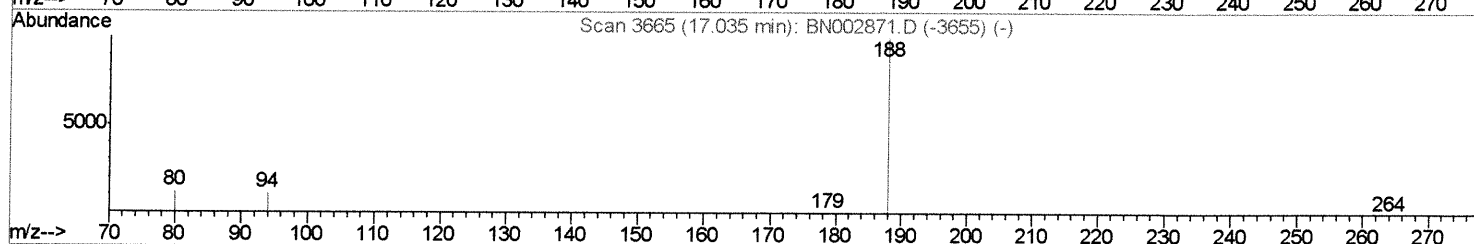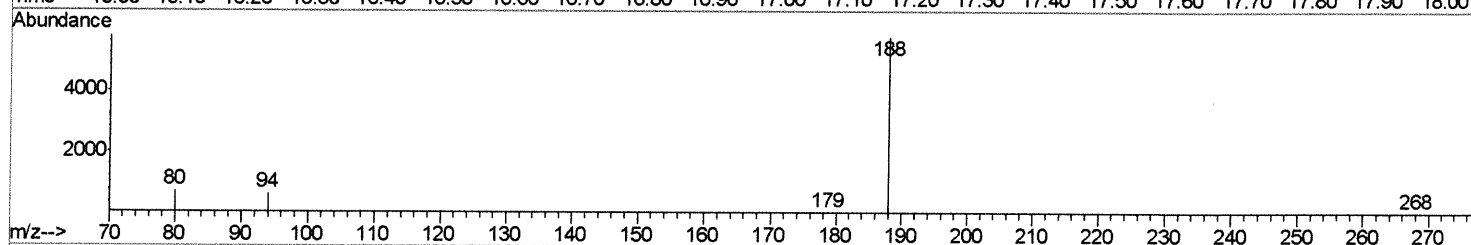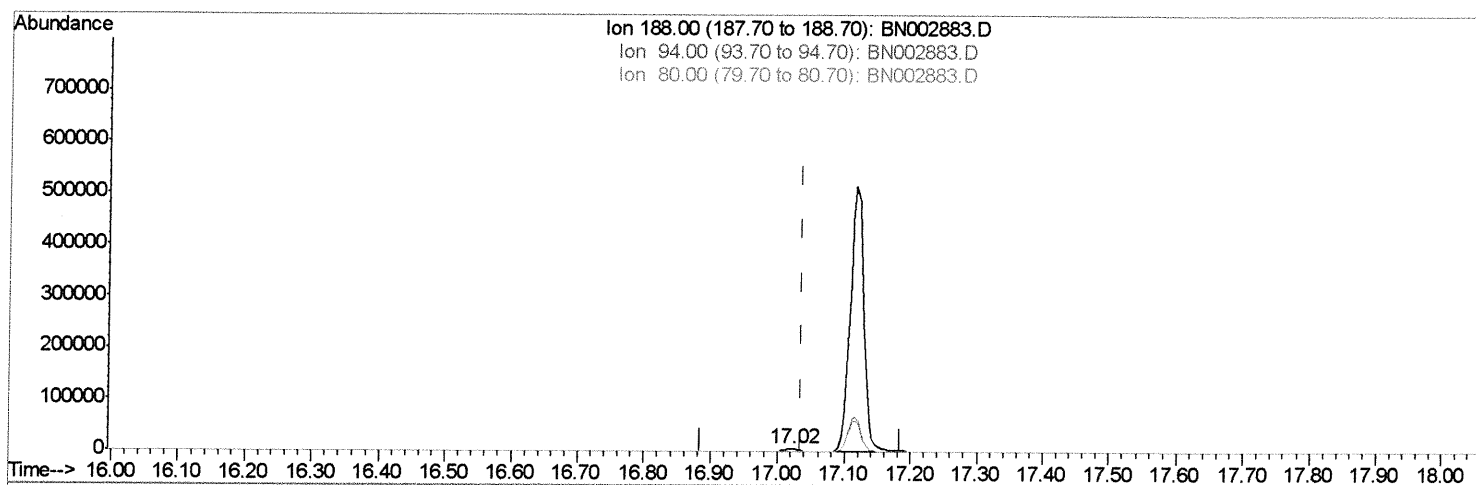

TIC: BN002883.D

(10) Phenanthrene-d10 (I)

17.023min (-0.013) 0.40ng/ul m

SJ 10/12/18

response 8162

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.15
80.00	11.80	12.37
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
 Data File : BN002883.D
 Acq On : 01 Oct 2018 17:23
 Operator : MJ/SJ
 Sample : J5117-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC86

Manual Integrations
 APPROVED

Sohil
 10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:46:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 01 14:40:21 2018
 Response via : Initial Calibration

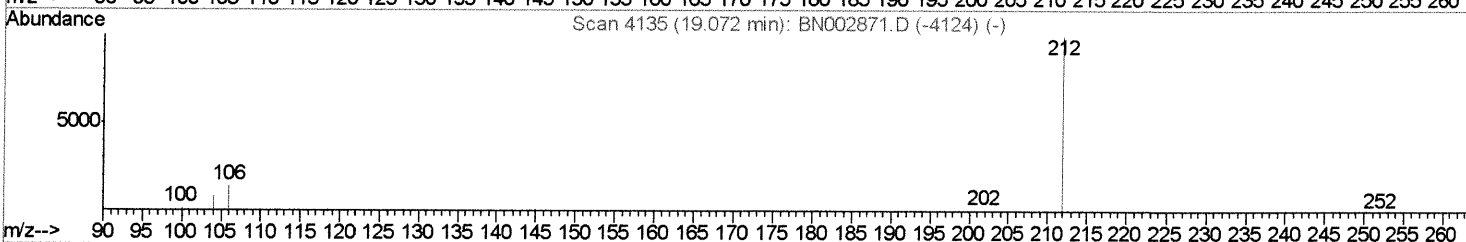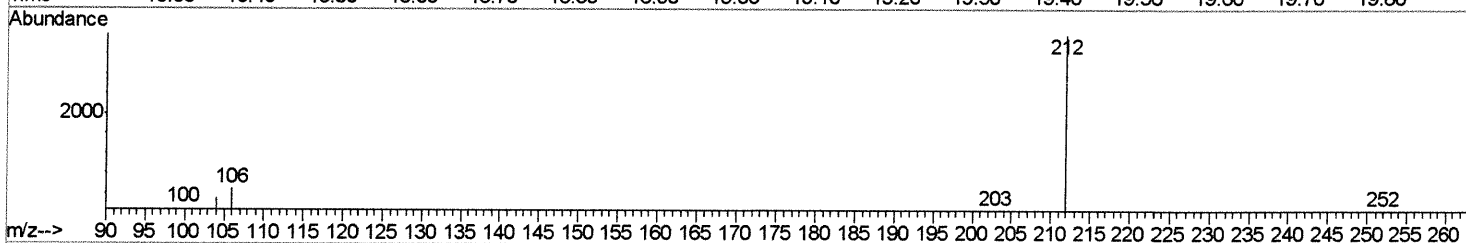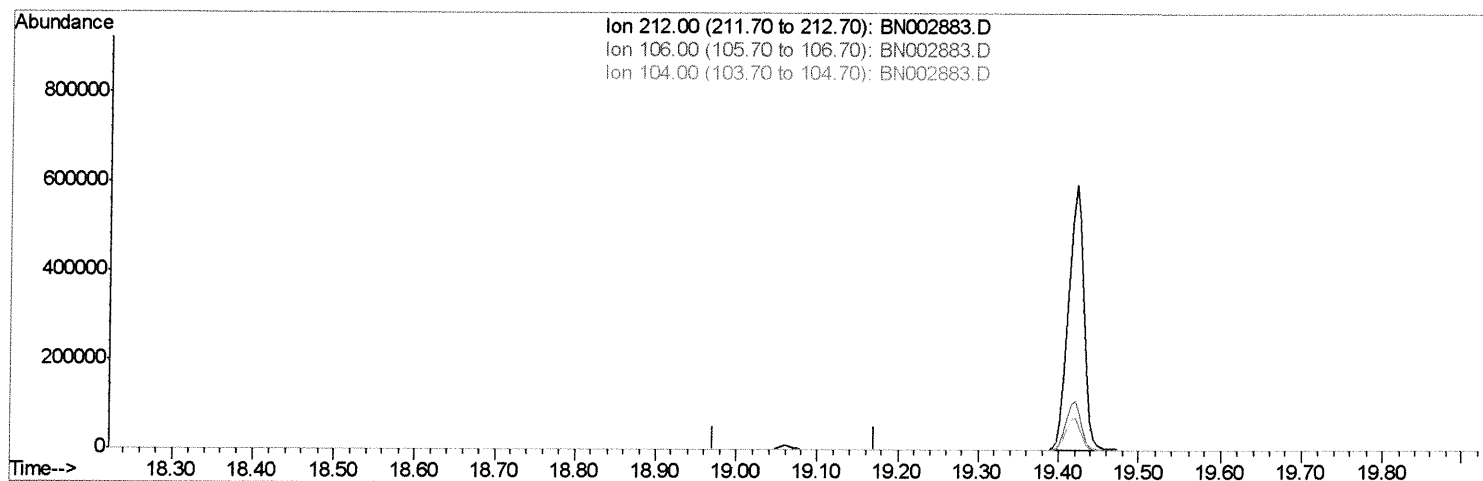

TIC: BN002883.D

(14) Fluoranthene-d10 (SURRE)

19.072min (-19.072) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
 Data File : BN002883.D
 Acq On : 01 Oct 2018 17:23
 Operator : MJ/SJ
 Sample : J5117-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC86

Manual Integrations
 APPROVED

Sohil
 10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:46:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 01 14:40:21 2018
 Response via : Initial Calibration

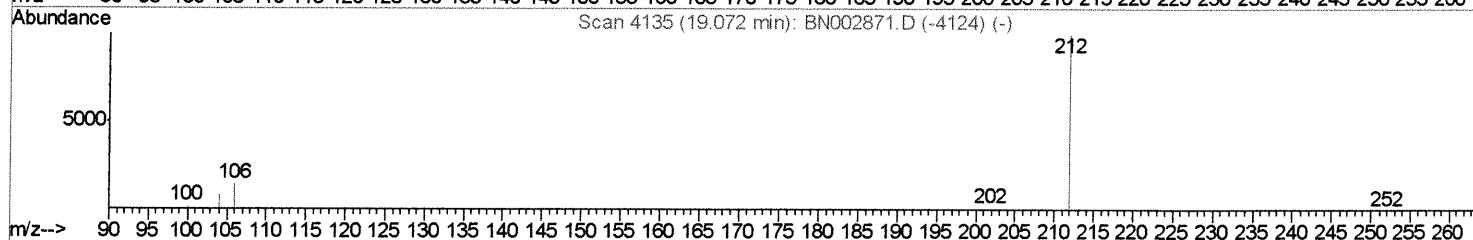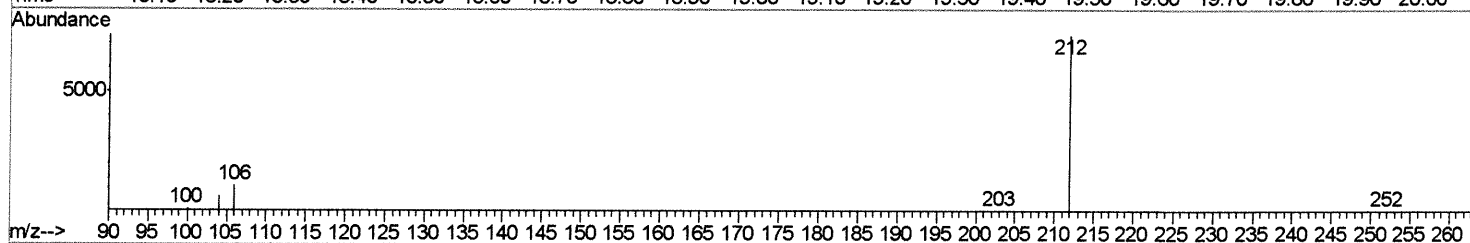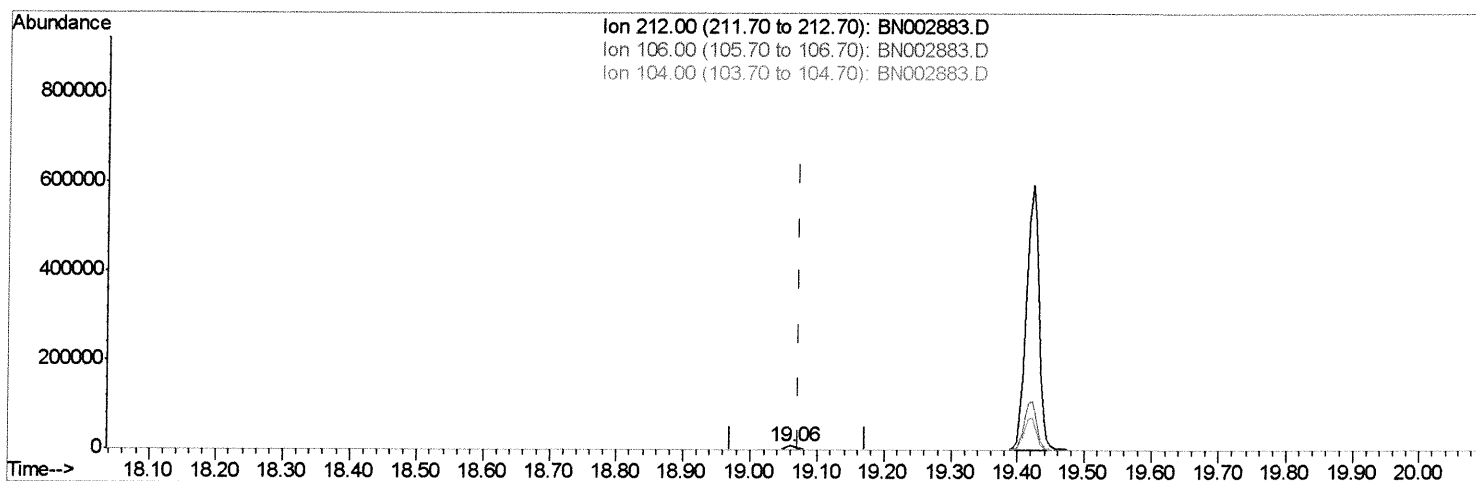

TIC: BN002883.D

(14) Fluoranthene-d10 (SURR)

19.062min (-0.009) 0.49ng/ul m

SJ 10/12/18

response 10382

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
 Data File : BN002883.D
 Acq On : 01 Oct 2018 17:23
 Operator : MJ/SJ
 Sample : J5117-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC86

Manual Integrations
 APPROVED

Sohil
 10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:46:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 01 14:40:21 2018
 Response via : Initial Calibration

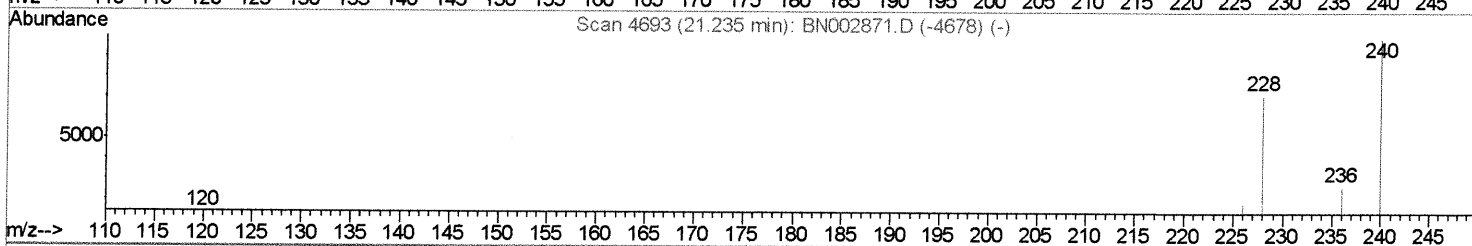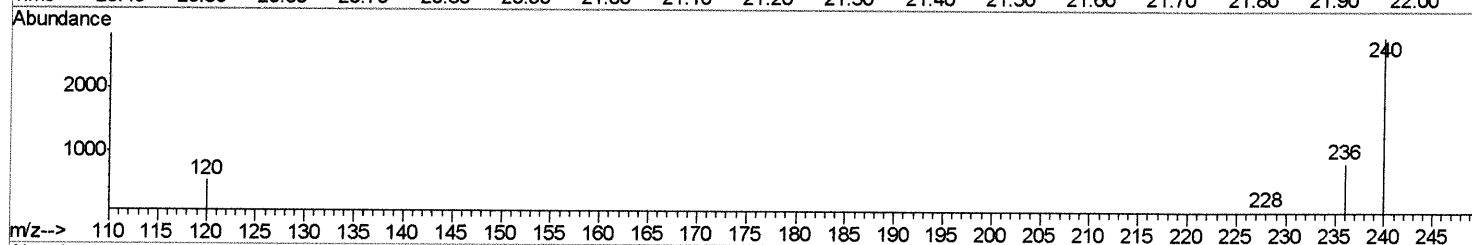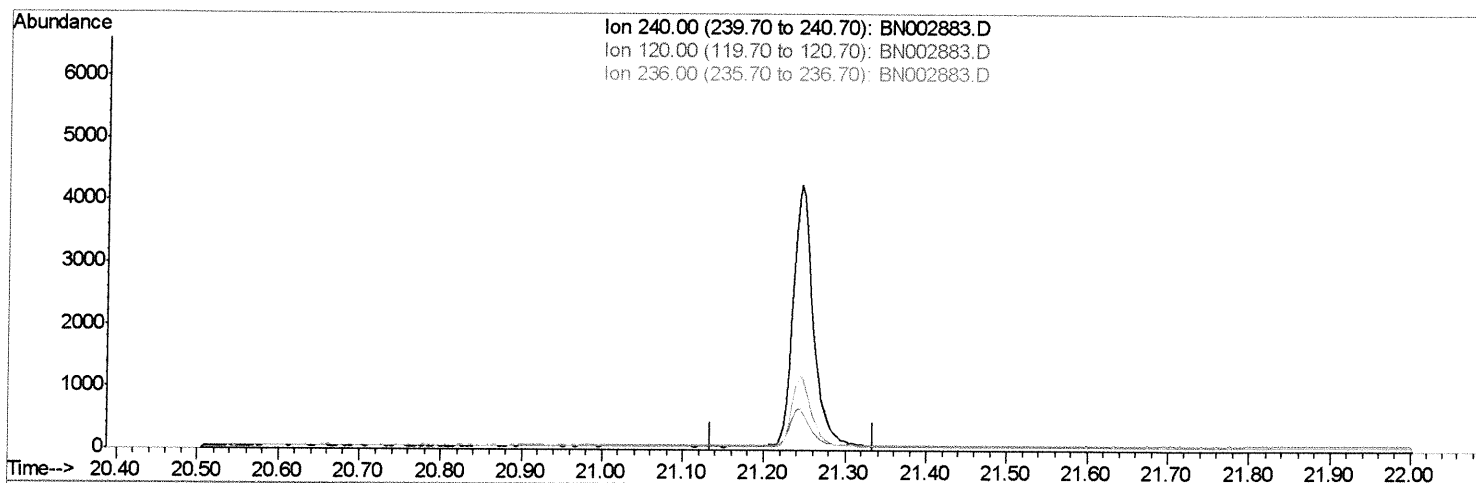

TIC: BN002883.D

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
 Data File : BN002883.D
 Acq On : 01 Oct 2018 17:23
 Operator : MJ/SJ
 Sample : J5117-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC86

Manual Integrations
 APPROVED

Sohil
 10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:46:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 01 14:40:21 2018
 Response via : Initial Calibration

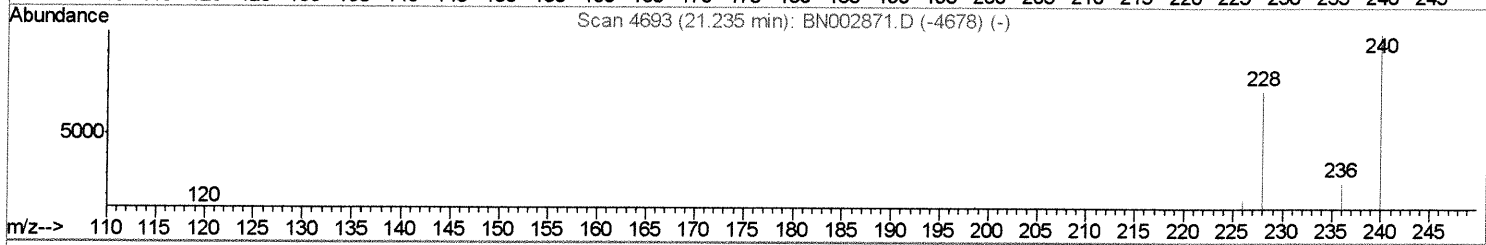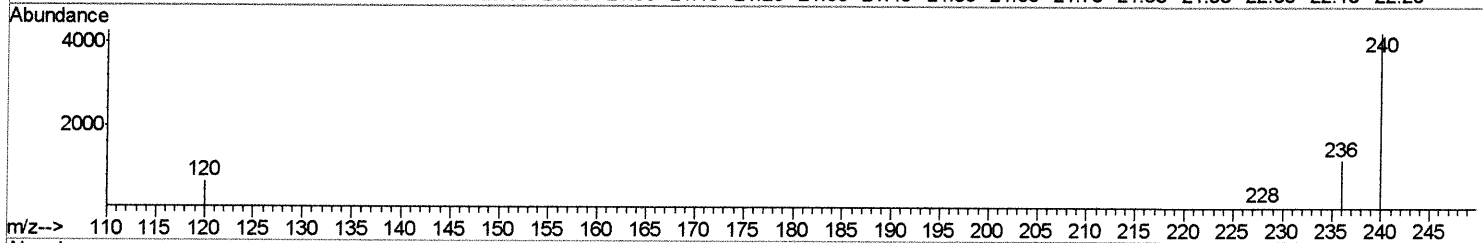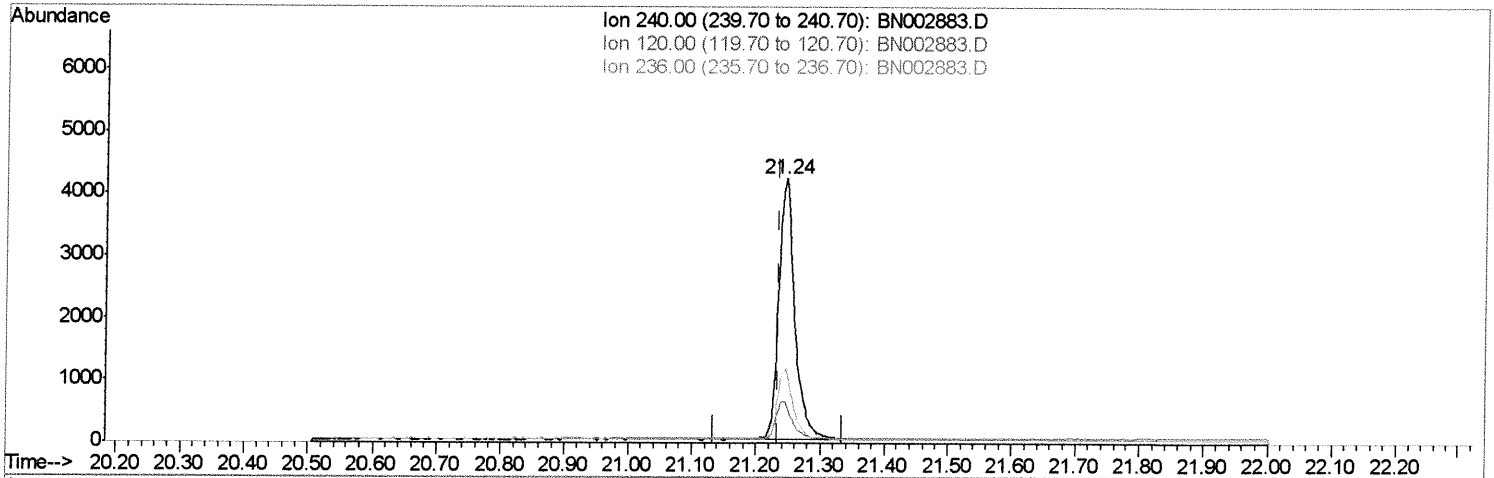

TIC: BN002883.D

(16) Chrysene-d12 (I)

21.244min (+0.009) 0.40ng/ul m

SJ 10/12/18

response 7370

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	15.55#
236.00	34.90	28.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100118\
Data File : BN002883.D
Acq On : 01 Oct 2018 17:23
Operator : MJ/SJ
Sample : J5117-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC86

Manual Integrations
APPROVED

Sohil
10/2/2018 5:45:52 PM

Quant Time: Oct 01 18:47:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 01 14:40:21 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1637	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.40	136	6692	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	3883	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	8162m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.24	240	7370m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	7407	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	4477	0.46	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	10382m	0.49	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> SJ 10/12/18

SJ 10/12/18