

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
 Data File : BN027992.D
 Acq On : 02 Oct 2023 18:05
 Operator : MA/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Oct 02 18:47:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 18:31:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	4732	0.400	ng	0.00
7) Naphthalene-d8	10.767	136	14845	0.400	ng	0.00
13) Acenaphthene-d10	14.587	164	9038	0.400	ng	-0.01
19) Phenanthrene-d10	17.344	188	19376	0.400	ng	0.00
29) Chrysene-d12	21.533	240	18865	0.400	ng	0.00
35) Perylene-d12	24.013	264	14753	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.481	112	40380	2.757	ng	0.00
5) Phenol-d6	7.106	99	52921	2.905	ng	0.00
8) Nitrobenzene-d5	9.145	82	40395	3.258	ng	0.00
11) 2-Methylnaphthalene-d10	12.351	152	71225	3.286	ng	0.00
14) 2,4,6-Tribromophenol	16.090	330	13568	3.388	ng	0.00
15) 2-Fluorobiphenyl	13.219	172	101446	3.149	ng	0.00
27) Fluoranthene-d10	19.379	212	161786	3.355	ng	0.00
31) Terphenyl-d14	19.964	244	127589	2.890	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.365	88	16539	2.708	ng	97
3) n-Nitrosodimethylamine	3.704	42	18954	3.086	ng	# 98
6) bis(2-Chloroethyl)ether	7.387	93	45015	3.120	ng	100
9) Naphthalene	10.821	128	122819	3.233	ng	98
10) Hexachlorobutadiene	11.045	225	21451	3.163	ng	# 99
12) 2-Methylnaphthalene	12.423	142	87009	3.288	ng	99
16) Acenaphthylene	14.320	152	133635	3.452	ng	100
17) Acenaphthene	14.651	154	82544	3.284	ng	100
18) Fluorene	15.643	166	108198	3.311	ng	100
20) 4,6-Dinitro-2-methylph...	16.797	198	807	2.872	ng	# 47
21) 4-Bromophenyl-phenylether	16.524	248	32848	3.350	ng	97
22) Hexachlorobenzene	16.611	284	33884	3.243	ng	98
23) Atrazine	16.797	200	29430	3.452	ng	98
24) Pentachlorophenol	16.984	266	18168	3.996	ng	94
25) Phenanthrene	17.393	178	171023	3.345	ng	99
26) Anthracene	17.480	178	165082	3.466	ng	100
28) Fluoranthene	19.407	202	199996	3.342	ng	100
30) Pyrene	19.774	202	207440	3.028	ng	99
32) Benzo(a)anthracene	21.516	228	195259	3.049	ng	99
33) Chrysene	21.578	228	185570	2.999	ng	98
34) Bis(2-ethylhexyl)phtha...	21.390	149	129181	2.768	ng	99
36) Indeno(1,2,3-cd)pyrene	26.612	276	153139	3.180	ng	99
37) Benzo(b)fluoranthene	23.244	252	155533	3.298	ng	# 88
38) Benzo(k)fluoranthene	23.294	252	158047	3.320	ng	# 88
39) Benzo(a)pyrene	23.899	252	145396	3.278	ng	# 84
40) Dibenzo(a,h)anthracene	26.630	278	125769	3.195	ng	# 89
41) Benzo(g,h,i)perylene	27.428	276	127468	3.153	ng	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
Data File : BN027992.D
Acq On : 02 Oct 2023 18:05
Operator : MA/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Oct 02 18:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 18:31:30 2023
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.951 min Scan# 702
 Delta R.T. 0.001 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:152 Resp: 4732
 Ion Ratio Lower Upper
 152 100
 150 153.3 125.6 188.4
 115 66.6 54.8 82.2



#2
 1,4-Dioxane
 Concen: 2.708 ng
 RT: 3.365 min Scan# 67
 Delta R.T. 0.000 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05

Tgt Ion: 88 Resp: 16539
 Ion Ratio Lower Upper
 88 100
 43 25.8 24.6 36.8
 58 66.6 53.8 80.6








#3
n-Nitrosodimethylamine
Concen: 3.086 ng
RT: 3.704 min Scan# 116
Delta R.T. -0.014 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 42 Resp: 18954
Ion Ratio Lower Upper
42 100
74 147.1 115.9 173.9
44 5.9 8.0 12.0#



#4
2-Fluorophenol
Concen: 2.757 ng
RT: 5.481 min Scan# 360
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion: 112 Resp: 40380
Ion Ratio Lower Upper
112 100
64 57.4 45.0 67.6
63 29.5 23.4 35.0








#5
Phenol-d6
Concen: 2.905 ng
RT: 7.106 min Scan# 585
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion: 99 Resp: 52921
Ion Ratio Lower Upper
99 100
42 17.9 14.6 22.0
71 34.4 28.3 42.5



#6
bis(2-Chloroethyl)ether
Concen: 3.120 ng
RT: 7.387 min Scan# 624
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion: 93 Resp: 45015
Ion Ratio Lower Upper
93 100
63 73.7 58.8 88.2
95 32.6 26.6 39.8








#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.767 min Scan# 982
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:	136	Resp:	14845
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.4	14.0
54	8.3	7.0	10.6
68	7.9	6.4	9.6



#8
Nitrobenzene-d5
Concen: 3.258 ng
RT: 9.145 min Scan# 830
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:	82	Resp:	40395
Ion Ratio	Lower	Upper	
82	100		
128	41.5	32.7	49.1
54	44.6	38.7	58.1









#9
Naphthalene
Concen: 3.233 ng
RT: 10.821 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:128 Resp: 122819
Ion Ratio Lower Upper
128 100
129 10.9 9.4 14.2
127 13.1 10.9 16.3



#10
Hexachlorobutadiene
Concen: 3.163 ng
RT: 11.045 min Scan# 1008
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:225 Resp: 21451
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.2 51.3 76.9









#11
2-Methylnaphthalene-d10
Concen: 3.286 ng
RT: 12.351 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 71225
Ion Ratio Lower Upper
152 100
151 20.5 16.5 24.7



#12
2-Methylnaphthalene
Concen: 3.288 ng
RT: 12.423 min Scan# 1294
Delta R.T. -0.004 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:142 Resp: 87009
Ion Ratio Lower Upper
142 100
141 89.4 70.7 106.1
115 35.3 28.6 42.8







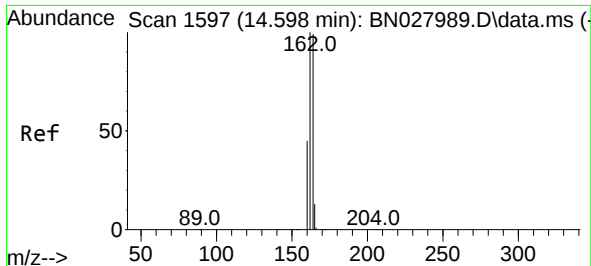

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.587 min Scan# 1596
Delta R.T. -0.011 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 9038
Ion Ratio Lower Upper
164 100
162 106.4 80.8 121.2
160 49.8 36.4 54.6



#14
2,4,6-Tribromophenol
Concen: 3.388 ng
RT: 16.090 min Scan# 1729
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:330 Resp: 13568
Ion Ratio Lower Upper
330 100
332 96.3 78.1 117.1
141 41.5 33.4 50.2









#15
2-Fluorobiphenyl
Concen: 3.149 ng
RT: 13.219 min Scan# 1468
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 101446
Ion Ratio Lower Upper
172 100
171 34.4 28.1 42.1
170 22.4 18.4 27.6



#16
Acenaphthylene
Concen: 3.452 ng
RT: 14.320 min Scan# 1571
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:152 Resp: 133635
Ion Ratio Lower Upper
152 100
151 19.5 15.8 23.6
153 13.0 10.2 15.4





#17

Acenaphthene

Concen: 3.284 ng

RT: 14.651 min Scan# 1602

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:154 Resp: 82544

Ion Ratio Lower Upper

154 100

153 113.5 90.8 136.2

152 54.2 43.9 65.9



#18

Fluorene

Concen: 3.311 ng

RT: 15.643 min Scan# 1693

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05




Tgt Ion:166 Resp: 108198


Ion Ratio Lower Upper

166 100

165 97.4 77.8 116.8

167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.344 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 19376
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.5 10.2 15.4



#20
4,6-Dinitro-2-methylphenol
Concen: 2.872 ng
RT: 16.797 min Scan# 1786
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:198 Resp: 807
Ion Ratio Lower Upper
198 100
51 43.3 180.7 271.1#
105 269.1 222.2 333.2









#21
4-Bromophenyl-phenylether
Concen: 3.350 ng
RT: 16.524 min Scan# 1764
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:248 Resp: 32848
Ion Ratio Lower Upper
248 100
250 92.4 72.3 108.5
141 86.9 71.8 107.6



#22
Hexachlorobenzene
Concen: 3.243 ng
RT: 16.611 min Scan# 1771
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:284 Resp: 33884
Ion Ratio Lower Upper
284 100
142 38.6 29.9 44.9
249 32.0 25.0 37.4









#23
 Atrazine
 Concen: 3.452 ng
 RT: 16.797 min Scan# 1786
 Delta R.T. 0.000 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:200 Resp: 29430
 Ion Ratio Lower Upper
 200 100
 173 29.8 24.7 37.1
 215 47.3 39.0 58.6



#24
 Pentachlorophenol
 Concen: 3.996 ng
 RT: 16.984 min Scan# 1801
 Delta R.T. 0.000 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05

Tgt Ion:266 Resp: 18168
 Ion Ratio Lower Upper
 266 100
 264 63.0 52.7 79.1
 268 63.9 56.2 84.2









#25
Phenanthrene
Concen: 3.345 ng
RT: 17.393 min Scan# 1834
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:178 Resp: 171023
Ion Ratio Lower Upper
178 100
176 18.8 15.3 22.9
179 15.3 12.4 18.6



#26
Anthracene
Concen: 3.466 ng
RT: 17.480 min Scan# 1841
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:178 Resp: 165082
Ion Ratio Lower Upper
178 100
176 18.2 14.7 22.1
179 15.3 12.2 18.2









#27
Fluoranthene-d10
Concen: 3.355 ng
RT: 19.379 min Scan# 2111
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 161786
Ion Ratio Lower Upper
212 100
106 14.2 11.3 16.9
104 8.0 6.4 9.6



#28
Fluoranthene
Concen: 3.342 ng
RT: 19.407 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:202 Resp: 199996
Ion Ratio Lower Upper
202 100
101 12.2 9.8 14.6
203 17.4 13.8 20.8



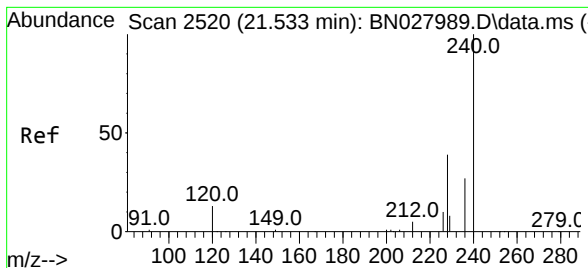

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.533 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:240 Resp: 18865

Ion Ratio Lower Upper

240 100

120 18.1 13.8 20.6

236 28.0 22.6 33.8

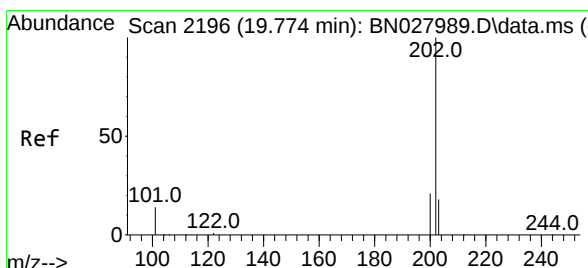

#30

Pyrene

Concen: 3.028 ng

RT: 19.774 min Scan# 2196

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05




Tgt Ion:202 Resp: 207440


Ion Ratio Lower Upper

202 100

200 20.6 16.5 24.7

203 18.0 14.7 22.1





#31

Terphenyl-d14

Concen: 2.890 ng

RT: 19.964 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:244 Resp: 127589

Ion Ratio Lower Upper

244 100

212 7.6 6.6 9.8

122 12.9 11.4 17.0



#32

Benzo(a)anthracene

Concen: 3.049 ng

RT: 21.516 min Scan# 2518

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05




Tgt Ion:228 Resp: 195259


Ion Ratio Lower Upper

228 100

226 27.3 22.0 33.0

229 19.5 16.0 24.0





#33

Chrysene

Concen: 2.999 ng

RT: 21.578 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:228 Resp: 185570

Ion Ratio Lower Upper

228 100

226 29.0 23.8 35.8

229 19.9 16.6 25.0



#34

Bis(2-ethylhexyl)phthalate

Concen: 2.768 ng

RT: 21.390 min Scan# 2504

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05




Tgt Ion:149 Resp: 129181


Ion Ratio Lower Upper

149 100

167 27.2 22.1 33.1

279 3.9 3.4 5.0









#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.013 min Scan# 3166
 Delta R.T. 0.000 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:264 Resp: 14753




Ion	Ratio	Lower	Upper
264	100		
260	26.0	20.2	30.4
265	73.8	54.8	82.2



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 3.180 ng
 RT: 26.612 min Scan# 4055
 Delta R.T. 0.000 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05

Tgt Ion:276 Resp: 153139

Ion	Ratio	Lower	Upper
276	100		
138	26.5	20.9	31.3
277	25.1	19.8	29.6





#37

Benzo(b)fluoranthene

Concen: 3.298 ng

RT: 23.244 min Scan# 2903

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:252 Resp: 155533

Ion Ratio Lower Upper

252 100

253 22.8 22.9 34.3#

125 11.4 13.8 20.8#



#38

Benzo(k)fluoranthene

Concen: 3.320 ng

RT: 23.294 min Scan# 2920

Delta R.T. 0.000 min

Lab File: BN027992.D

Acq: 02 Oct 2023 18:05




Tgt Ion:252 Resp: 158047

Ion Ratio Lower Upper

252 100

253 22.7 23.1 34.7#

125 11.5 13.8 20.8#









#39
Benzo(a)pyrene
Concen: 3.278 ng
RT: 23.899 min Scan# 3127
Delta R.T. -0.003 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 145396
Ion Ratio Lower Upper
252 100
253 22.6 25.0 37.4#
125 12.7 16.6 24.8#



#40
Dibenzo(a,h)anthracene
Concen: 3.195 ng
RT: 26.630 min Scan# 4061
Delta R.T. 0.000 min
Lab File: BN027992.D
Acq: 02 Oct 2023 18:05

Tgt Ion:278 Resp: 125769
Ion Ratio Lower Upper
278 100
139 17.7 17.7 26.5#
279 24.6 25.2 37.8#



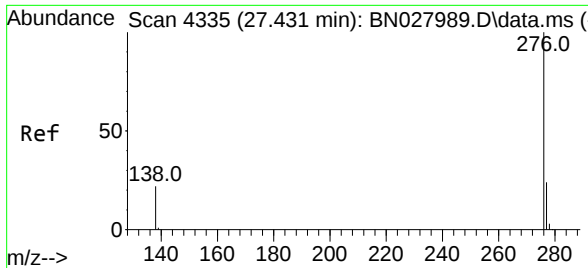

#41
 Benzo(g,h,i)perylene
 Concen: 3.153 ng
 RT: 27.428 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: BN027992.D
 Acq: 02 Oct 2023 18:05

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:	276	Resp:	127468
Ion	Ratio	Lower	Upper
276	100		
277	24.0	22.1	33.1
138	23.0	20.8	31.2

