
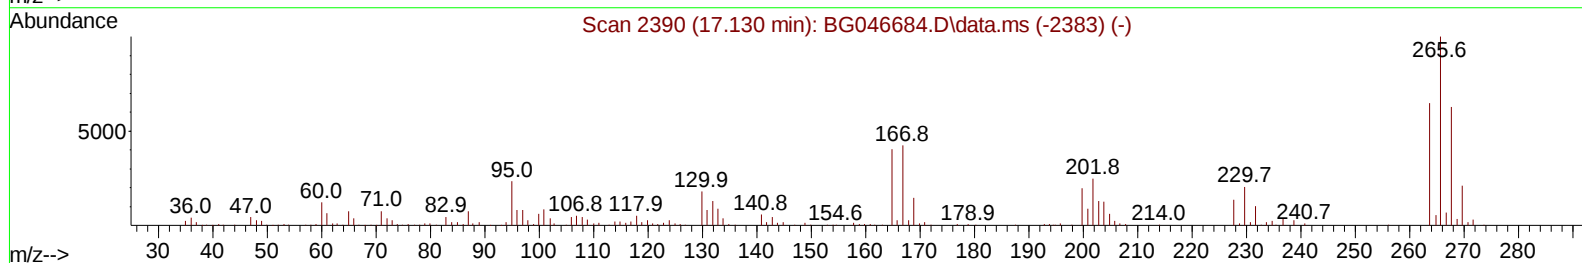
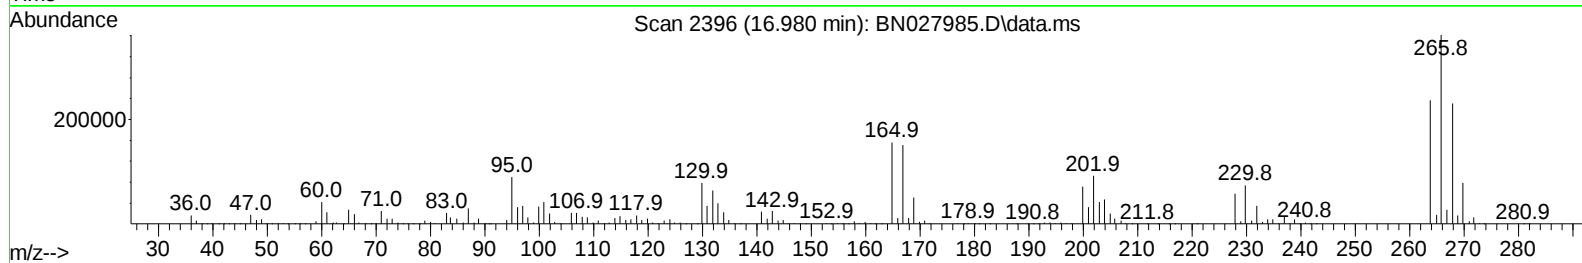


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
Data File : BN027985.D
Acq On : 02 Oct 2023 13:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 05:57:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 05:57:21 2023
Response via : Initial Calibration

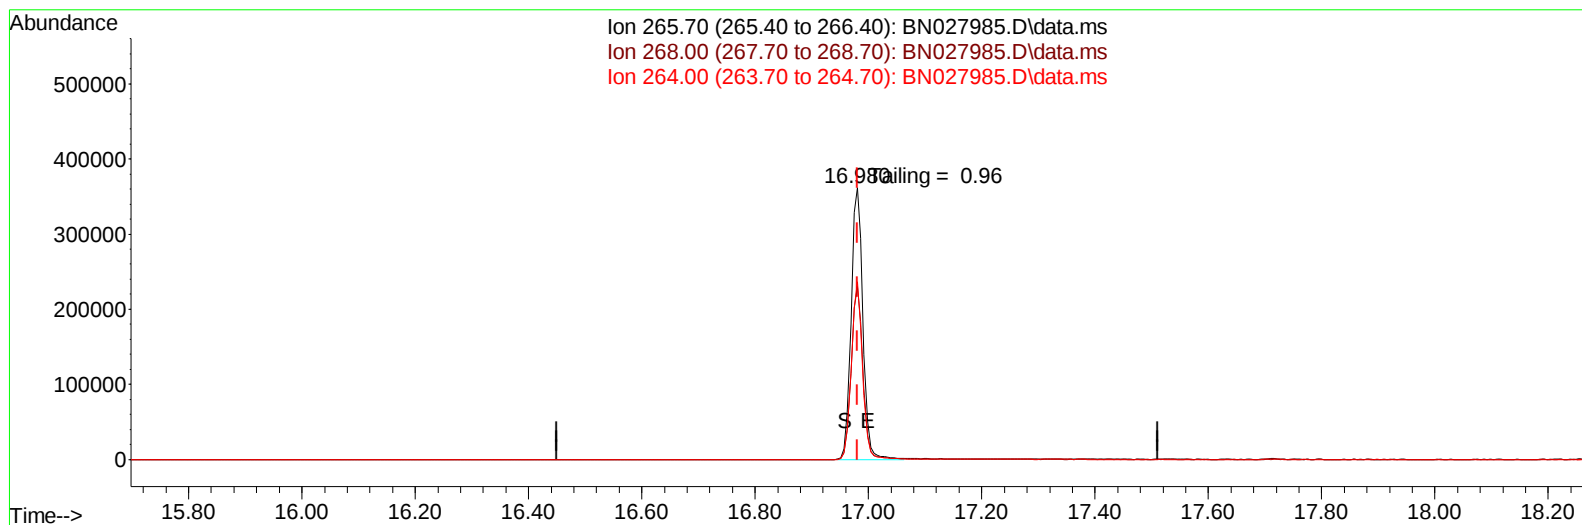




TIC: BN027985.D\data.ms

(70) Pentachloropheno1 (C)**16.980min (0.000) 24036.84 ng****response 527235**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.74
264.00	61.60	65.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
Data File : BN027985.D
Acq On : 02 Oct 2023 13:46
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 05:57:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 05:57:21 2023
Response via : Initial Calibration

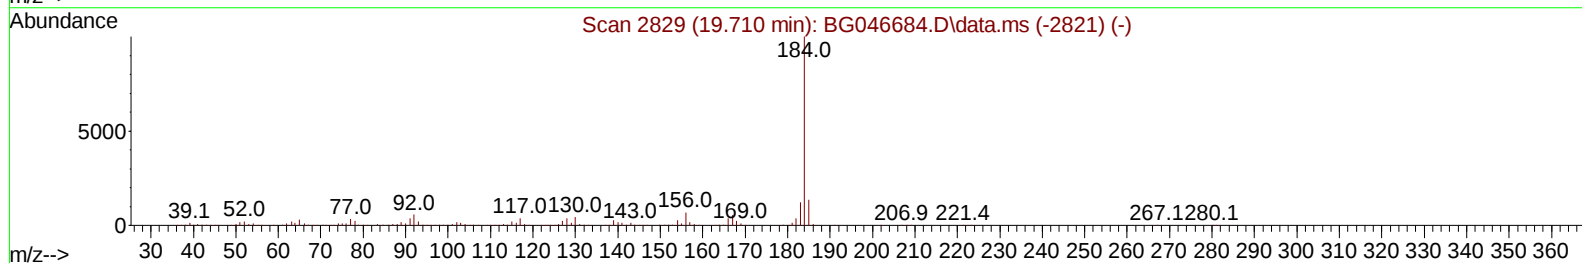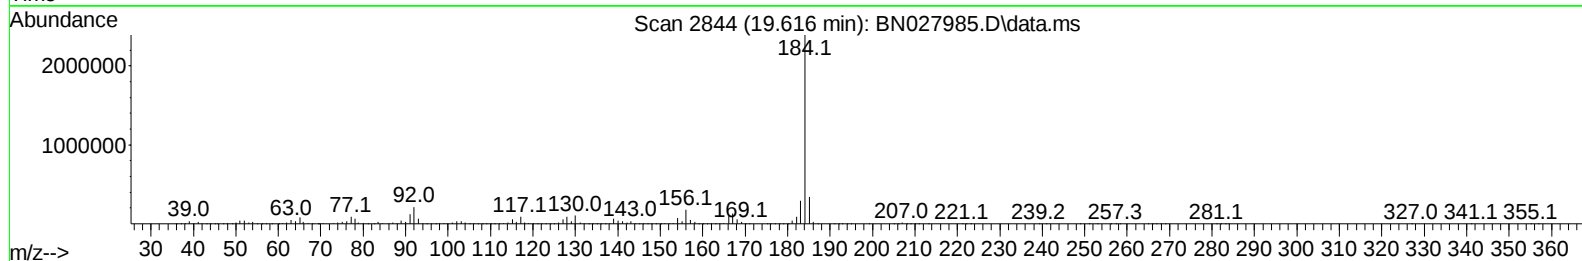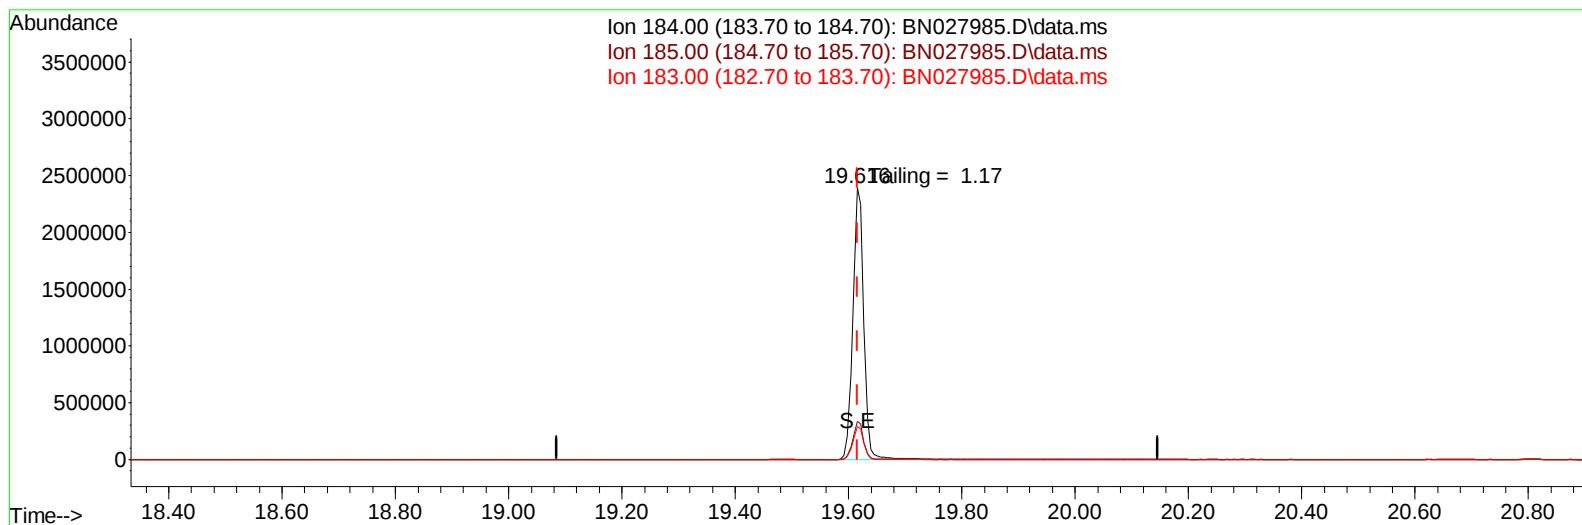

TIC: BN027985.D\data.ms

(77) Benzidine**19.616min (0.000) 282439.39 ng****response 3230037**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	12.07
0.00	0.00	0.00