
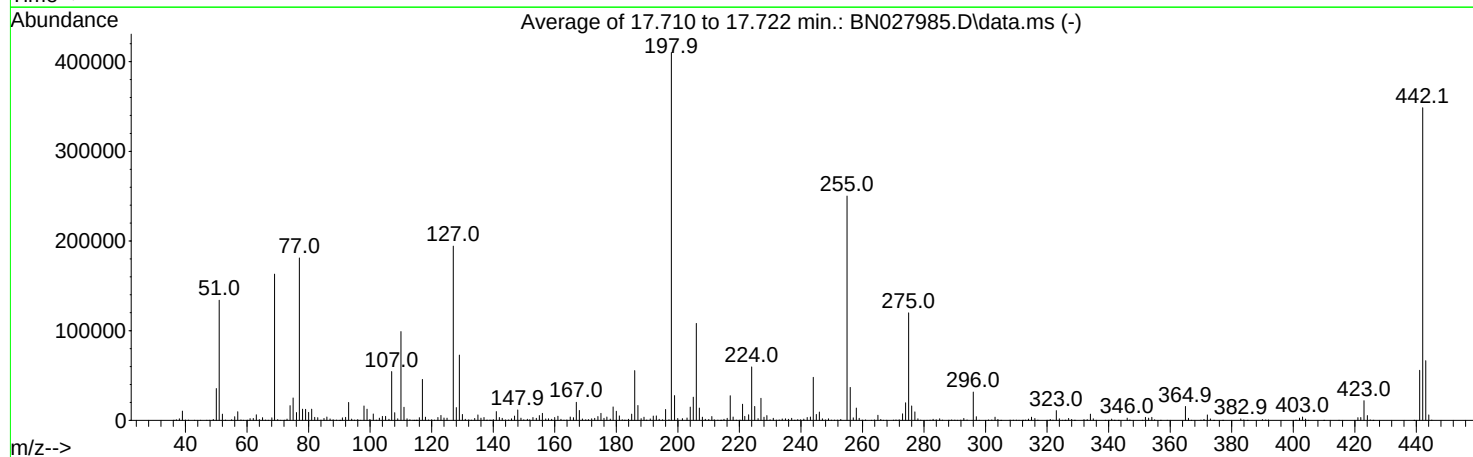


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
Data File : BN027985.D
Acq On : 02 Oct 2023 13:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 02 19:18:04 2023

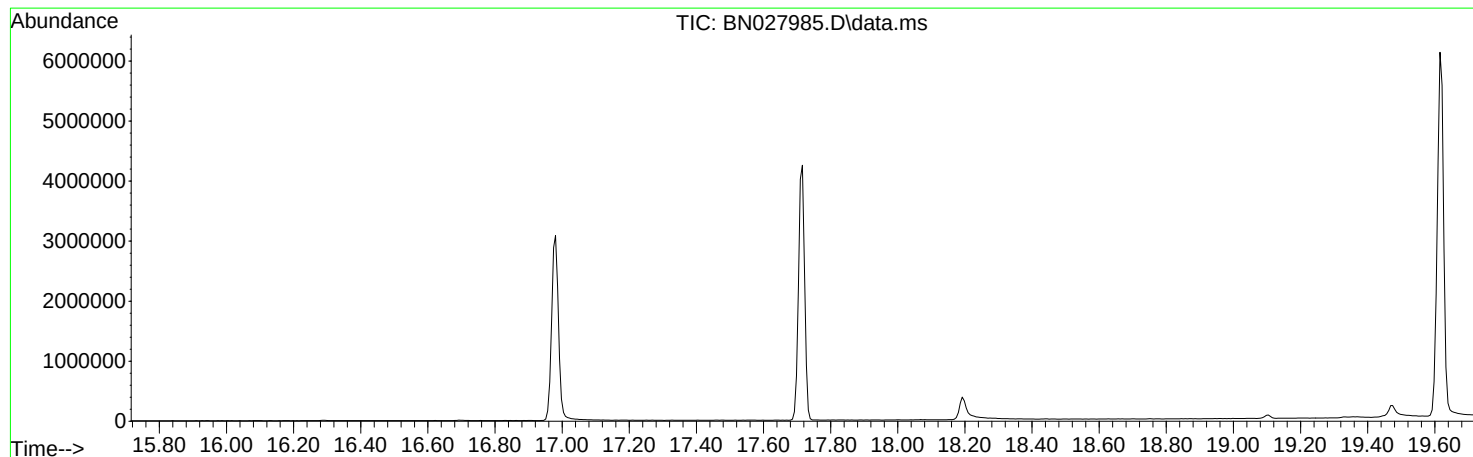




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	133937	PASS
68	69	0.00	2	1.8	2893	PASS
69	198	0.00	100	39.7	163009	PASS
70	69	0.00	2	0.6	956	PASS
127	198	10	80	47.4	194277	PASS
197	198	0.00	2	0.2	767	PASS
198	198	100	100	100.0	410219	PASS
199	198	5	9	6.7	27653	PASS
275	198	10	60	29.2	119824	PASS
365	198	1	100	3.8	15472	PASS
441	198	0.01	100	13.6	55939	PASS
442	442	50	100	100.0	348608	PASS
443	442	15	24	19.1	66576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
Data File : BN027985.D
Acq On : 02 Oct 2023 13:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 03 05:57:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 05:57:21 2023
Response via : Initial Calibration

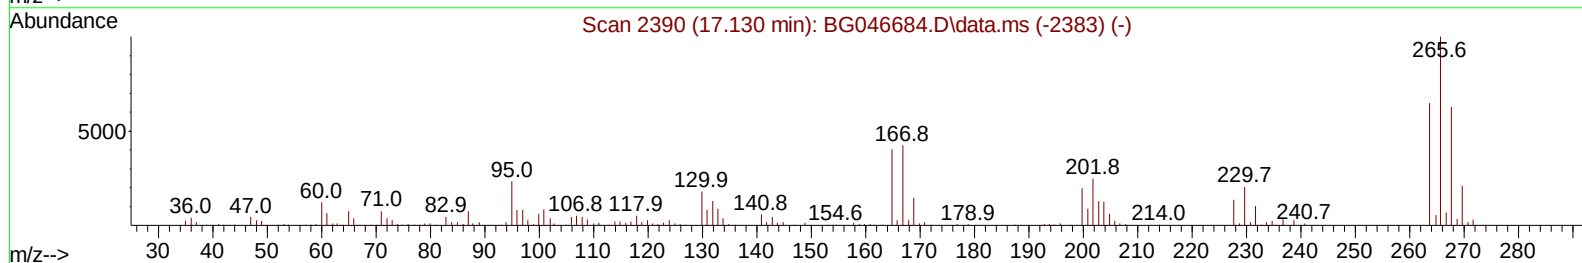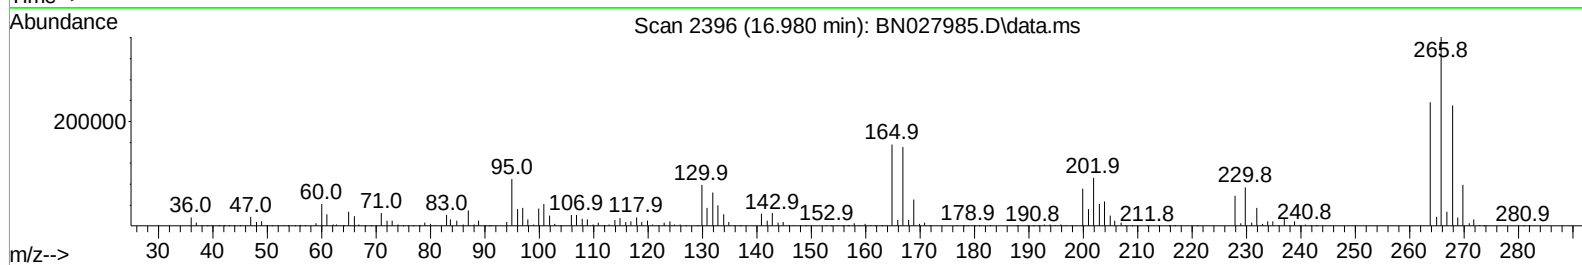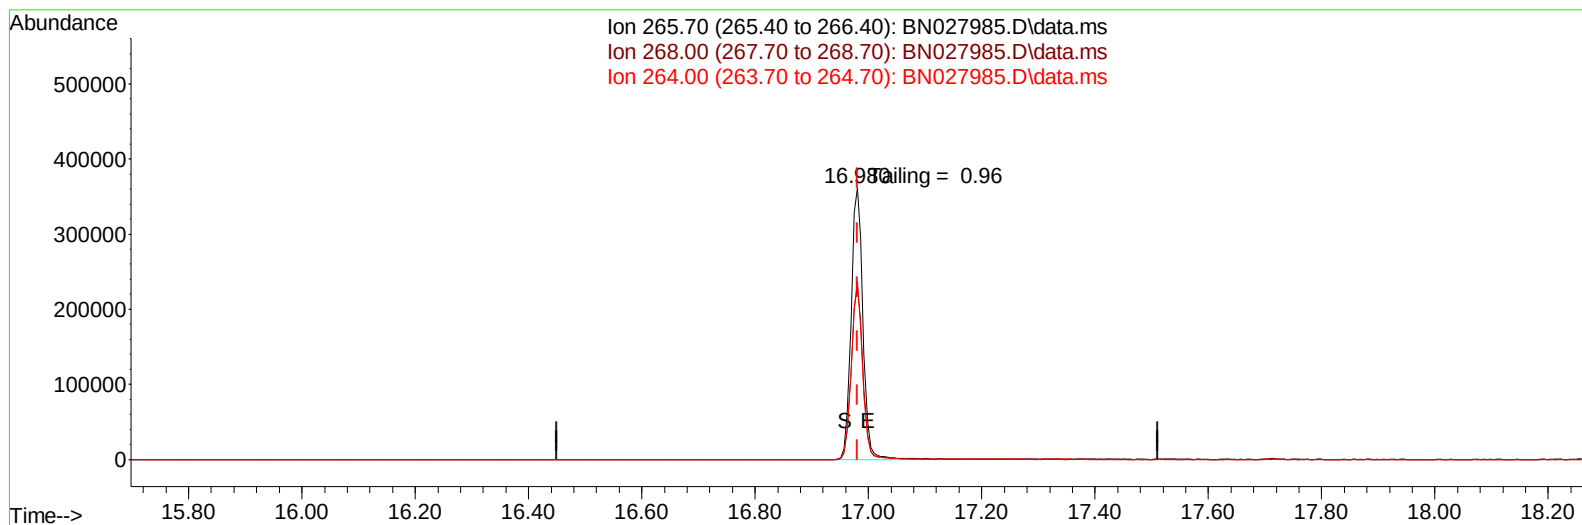

TIC: BN027985.D\data.ms

(70) Pentachlorophenol (C)

16.980min (0.000) 24036.84 ng




response 527235

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.74
264.00	61.60	65.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100223\
Data File : BN027985.D
Acq On : 02 Oct 2023 13:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 03 05:57:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 05:57:21 2023
Response via : Initial Calibration

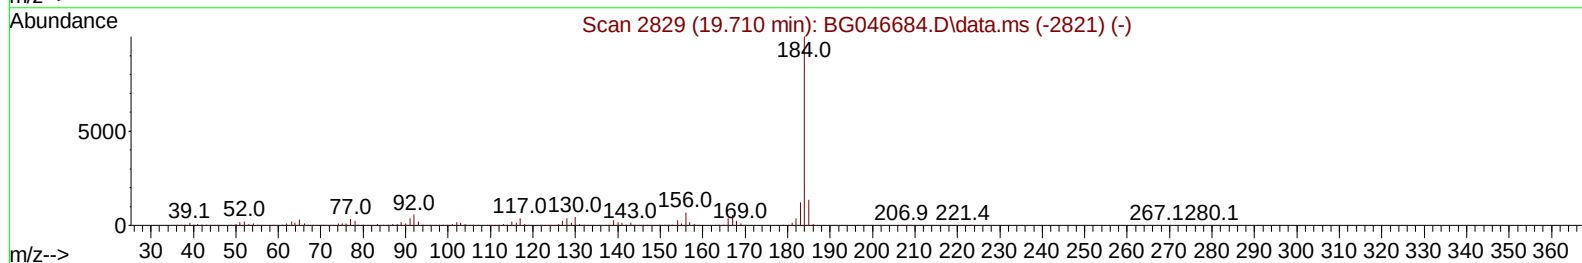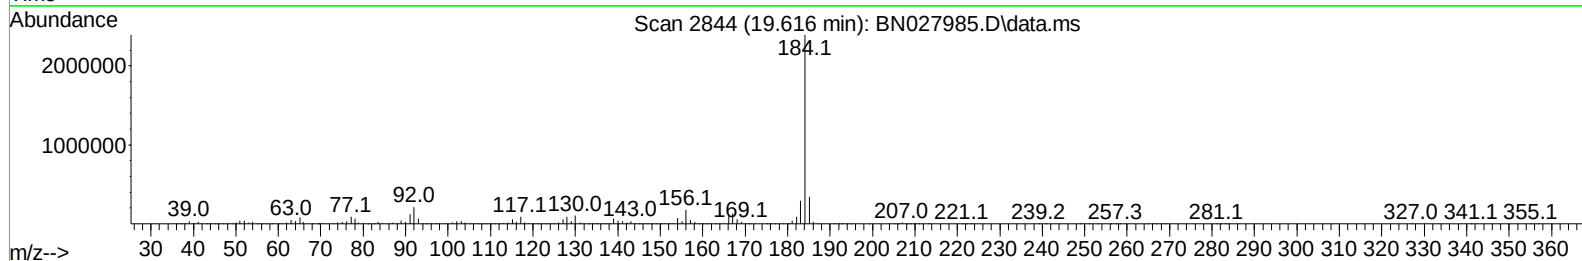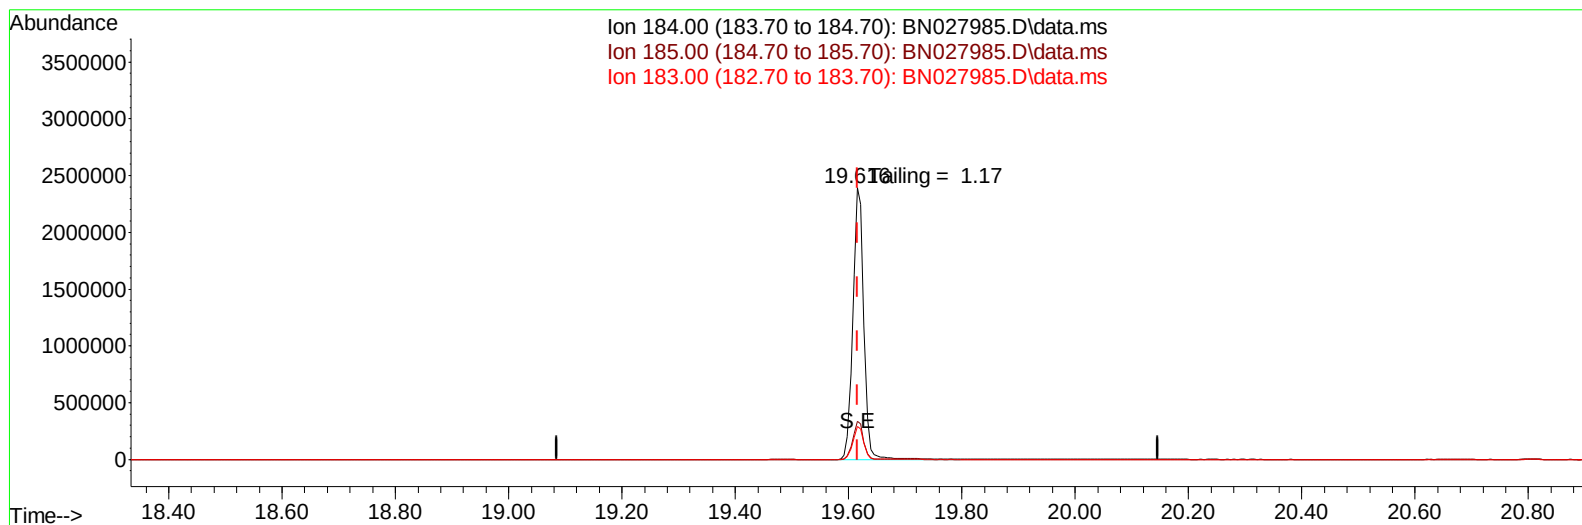

TIC: BN027985.D\data.ms

(77) Benzidine

19.616min (0.000) 282439.39 ng

response 3230037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/2/2023	BNA_N	<u>BN027985.D</u>
Compound Name	Response	Retention Time
DDT	1524265	20.84
DDD	21598	20.41
DDE	712	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22310	1546575	1.44

Instrument :
BNA_N
ClientSampleId :
DFTPP