

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100318\
 Data File : BN002888.D
 Acq On : 03 Oct 2018 07:39
 Operator : MJ/SJ
 Sample : AR1254-50PPM
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 AR1254-50PPM

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	31	rVB	571316	567621	22.63%	1.721%
2	7.616	780	787	798	rVB	725447	1153540	45.99%	3.497%
3	10.387	1250	1258	1271	rBV	1005522	1645176	65.60%	4.988%
4	14.257	1910	1916	1927	rVB2	1403417	2167220	86.41%	6.571%
5	17.010	2378	2384	2395	rBV2	1698258	2508000	100.00%	7.604%
6	17.610	2482	2486	2493	rBV4	23074	42143	1.68%	0.128%
7	17.916	2532	2538	2552	rBV3	123272	253043	10.09%	0.767%
8	18.087	2561	2567	2572	rBV	736245	954795	38.07%	2.895%
9	18.145	2572	2577	2582	rBV	146727	181146	7.22%	0.549%
10	18.369	2610	2615	2621	rBV	285180	390710	15.58%	1.185%
11	18.463	2627	2631	2636	rBV3	23105	37444	1.49%	0.114%
12	18.516	2636	2640	2643	rVV4	22567	36163	1.44%	0.110%
13	18.551	2643	2646	2651	rVB	78347	96028	3.83%	0.291%
14	18.863	2694	2699	2703	rBV	102232	138431	5.52%	0.420%
15	18.916	2703	2708	2709	rVV	474559	577110	23.01%	1.750%
16	18.939	2709	2712	2720	rVB	870717	1273182	50.76%	3.860%
17	19.028	2722	2727	2731	rVB	117742	145040	5.78%	0.440%
18	19.151	2743	2748	2754	rBV2	191161	303787	12.11%	0.921%
19	19.228	2755	2761	2767	rVV	1277607	1818123	72.49%	5.512%
20	19.292	2767	2772	2776	rVV	398507	500750	19.97%	1.518%
21	19.357	2776	2783	2788	rVV	686390	777964	31.02%	2.359%
22	19.422	2788	2794	2795	rVV3	70499	97581	3.89%	0.296%
23	19.486	2799	2805	2812	rVV2	448457	852705	34.00%	2.585%
24	19.569	2812	2819	2824	rVV	539112	722815	28.82%	2.192%
25	19.622	2824	2828	2831	rVV	151038	199470	7.95%	0.605%
26	19.675	2831	2837	2843	rVB	1080581	1467892	58.53%	4.451%
27	19.804	2854	2859	2860	rBV2	92015	116965	4.66%	0.355%
28	19.822	2860	2862	2864	rVV2	119556	135556	5.40%	0.411%
29	19.845	2864	2866	2871	rVV3	84226	112208	4.47%	0.340%
30	19.892	2871	2874	2877	rVV2	49329	55291	2.20%	0.168%
31	19.939	2877	2882	2886	rVV2	497901	638925	25.48%	1.937%
32	19.992	2886	2891	2896	rVB	873643	1128443	44.99%	3.421%
33	20.069	2901	2904	2910	rVB3	57996	63711	2.54%	0.193%
34	20.145	2910	2917	2922	rBV3	100885	162820	6.49%	0.494%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100318\
 Data File : BN002888.D
 Acq On : 03 Oct 2018 07:39
 Operator : MJ/SJ
 Sample : AR1254-50PPM
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 AR1254-50PPM

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Title : SVOA CALIBRATION

35	20.222	2925	2930	2935	rBV	526237	594329	23.70%	1.802%
36	20.275	2935	2939	2941	rBV2	284035	350574	13.98%	1.063%
37	20.304	2941	2944	2949	rVB	361475	428363	17.08%	1.299%
38	20.375	2952	2956	2959	rVV3	123550	150971	6.02%	0.458%
39	20.410	2959	2962	2966	rVV	549232	592981	23.64%	1.798%
40	20.445	2966	2968	2970	rVV3	54216	61817	2.46%	0.187%
41	20.475	2970	2973	2976	rVV	207490	234961	9.37%	0.712%
42	20.539	2976	2984	2991	rVV2	619310	1098490	43.80%	3.331%
43	20.628	2995	2999	3003	rBV4	49542	56952	2.27%	0.173%
44	20.686	3003	3009	3015	rVB7	25843	54009	2.15%	0.164%
45	20.751	3015	3020	3023	rBV6	18788	28304	1.13%	0.086%
46	20.845	3032	3036	3041	rBV	200222	237322	9.46%	0.720%
47	20.916	3043	3048	3050	rVV	354585	407886	16.26%	1.237%
48	20.939	3050	3052	3059	rVV	186514	242706	9.68%	0.736%
49	21.010	3061	3064	3068	rVB2	31248	34726	1.38%	0.105%
50	21.098	3076	3079	3083	rVB	96289	110060	4.39%	0.334%
51	21.222	3094	3100	3111	rVV	1832229	2401583	95.76%	7.281%
52	21.333	3115	3119	3123	rVV	182280	215012	8.57%	0.652%
53	21.380	3123	3127	3133	rVB	285173	312802	12.47%	0.948%
54	21.557	3153	3157	3161	rBV6	54267	73226	2.92%	0.222%
55	21.810	3196	3200	3205	rVB	253983	300046	11.96%	0.910%
56	22.263	3272	3277	3285	rVB	297895	380106	15.16%	1.152%
57	22.757	3356	3361	3370	rBV	262229	388960	15.51%	1.179%
58	23.304	3449	3454	3461	rVB	218147	367499	14.65%	1.114%
59	23.427	3468	3475	3488	rVB	875932	1766564	70.44%	5.356%
60	23.798	3536	3538	3545	rVB4	49697	85616	3.41%	0.260%
61	23.933	3555	3561	3568	rVB	159127	300192	11.97%	0.910%
62	24.651	3677	3683	3690	rBV	120840	243813	9.72%	0.739%
63	25.492	3821	3826	3834	rVB3	59245	140365	5.60%	0.426%


Sum of corrected areas: 32982033

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100318\
Data File : BN002888.D
Acq On : 03 Oct 2018 07:39
Operator : MJ/SJ
Sample : AR1254-50PPM
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
AR1254-50PPM

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

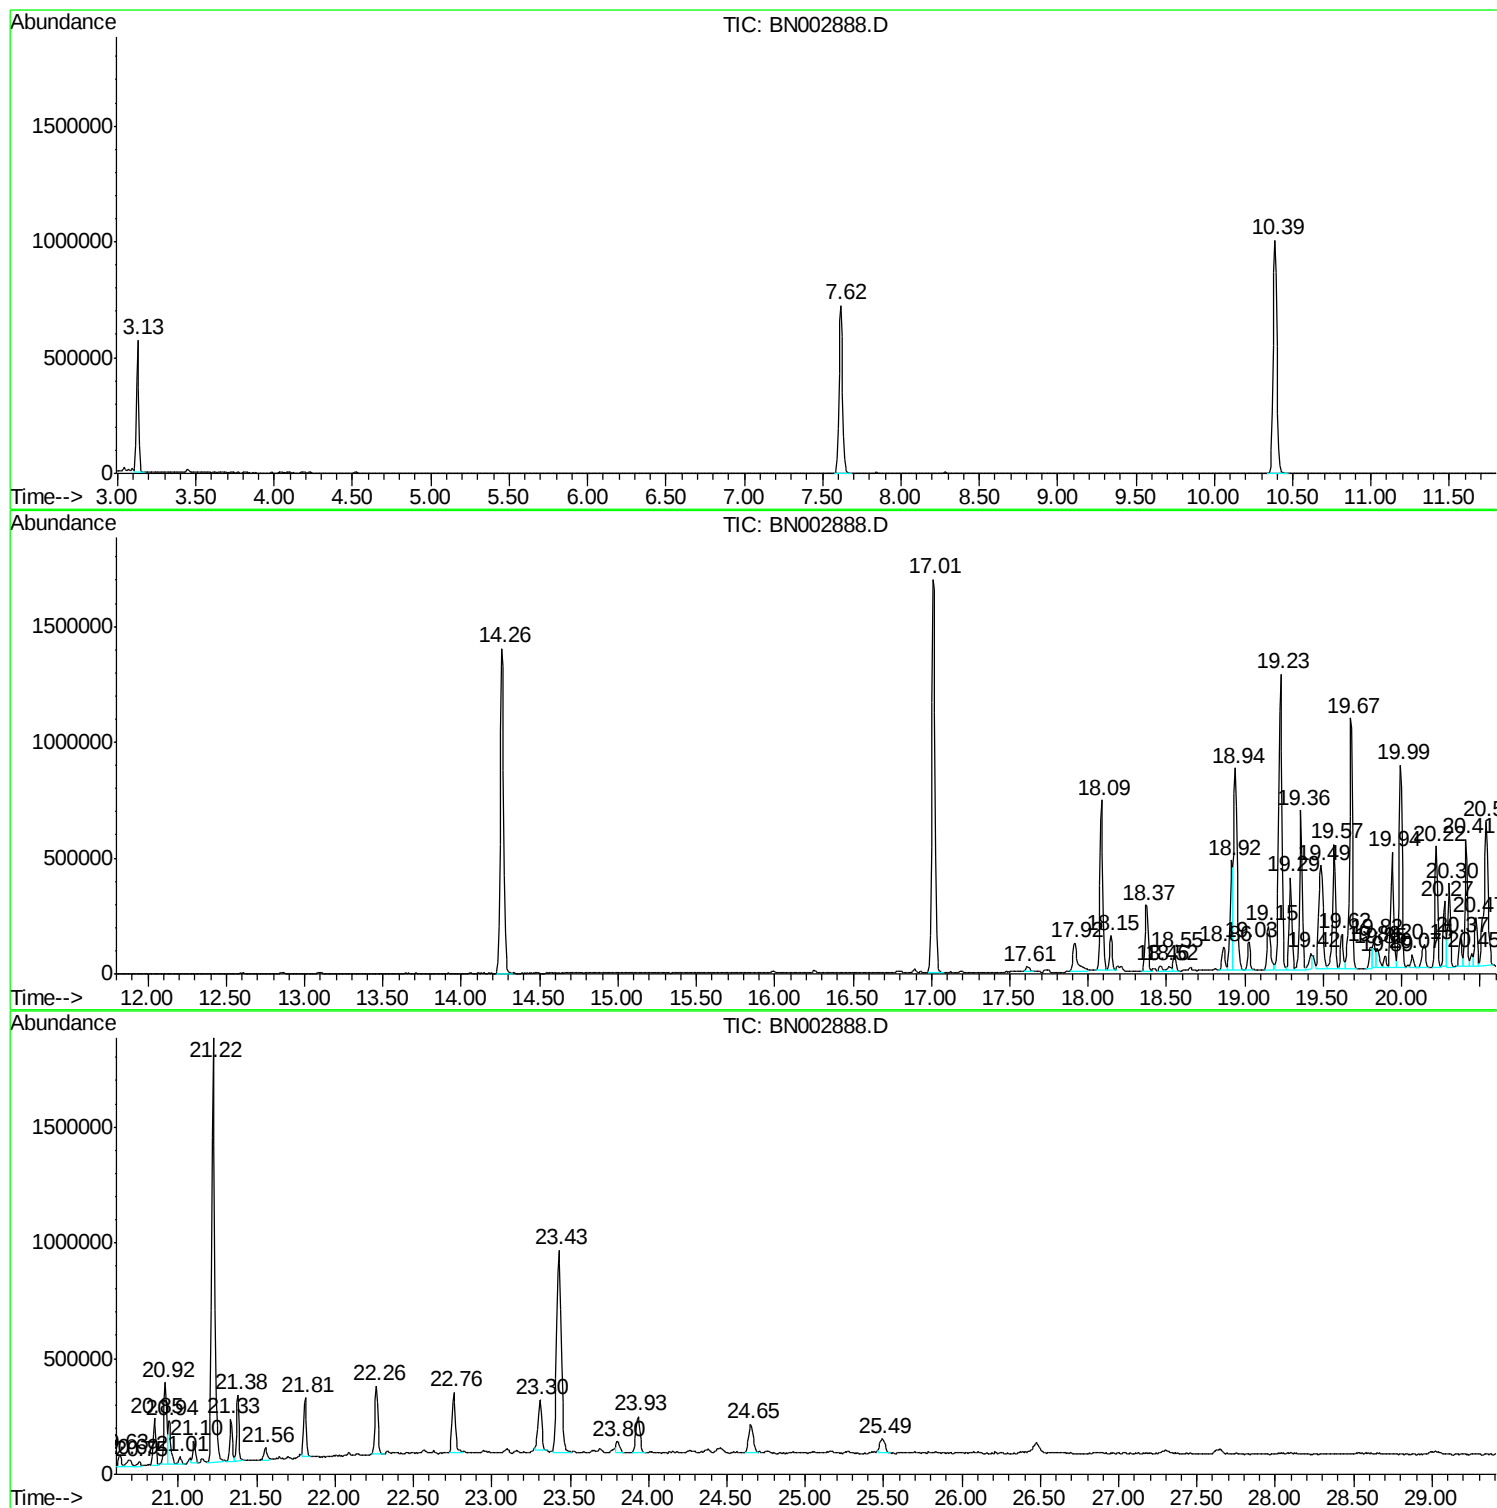

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100318\
Data_File : BN002888.D
Acq_On : 03_Oct_2018_ 07:399
Operator : MJ/SJJ
Sample : AR1254-50PPMM
Misc :
ALS_Vial : 1_ Sample_Multiplier: 11

Instrument :
BNA_N
ClientSampleId :
AR1254-50PPM

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
