

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
 Data File : BN021979.D
 Acq On : 03 Oct 2022 15:37
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Oct 04 01:12:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 01:08:47 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.986	152	4477	0.400	ng	0.00
7) Naphthalene-d8	10.816	136	12332	0.400	ng	0.00
13) Acenaphthene-d10	14.653	164	6665	0.400	ng	0.00
19) Phenanthrene-d10	17.400	188	13143	0.400	ng	#-0.01
29) Chrysene-d12	21.600	240	11931	0.400	ng	# 0.00
35) Perylene-d12	24.084	264	8961	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.508	112	49848	4.260	ng	0.00
5) Phenol-d6	7.141	99	67992	4.537	ng	0.00
8) Nitrobenzene-d5	9.161	82	52472	4.865	ng	0.00
11) 2-Methylnaphthalene-d10	12.406	152	114260	4.984	ng	0.00
14) 2,4,6-Tribromophenol	16.146	330	15798	5.345	ng	0.00
15) 2-Fluorobiphenyl	13.274	172	140937	4.883	ng	-0.01
27) Fluoranthene-d10	19.441	212	182908	5.078	ng	0.00
31) Terphenyl-d14	20.033	244	110031	4.575	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.320	88	25447	4.268	ng	99
3) n-Nitrosodimethylamine	3.652	42	29413	4.352	ng	# 96
6) bis(2-Chloroethyl)ether	7.401	93	66533	4.373	ng	97
9) Naphthalene	10.859	128	180997	4.839	ng	99
10) Hexachlorobutadiene	11.147	225	30133	4.698	ng	# 99
12) 2-Methylnaphthalene	12.108	142	38561	5.316	ng	# 81
16) Acenaphthylene	14.375	152	179689	5.678	ng	100
17) Acenaphthene	14.717	154	111841	4.987	ng	98
18) Fluorene	15.701	166	137388	5.154	ng	94
20) 4,6-Dinitro-2-methylph...	15.774	198	14856	6.681	ng	# 57
21) 4-Bromophenyl-phenylether	16.593	248	42184	5.081	ng	# 89
22) Hexachlorobenzene	16.705	284	48181	4.973	ng	99
23) Atrazine	16.866	200	34195	5.113	ng	# 93
24) Pentachlorophenol	17.052	266	21458	5.601	ng	98
25) Phenanthrene	17.449	178	226895	4.965	ng	100
26) Anthracene	17.536	178	204527	5.479	ng	100
28) Fluoranthene	19.470	202	251830	5.106	ng	99
30) Pyrene	19.837	202	253804	4.732	ng	100
32) Benzo(a)anthracene	21.591	228	233644	5.068	ng	98
33) Chrysene	21.645	228	234929	4.715	ng	99
34) Bis(2-ethylhexyl)phtha...	21.501	149	117641	5.096	ng	98
36) Indeno(1,2,3-cd)pyrene	26.686	276	235000	5.267	ng	99
37) Benzo(b)fluoranthene	23.318	252	213758	4.949	ng	# 90
38) Benzo(k)fluoranthene	23.371	252	216488	5.131	ng	# 91
39) Benzo(a)pyrene	23.970	252	171351	5.278	ng	# 83
40) Dibenzo(a,h)anthracene	26.707	278	186240	5.220	ng	95
41) Benzo(g,h,i)perylene	27.487	276	194946	5.232	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
 Data File : BN021979.D
 Acq On : 03 Oct 2022 15:37
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Oct 04 01:12:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 01:08:47 2022
 Response via : Initial Calibration




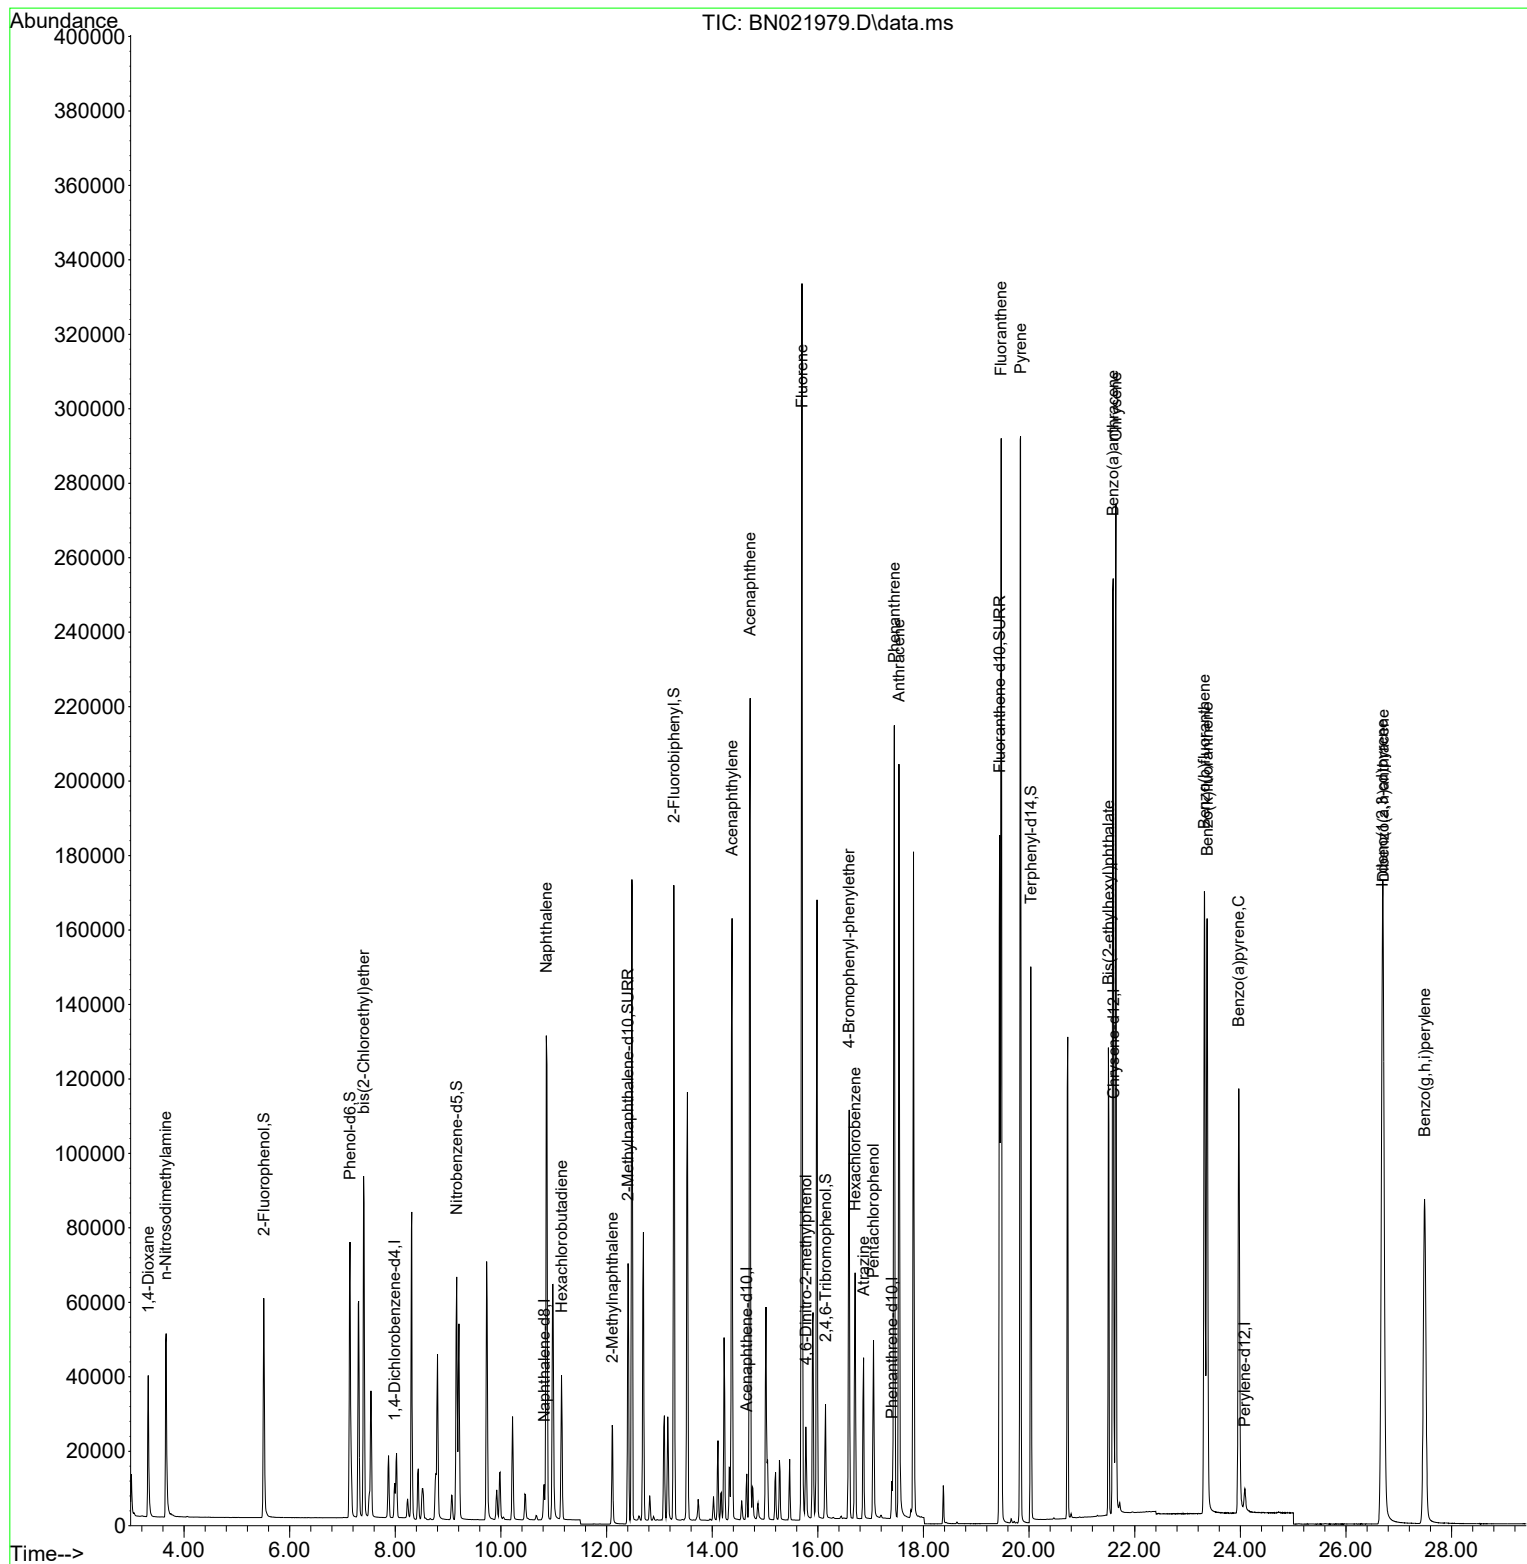




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.986 min Scan# 693
 Delta R.T. 0.001 min
 Lab File: BN021979.D
 Acq: 03 Oct 2022 15:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 4477
 Ion Ratio Lower Upper
 152 100
 150 156.9 127.2 190.8
 115 62.2 51.4 77.0

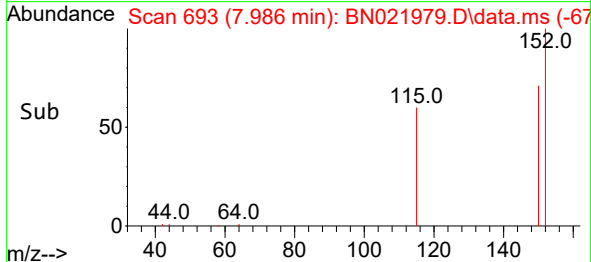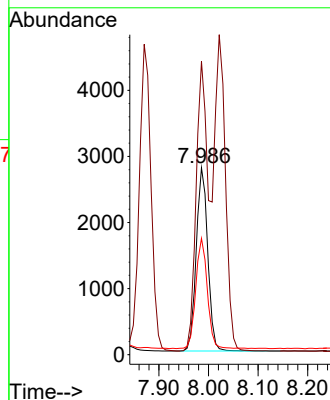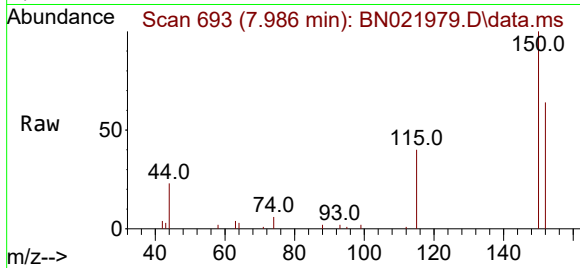

#2
 1,4-Dioxane
 Concen: 4.268 ng
 RT: 3.320 min Scan# 47
 Delta R.T. -0.007 min
 Lab File: BN021979.D
 Acq: 03 Oct 2022 15:37

Tgt Ion: 88 Resp: 25447
 Ion Ratio Lower Upper
 88 100
 43 28.5 22.6 34.0
 58 73.8 58.6 88.0


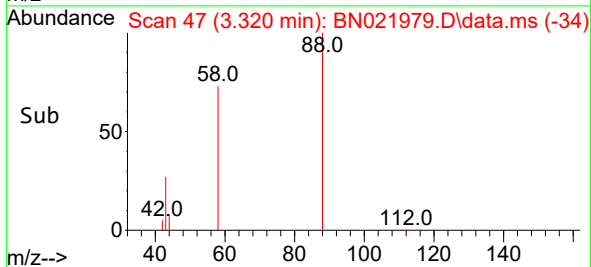
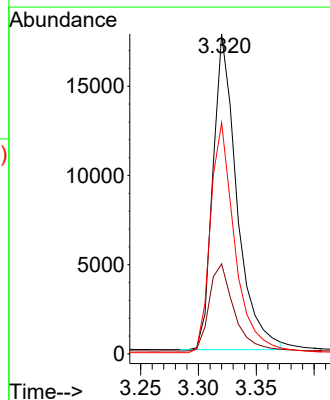
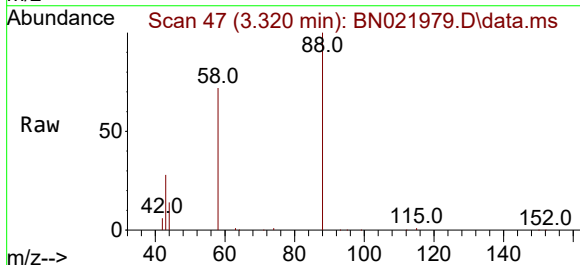




#3
 n-Nitrosodimethylamine
 Concen: 4.352 ng
 RT: 3.652 min Scan# 91
 Delta R.T. -0.014 min
 Lab File: BN021979.D
 Acq: 03 Oct 2022 15:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion: 42 Resp: 29413
 Ion Ratio Lower Upper
 42 100
 74 130.0 101.6 152.4
 44 6.9 10.4 15.6#

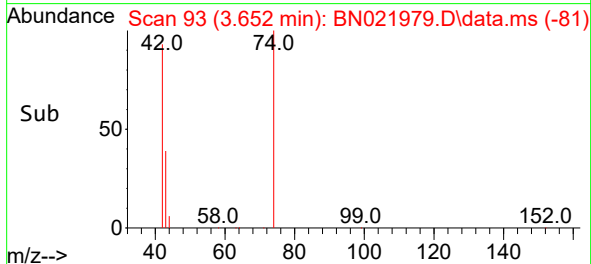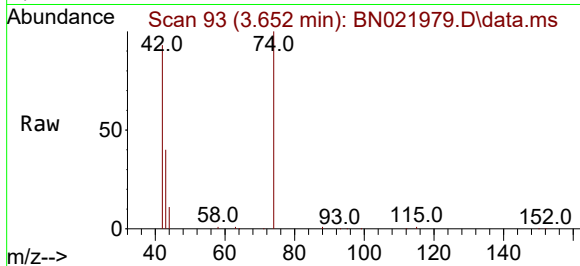

#4
 2-Fluorophenol
 Concen: 4.260 ng
 RT: 5.508 min Scan# 350
 Delta R.T. -0.007 min
 Lab File: BN021979.D
 Acq: 03 Oct 2022 15:37

Tgt Ion: 112 Resp: 49848
 Ion Ratio Lower Upper
 112 100
 64 58.3 46.9 70.3
 63 30.2 24.6 37.0


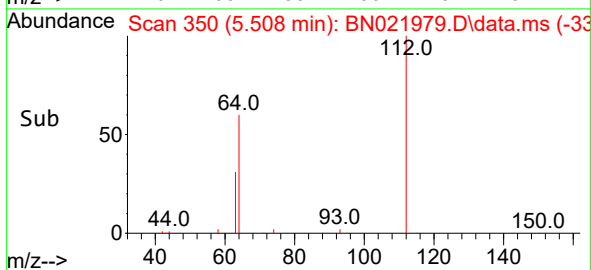

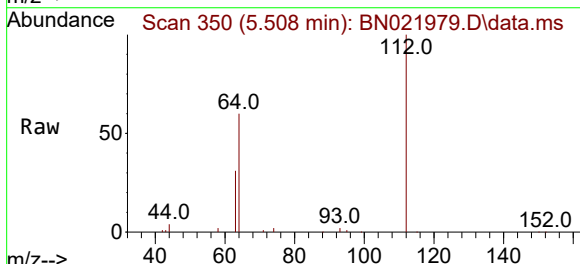




#5
Phenol-d6
Concen: 4.537 ng
RT: 7.141 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 67992
Ion Ratio Lower Upper
99 100
42 19.7 15.9 23.9
71 32.1 25.6 38.4

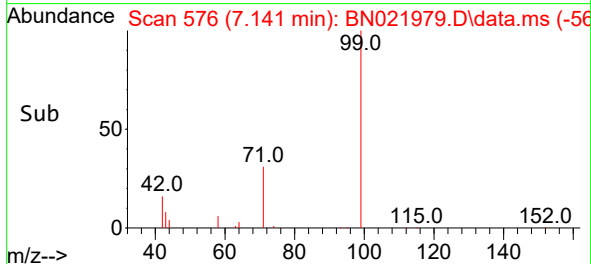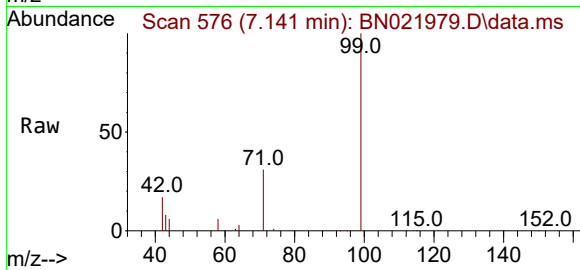

#6
bis(2-Chloroethyl)ether
Concen: 4.373 ng
RT: 7.401 min Scan# 612
Delta R.T. -0.007 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion: 93 Resp: 66533
Ion Ratio Lower Upper
93 100
63 77.9 64.8 97.2
95 32.4 26.6 40.0


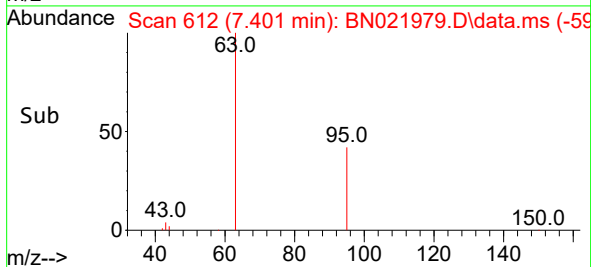

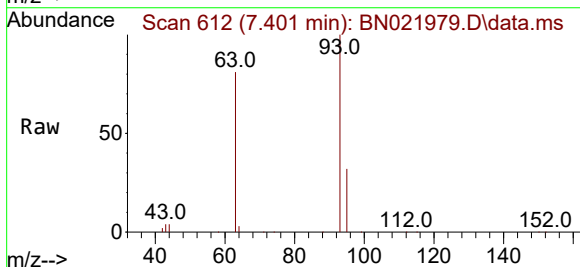




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.816 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	12332
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.2	13.8
54	7.7	7.1	10.7
68	6.7	6.2	9.2

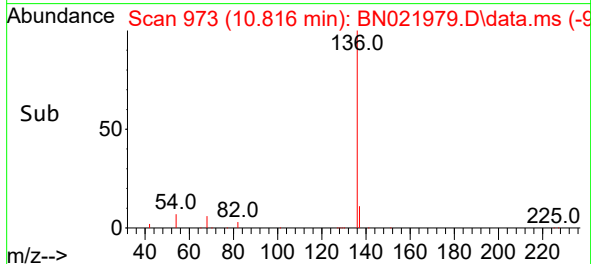

#8
Nitrobenzene-d5
Concen: 4.865 ng
RT: 9.161 min Scan# 818
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:	82	Resp:	52472
Ion	Ratio	Lower	Upper
82	100		
128	41.7	29.9	44.9
54	47.0	43.5	65.3


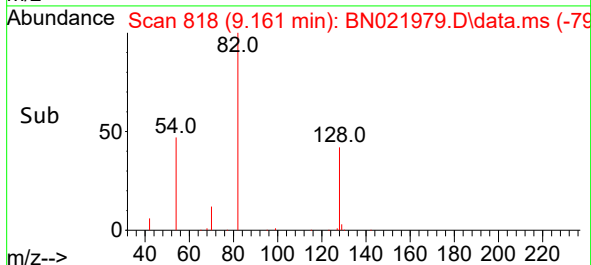
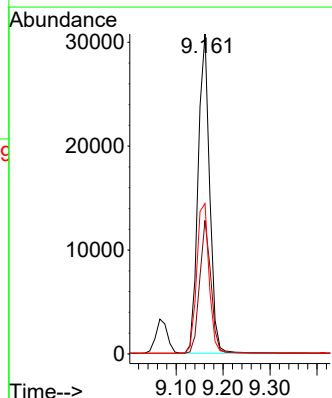
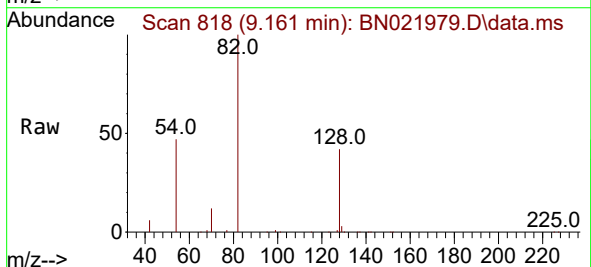




#9
Naphthalene
Concen: 4.839 ng
RT: 10.859 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:128 Resp: 180997
Ion Ratio Lower Upper
128 100
129 10.8 9.3 13.9
127 13.1 10.6 16.0

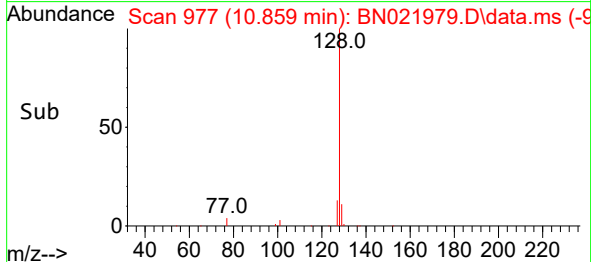

#10
Hexachlorobutadiene
Concen: 4.698 ng
RT: 11.147 min Scan# 1004
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:225 Resp: 30133
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.5 51.3 76.9


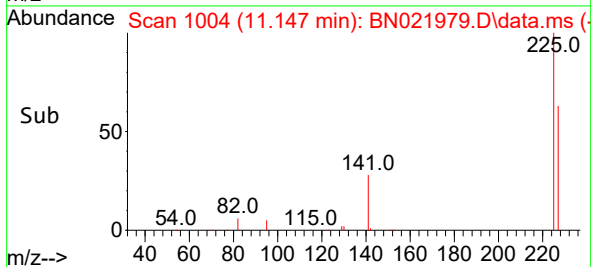

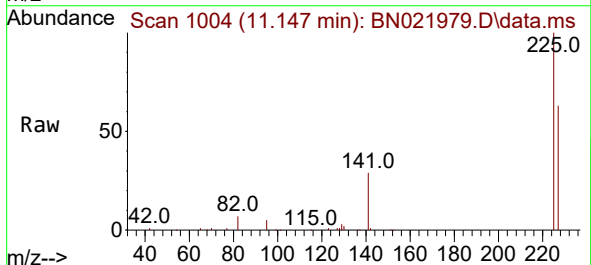




#11
2-Methylnaphthalene-d10
Concen: 4.984 ng
RT: 12.406 min Scan# 1196
Delta R.T. -0.004 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 114260
Ion Ratio Lower Upper
152 100
151 20.2 13.8 20.6

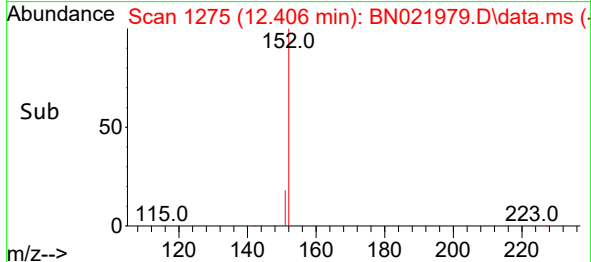

#12
2-Methylnaphthalene
Concen: 5.316 ng
RT: 12.108 min Scan# 1196
Delta R.T. -0.011 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:142 Resp: 38561
Ion Ratio Lower Upper
142 100
141 10.7 13.6 20.4#
115 2.1 9.7 14.5#


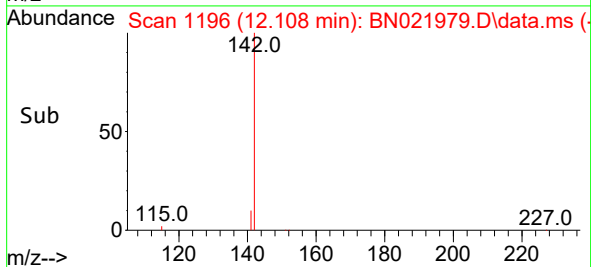

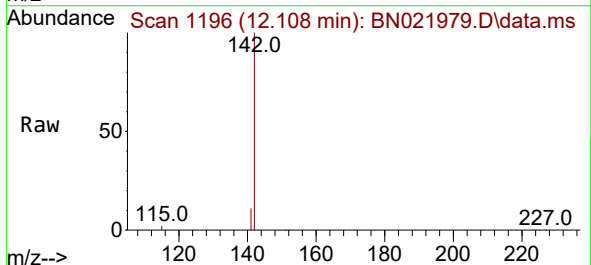


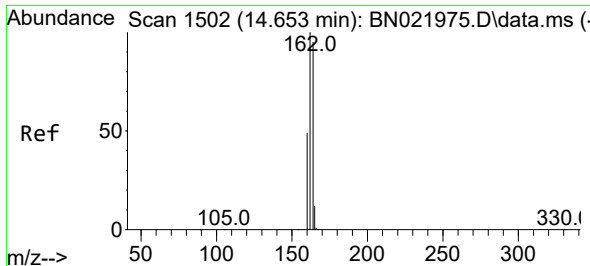

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.653 min Scan# 1502
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 6665
Ion Ratio Lower Upper
164 100
162 103.9 84.3 126.5
160 50.6 41.7 62.5

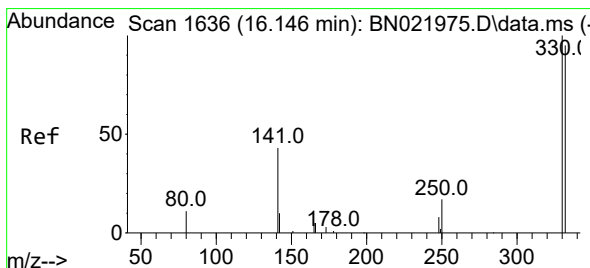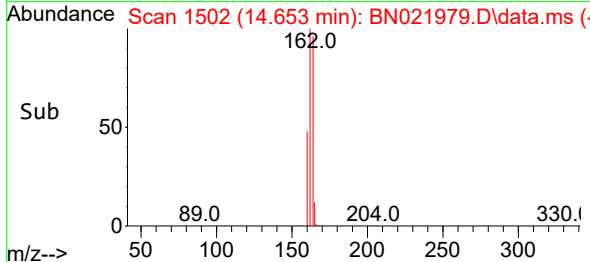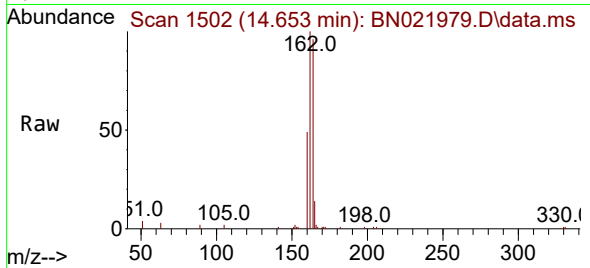

#14
2,4,6-Tribromophenol
Concen: 5.345 ng
RT: 16.146 min Scan# 1636
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:330 Resp: 15798
Ion Ratio Lower Upper
330 100
332 96.6 77.0 115.4
141 43.5 35.3 52.9


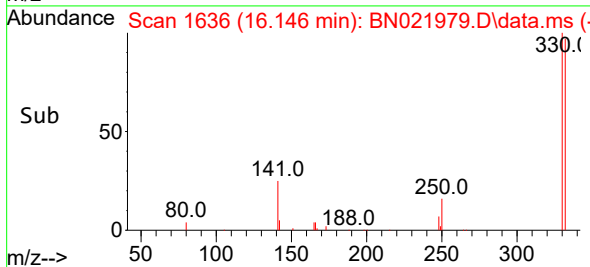

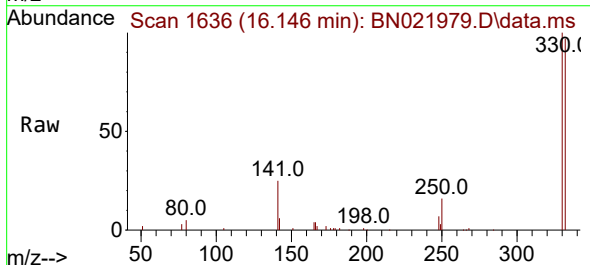




#15
2-Fluorobiphenyl
Concen: 4.883 ng
RT: 13.274 min Scan# 1374
Delta R.T. -0.011 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 140937
Ion Ratio Lower Upper
172 100
171 34.6 27.2 40.8
170 23.4 18.3 27.5

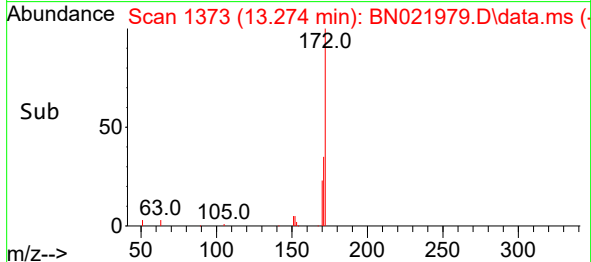

#16
Acenaphthylene
Concen: 5.678 ng
RT: 14.375 min Scan# 1476
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:152 Resp: 179689
Ion Ratio Lower Upper
152 100
151 19.2 15.5 23.3
153 13.0 10.4 15.6


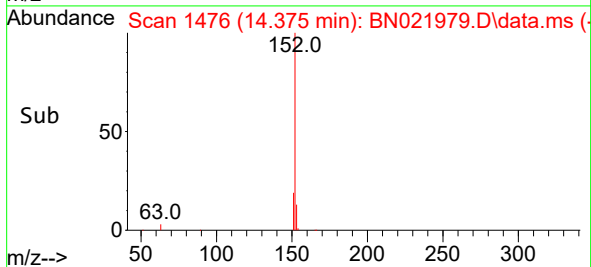

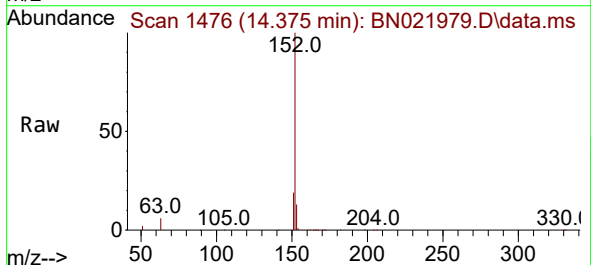




#17
Acenaphthene
Concen: 4.987 ng
RT: 14.717 min Scan# 1508
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 111841
Ion Ratio Lower Upper
154 100
153 113.3 92.1 138.1
152 57.1 47.8 71.6

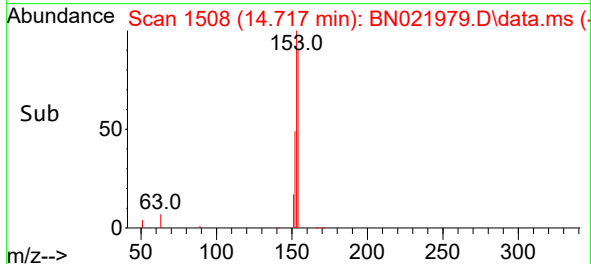

#18
Fluorene
Concen: 5.154 ng
RT: 15.701 min Scan# 1600
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:166 Resp: 137388
Ion Ratio Lower Upper
166 100
165 93.4 80.0 120.0
167 12.8 10.9 16.3

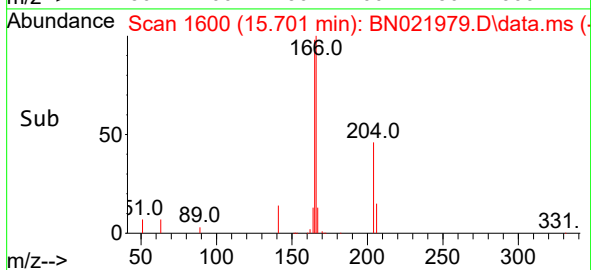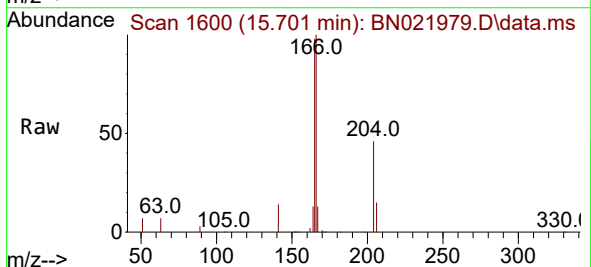



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.400 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:188 Resp: 13143

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 16.6 7.5 11.3#

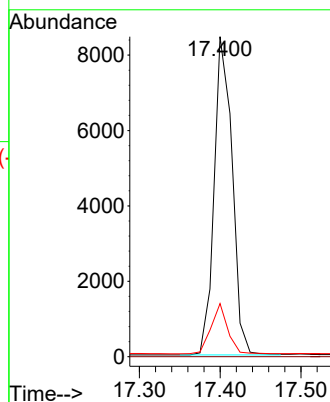

#20

4,6-Dinitro-2-methylphenol

Concen: 6.681 ng

RT: 15.774 min Scan# 1606

Delta R.T. -0.012 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37




Tgt Ion:198 Resp: 14856


Ion Ratio Lower Upper

198 100

51 57.6 96.6 144.8#

105 59.5 64.4 96.6#


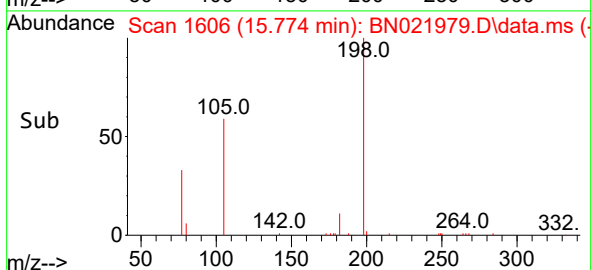
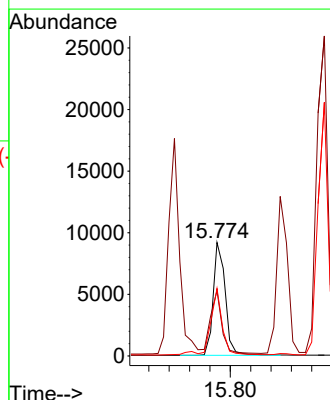



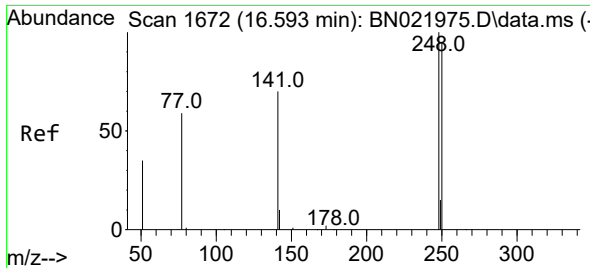

#21
4-Bromophenyl-phenylether
Concen: 5.081 ng
RT: 16.593 min Scan# 1672
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 42184
Ion Ratio Lower Upper
248 100
250 96.7 76.6 114.8
141 51.9 57.5 86.3#

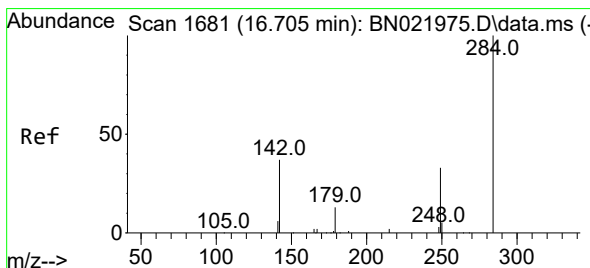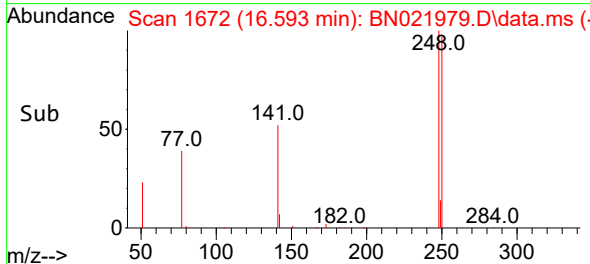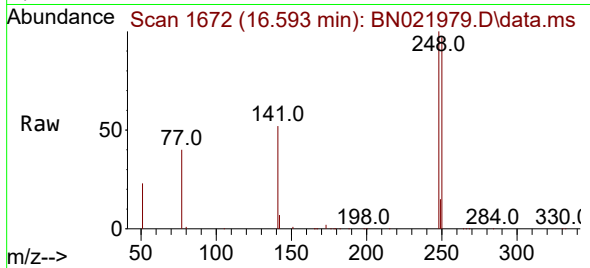

#22
Hexachlorobenzene
Concen: 4.973 ng
RT: 16.705 min Scan# 1681
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:284 Resp: 48181
Ion Ratio Lower Upper
284 100
142 41.3 33.4 50.0
249 31.0 25.1 37.7


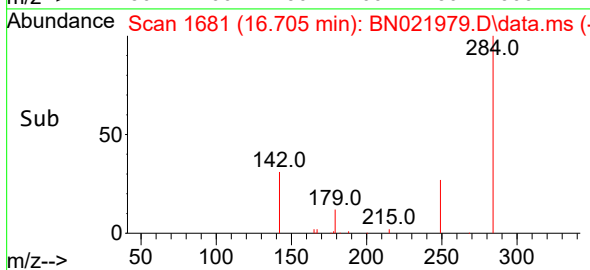

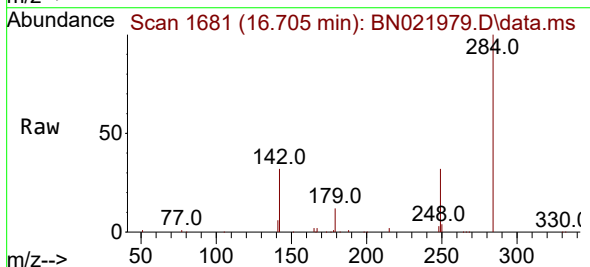


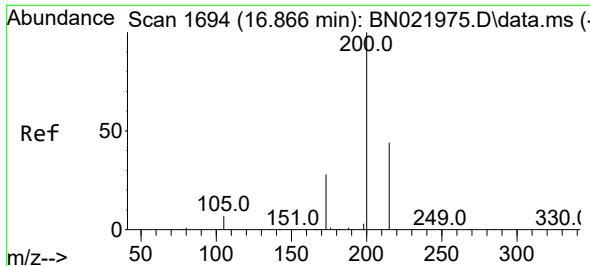

#23
Atrazine
Concen: 5.113 ng
RT: 16.866 min Scan# 1709
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:200 Resp: 34195
Ion Ratio Lower Upper
200 100
173 22.4 24.6 36.8#
215 45.8 37.1 55.7

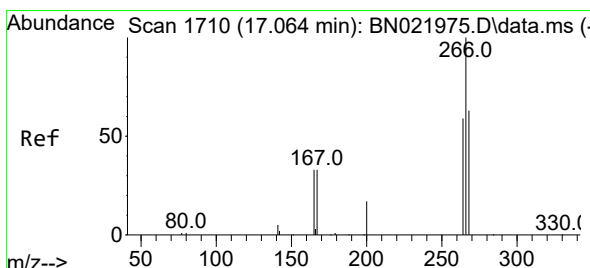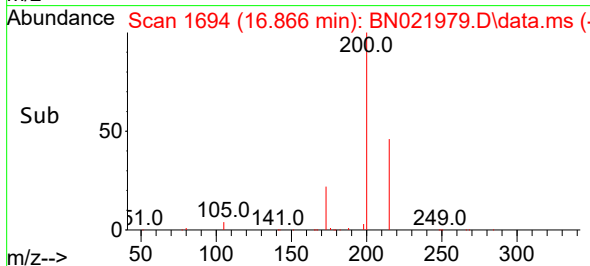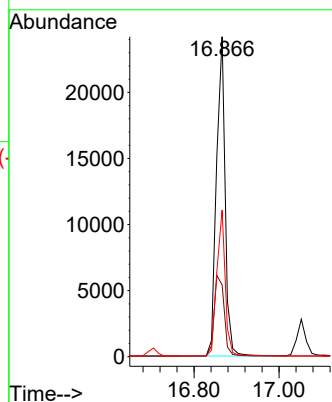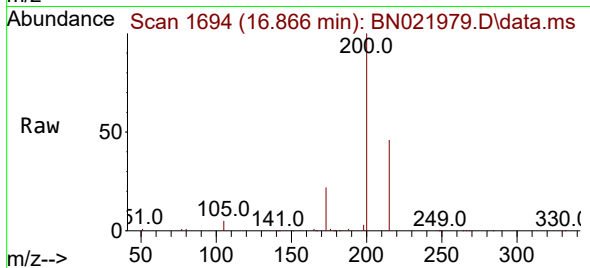

#24
Pentachlorophenol
Concen: 5.601 ng
RT: 17.052 min Scan# 1709
Delta R.T. -0.012 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:266 Resp: 21458
Ion Ratio Lower Upper
266 100
264 63.2 49.8 74.6
268 64.0 49.6 74.4

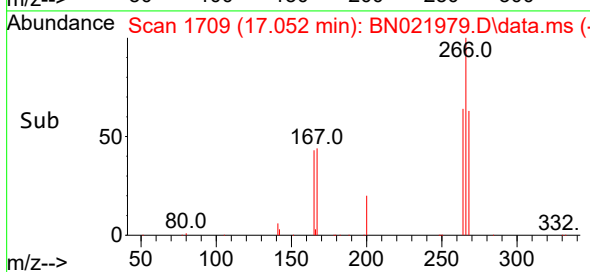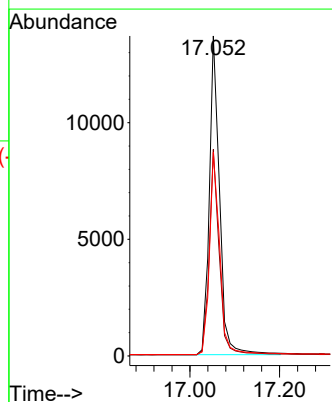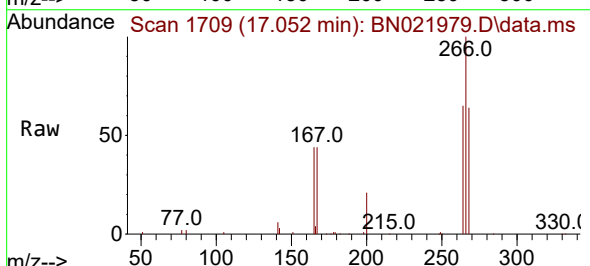



#25

Phenanthrene

Concen: 4.965 ng

RT: 17.449 min Scan# 1741

Delta R.T. 0.000 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:178 Resp: 226895

Ion Ratio Lower Upper

178 100

176 19.4 15.4 23.0

179 15.2 12.2 18.2

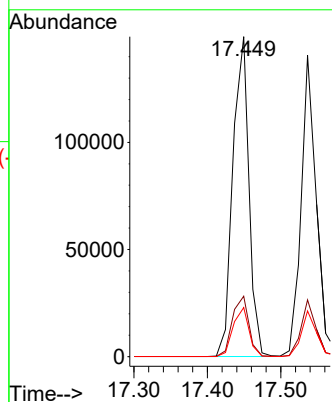

#26

Anthracene

Concen: 5.479 ng

RT: 17.536 min Scan# 1748

Delta R.T. 0.000 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37




Tgt Ion:178 Resp: 204527


Ion Ratio Lower Upper

178 100

176 18.6 14.8 22.2

179 15.3 12.2 18.2


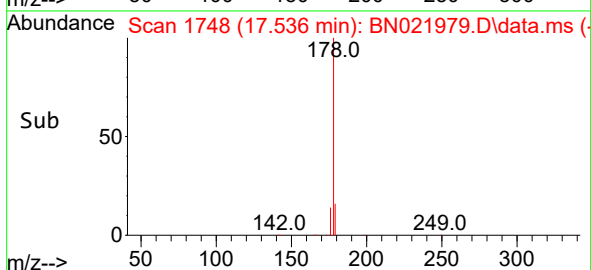






#27
Fluoranthene-d10
Concen: 5.078 ng
RT: 19.441 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 182908
Ion Ratio Lower Upper
212 100
106 18.9 15.2 22.8
104 10.6 8.6 13.0

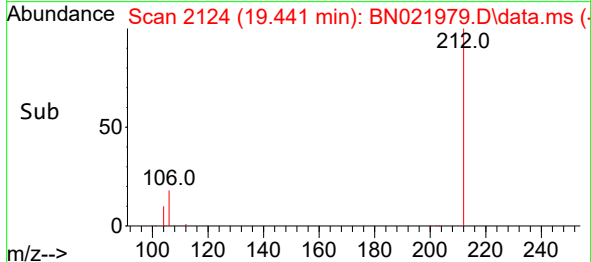

#28
Fluoranthene
Concen: 5.106 ng
RT: 19.470 min Scan# 2131
Delta R.T. -0.004 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:202 Resp: 251830
Ion Ratio Lower Upper
202 100
101 14.2 11.4 17.0
203 17.3 13.5 20.3

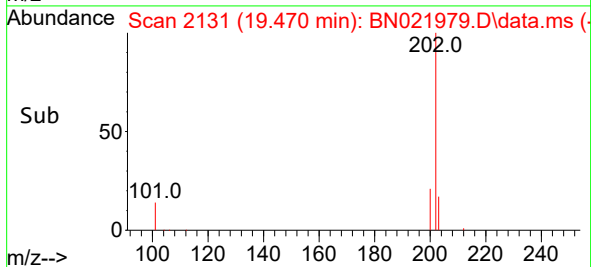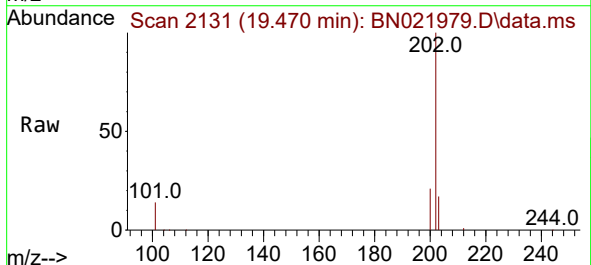

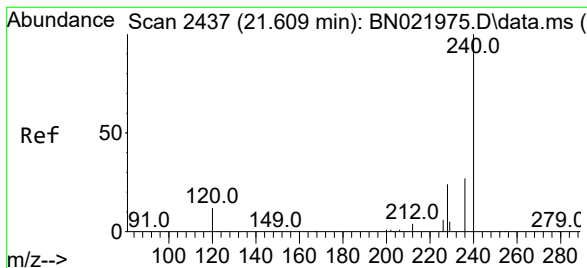

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.600 min Scan# 2437

Delta R.T. -0.009 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:240 Resp: 11931

Ion Ratio Lower Upper

240 100

120 21.4 11.8 17.6#

236 28.5 22.4 33.6

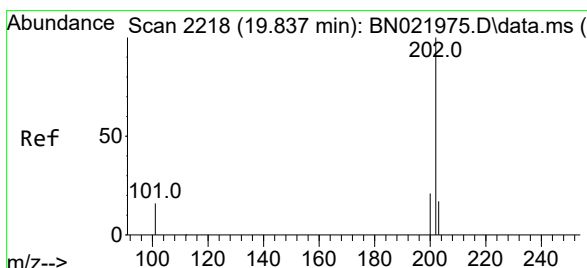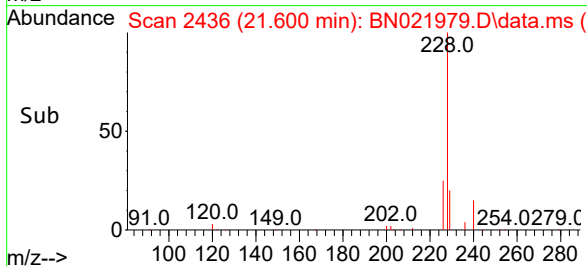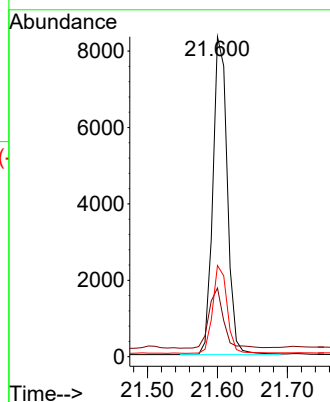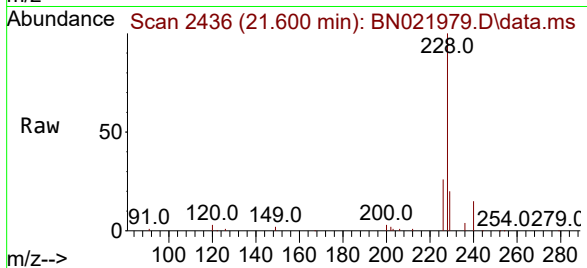

#30

Pyrene

Concen: 4.732 ng

RT: 19.837 min Scan# 2218

Delta R.T. 0.000 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37




Tgt Ion:202 Resp: 253804


Ion Ratio Lower Upper

202 100

200 21.0 16.6 25.0

203 17.8 14.1 21.1

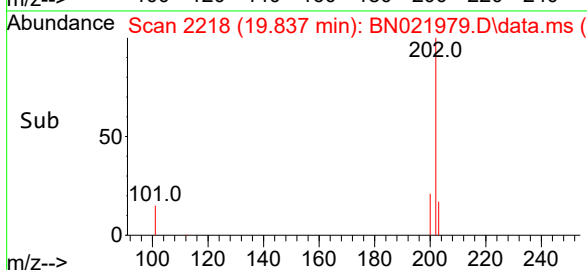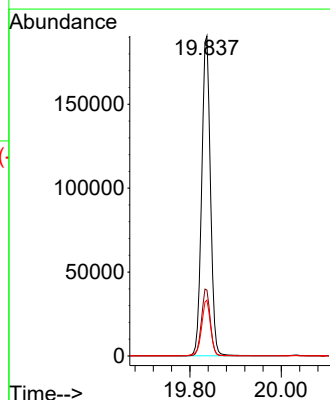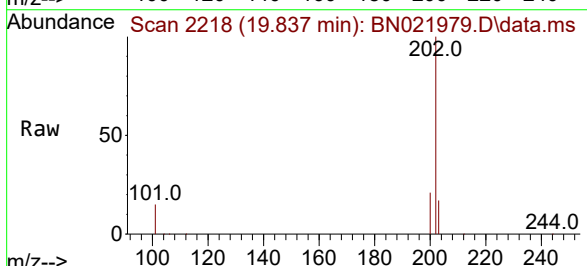

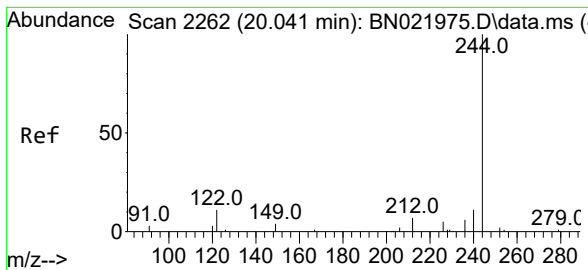

#31

Terphenyl-d14

Concen: 4.575 ng

RT: 20.033 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:244 Resp: 110031

Ion Ratio Lower Upper

244 100

212 9.2 6.5 9.7

122 18.9 9.1 13.7#

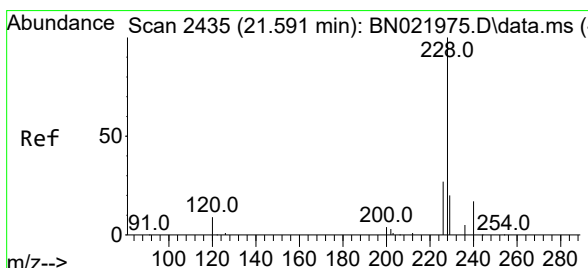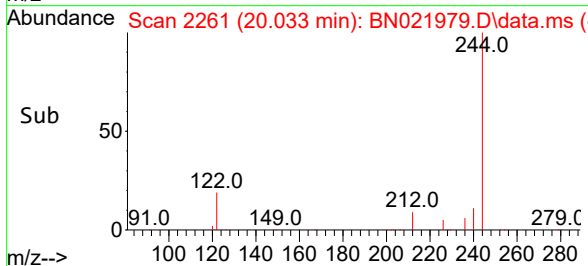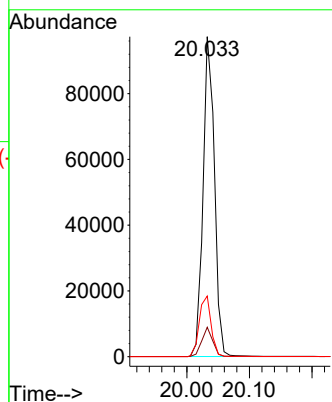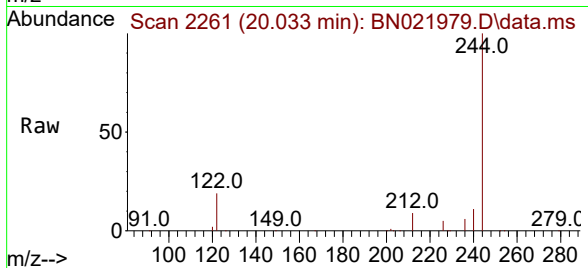

#32

Benzo(a)anthracene

Concen: 5.068 ng

RT: 21.591 min Scan# 2435

Delta R.T. 0.000 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37




Tgt Ion:228 Resp: 233644


Ion Ratio Lower Upper

228 100

226 26.7 22.2 33.4

229 19.7 16.2 24.2

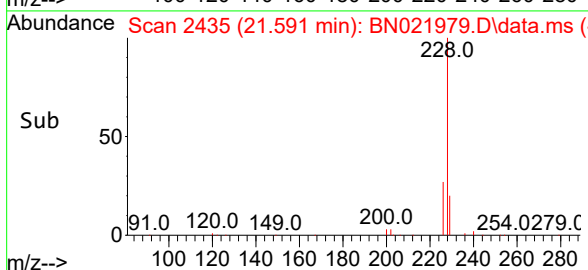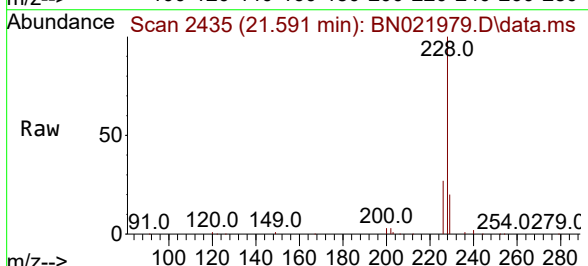

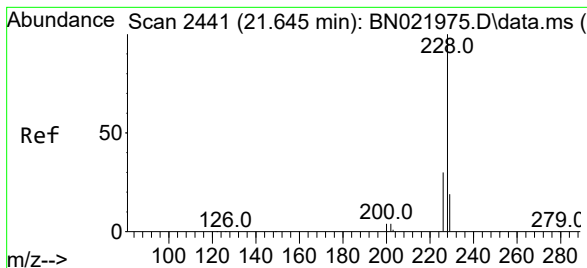

#33

Chrysene

Concen: 4.715 ng

RT: 21.645 min Scan# 2441

Delta R.T. 0.000 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 234929

Ion Ratio Lower Upper

228 100

226 29.6 24.2 36.2

229 19.5 15.8 23.6

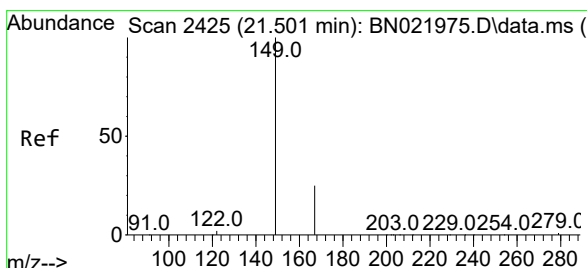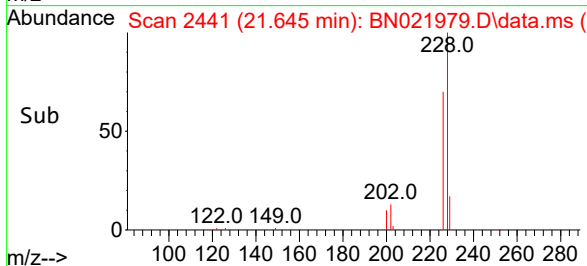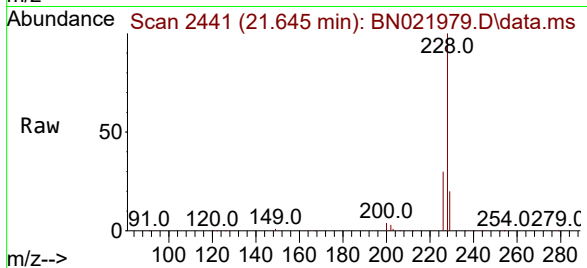

#34

Bis(2-ethylhexyl)phthalate

Concen: 5.096 ng

RT: 21.501 min Scan# 2425

Delta R.T. 0.000 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37




Tgt Ion:149 Resp: 117641


Ion Ratio Lower Upper

149 100

167 26.3 20.2 30.4

279 2.5 2.3 3.5

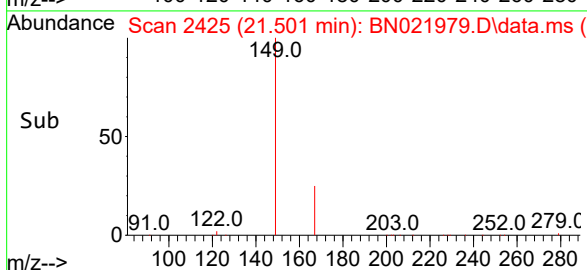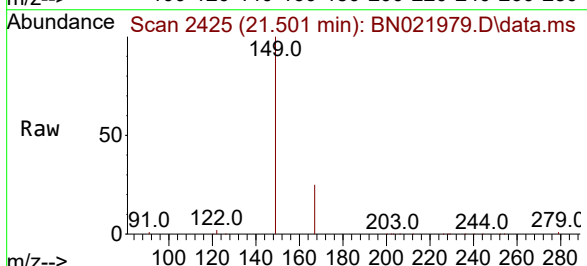







#35
Perylene-d12
Concen: 0.400 ng
RT: 24.084 min Scan# 3100
Delta R.T. -0.003 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:264 Resp: 8961




Ion	Ratio	Lower	Upper
264	100		
260	27.2	21.3	31.9
265	71.5	63.0	94.4

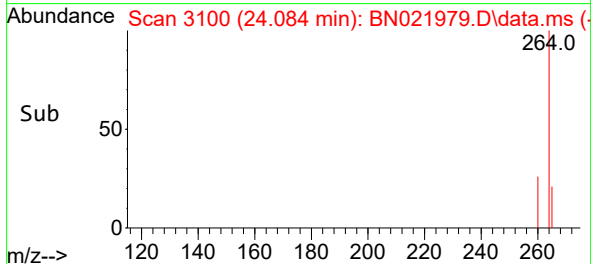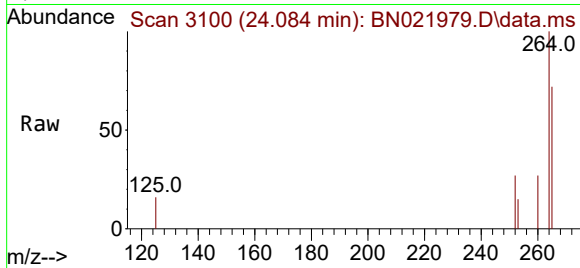


#36
Indeno(1,2,3-cd)pyrene
Concen: 5.267 ng
RT: 26.686 min Scan# 3990
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Tgt Ion:276 Resp: 235000

Ion	Ratio	Lower	Upper
276	100		
138	34.1	28.0	42.0
277	24.7	19.8	29.8

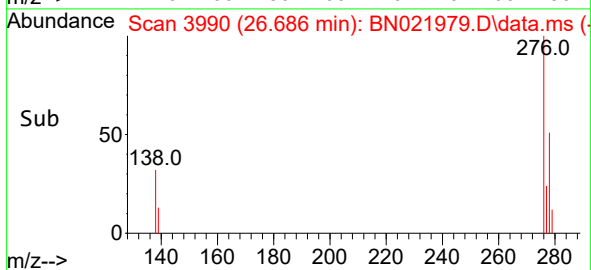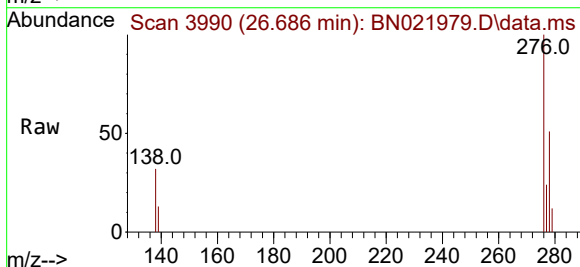



#37

Benzo(b)fluoranthene

Concen: 4.949 ng

RT: 23.318 min Scan# 2838

Delta R.T. -0.006 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 213758

Ion Ratio Lower Upper

252 100

253 21.6 20.6 31.0

125 14.0 15.6 23.4#

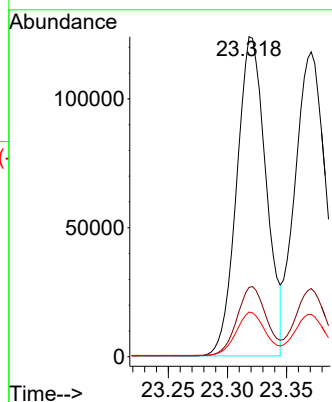

#38

Benzo(k)fluoranthene

Concen: 5.131 ng

RT: 23.371 min Scan# 2856

Delta R.T. -0.003 min

Lab File: BN021979.D

Acq: 03 Oct 2022 15:37




Tgt Ion:252 Resp: 216488


Ion Ratio Lower Upper

252 100

253 22.4 20.4 30.6


125 13.9 15.8 23.6#

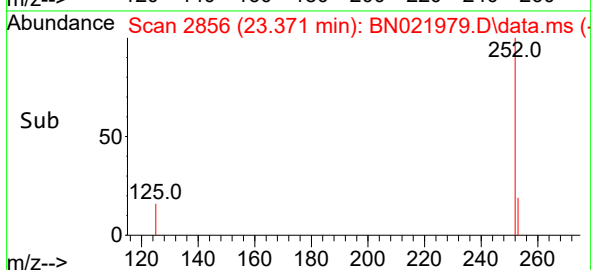






#39
Benzo(a)pyrene
Concen: 5.278 ng
RT: 23.970 min Scan# 3061
Delta R.T. -0.006 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:252 Resp: 171351
Ion Ratio Lower Upper
252 100
253 21.6 23.2 34.8#
125 15.4 21.1 31.7#

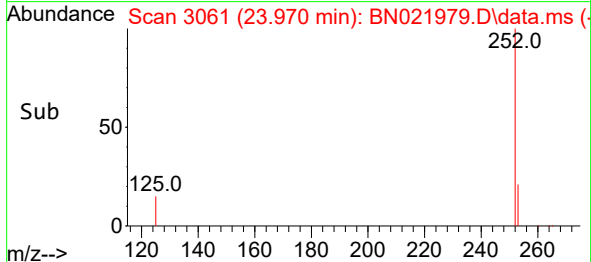

#40
Dibenzo(a,h)anthracene
Concen: 5.220 ng
RT: 26.707 min Scan# 3997
Delta R.T. -0.006 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37


Tgt Ion:278 Resp: 186240
Ion Ratio Lower Upper
278 100
139 23.2 19.9 29.9
279 23.7 21.9 32.9

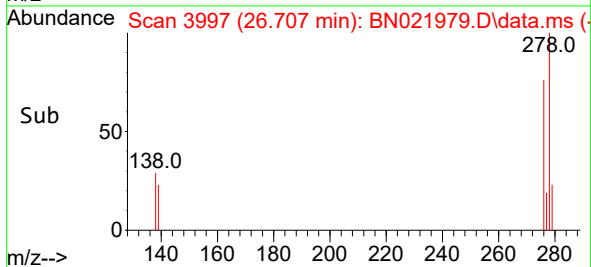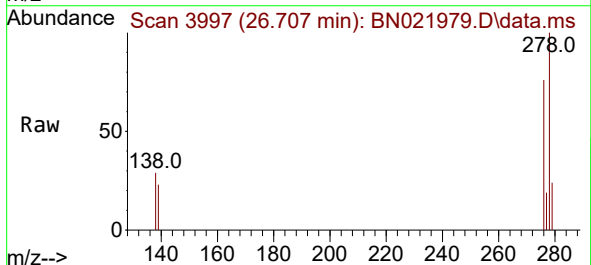



#41
Benzo(g,h,i)perylene
Concen: 5.232 ng
RT: 27.487 min Scan# 41
Delta R.T. 0.000 min
Lab File: BN021979.D
Acq: 03 Oct 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

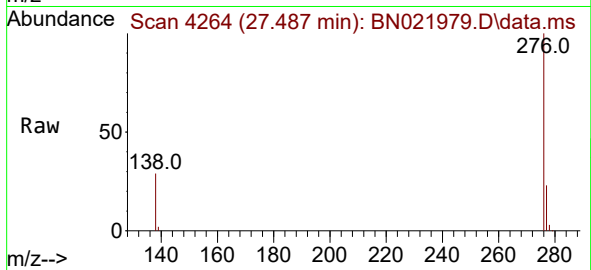

Tgt Ion:276 Resp: 194946
Ion Ratio Lower Upper
276 100
277 23.5 20.0 30.0
138 29.2 25.2 37.8

