


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
 Data File : BN021971.D
 Acq On : 03 Oct 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 01:32:21 2022

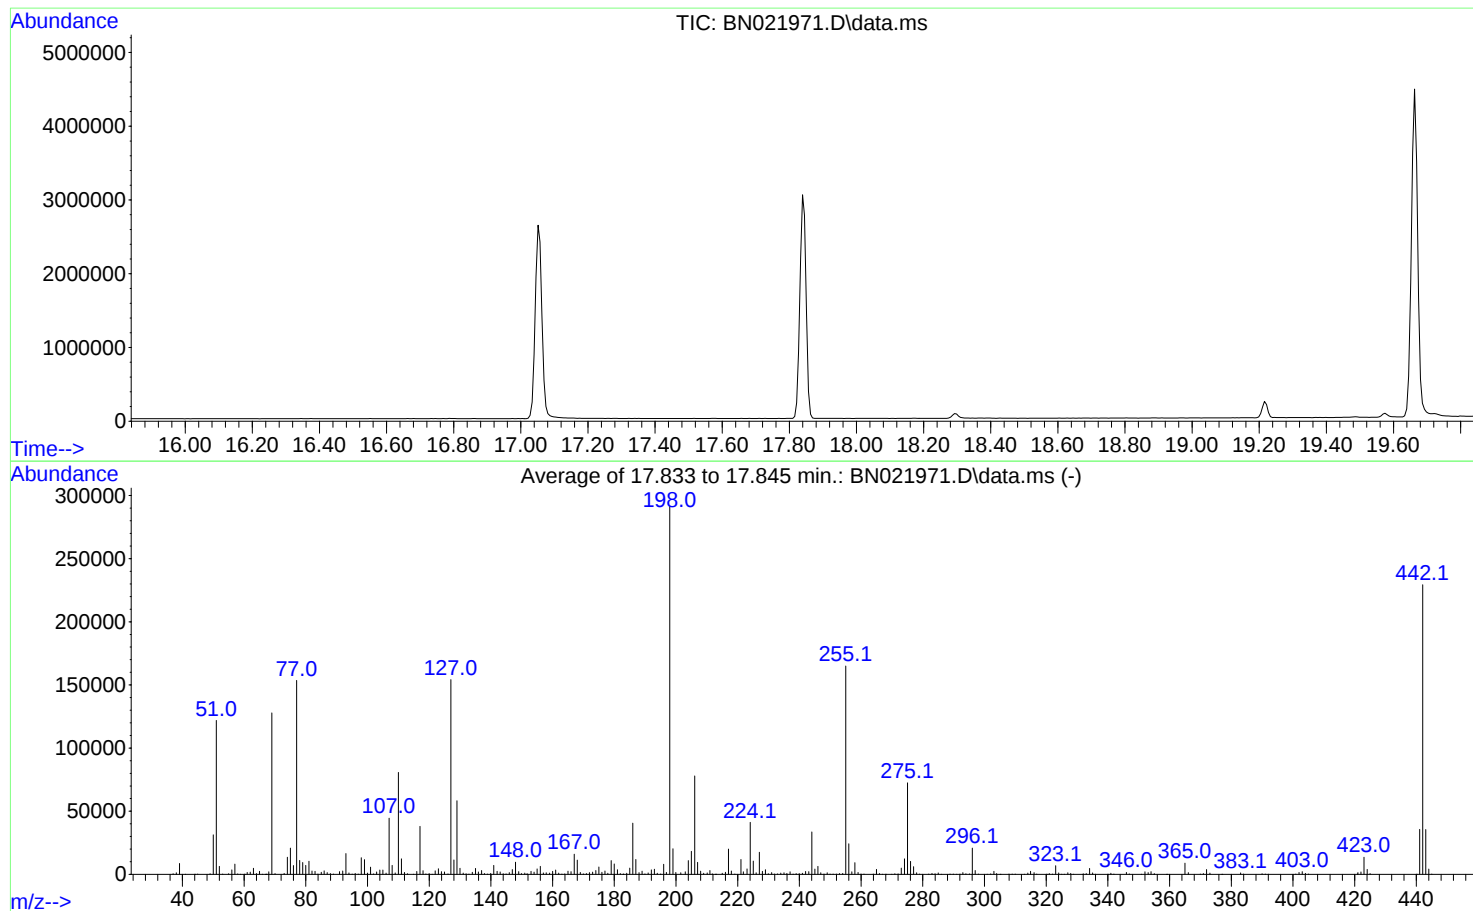




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	121882	PASS
68	69	0.00	2	1.6	2087	PASS
69	198	0.00	100	43.9	127835	PASS
70	69	0.00	2	0.5	691	PASS
127	198	10	80	52.9	154219	PASS
197	198	0.00	2	0.5	1484	PASS
198	198	100	100	100.0	291307	PASS
199	198	5	9	7.0	20309	PASS
275	198	10	60	24.9	72531	PASS
365	198	1	100	3.1	8938	PASS
441	198	0.01	100	12.2	35672	PASS
442	442	50	100	100.0	229333	PASS
443	442	15	24	15.5	35536	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
 Data File : BN021971.D
 Acq On : 03 Oct 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 04 05:09:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 05:09:49 2022
 Response via : Initial Calibration

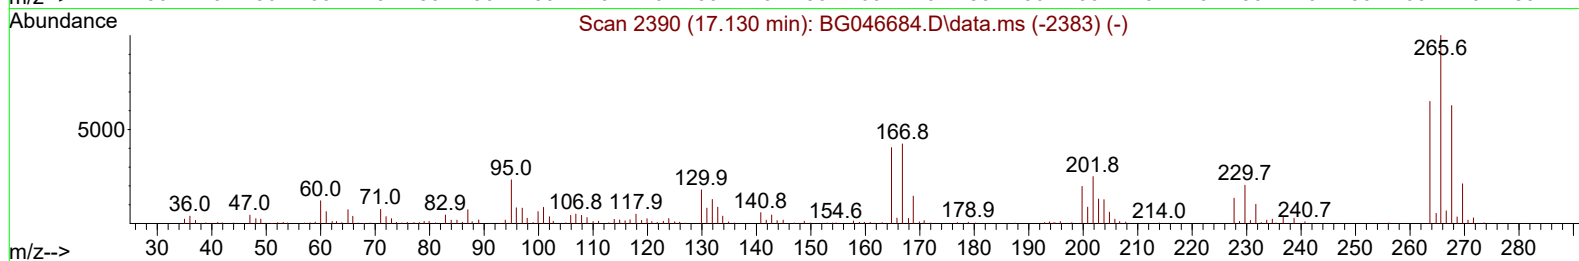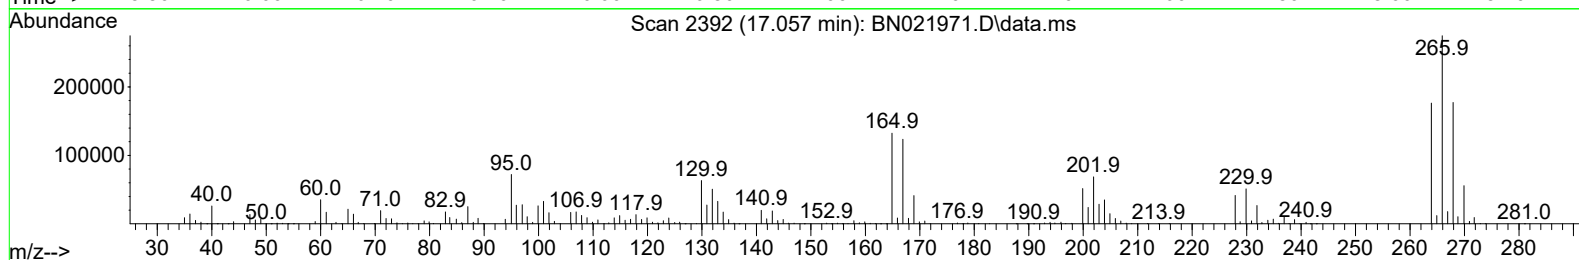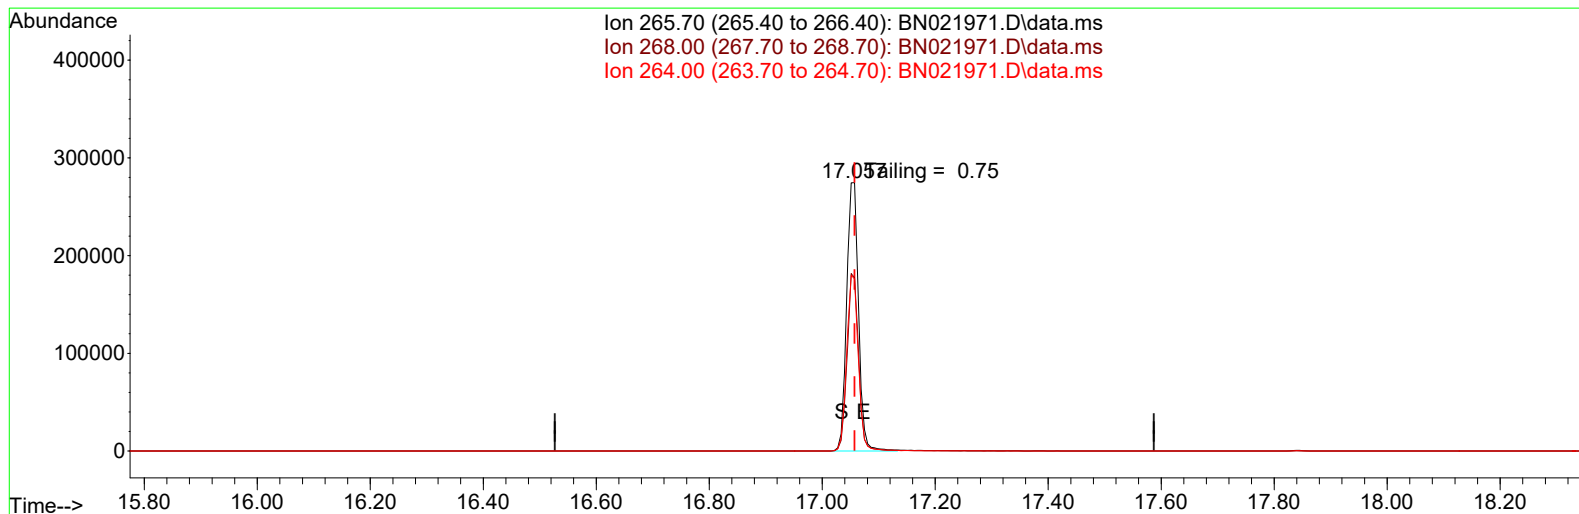

TIC: BN021971.D\data.ms

(70) Pentachlorophenol (C)

17.057min (0.000) 25380.90 ng




response 402947

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.56
264.00	61.60	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
Data File : BN021971.D
Acq On : 03 Oct 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 05:09:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 05:09:49 2022
Response via : Initial Calibration

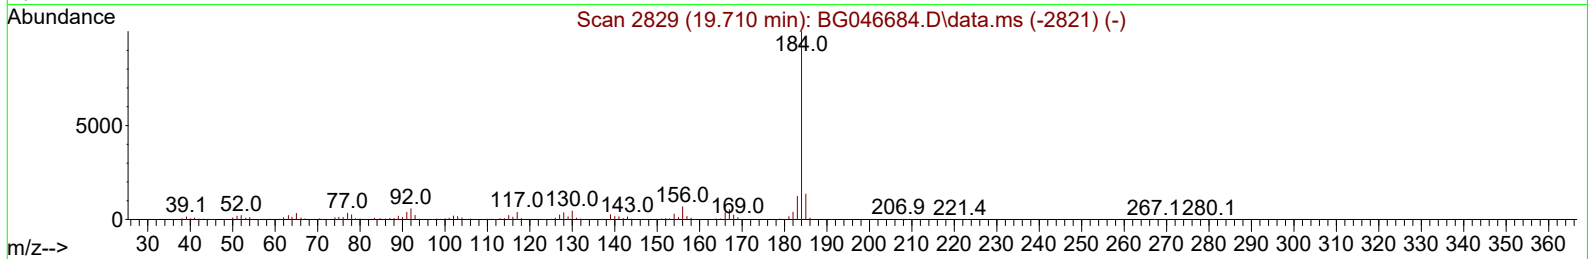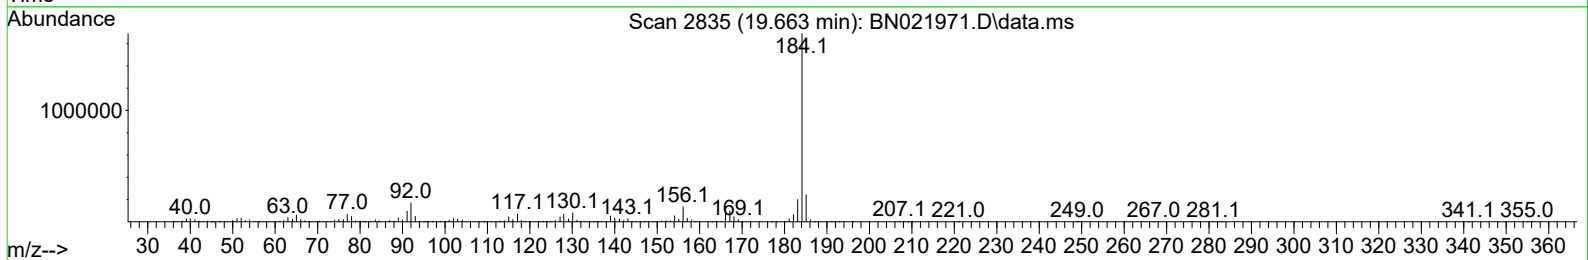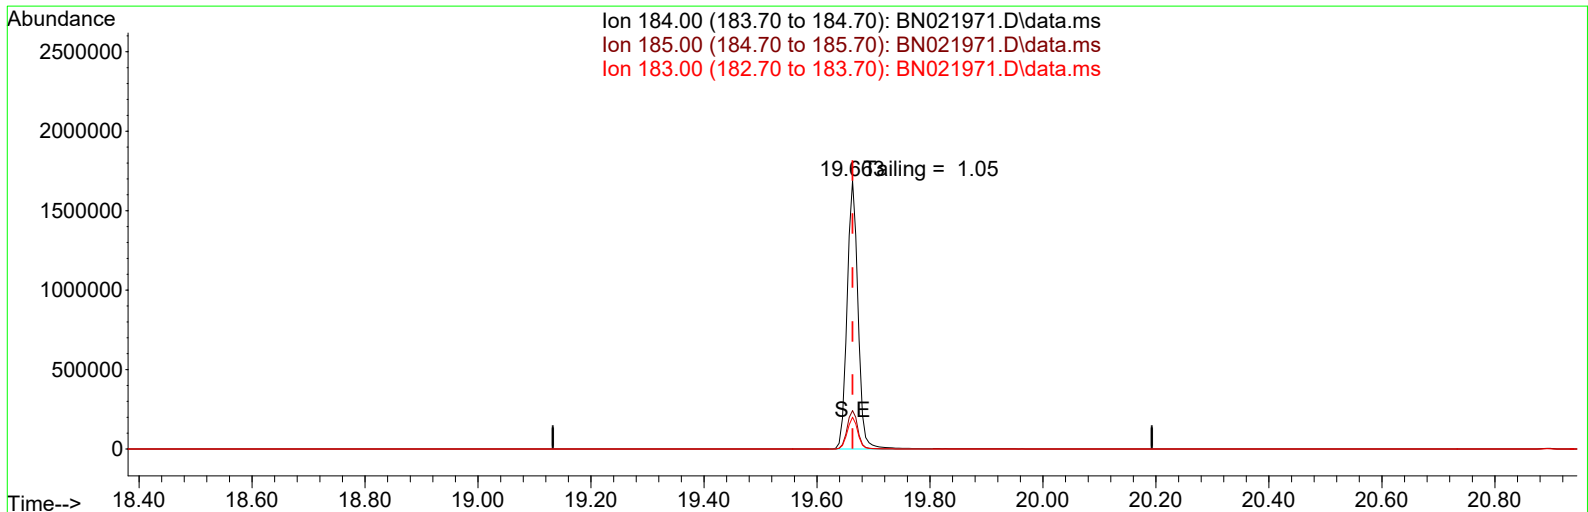

TIC: BN021971.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 2276582

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2022	BNA_N	<u>BN021971.D</u>
Compound Name	Response	Retention Time
DDT	1133486	20.892
DDD	8985	20.451
DDE	425	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9410	1142896	0.82

Instrument :
BNA_N
ClientSampleId :
DFTPP