


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
 Data File : BN021982.D
 Acq On : 03 Oct 2022 18:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 01:32:21 2022

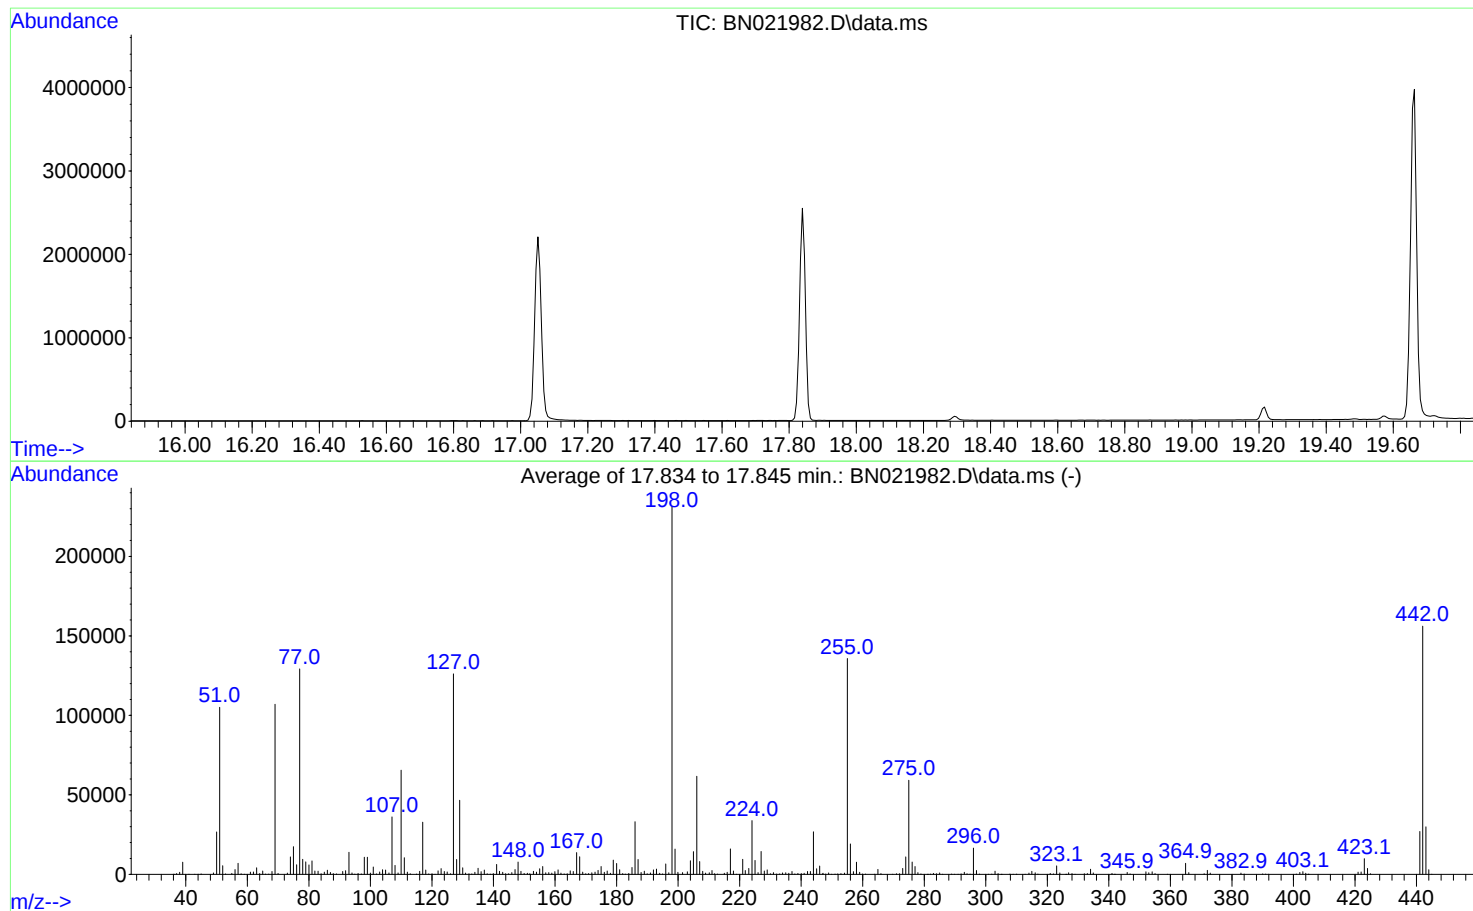




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	105109	PASS
68	69	0.00	2	1.7	1788	PASS
69	198	0.00	100	46.2	106987	PASS
70	69	0.00	2	0.6	628	PASS
127	198	10	80	54.5	126072	PASS
197	198	0.00	2	0.4	1012	PASS
198	198	100	100	100.0	231381	PASS
199	198	5	9	6.9	15892	PASS
275	198	10	60	25.6	59208	PASS
365	198	1	100	3.0	6991	PASS
441	198	0.01	100	11.7	26960	PASS
442	442	50	100	100.0	156109	PASS
443	442	15	24	19.1	29888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100322\
Data File : BN021982.D
Acq On : 03 Oct 2022 18:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 05:11:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 05:09:49 2022
Response via : Initial Calibration

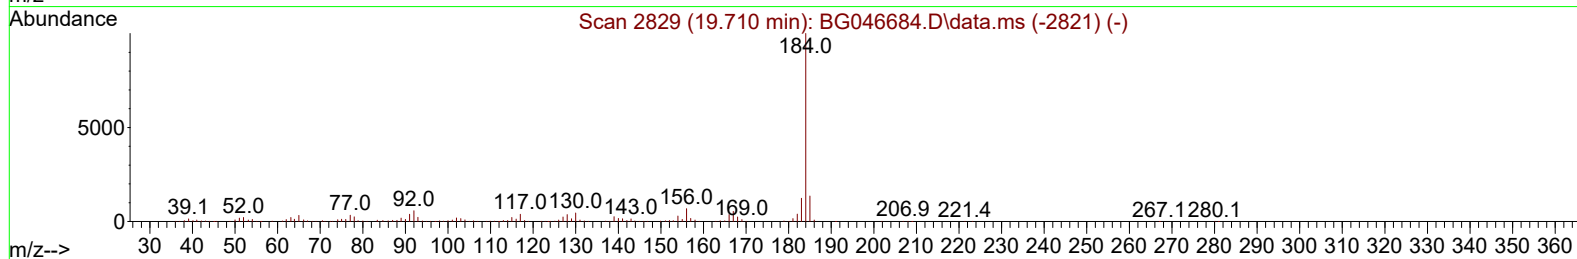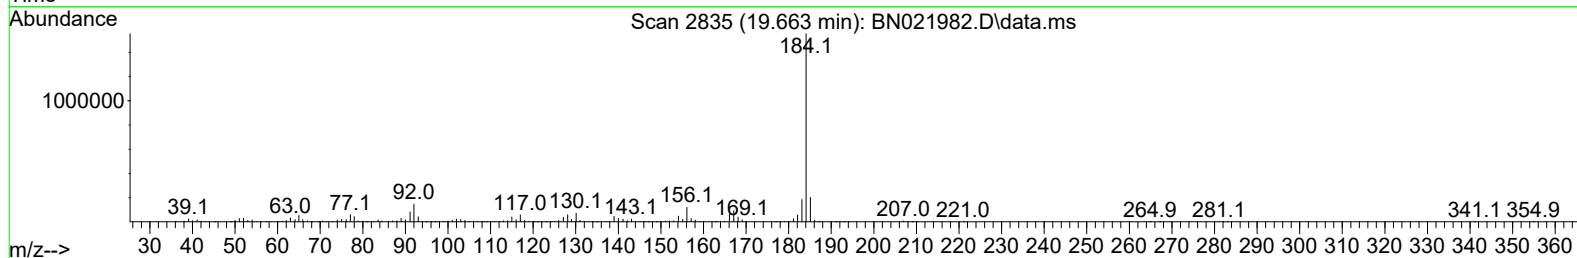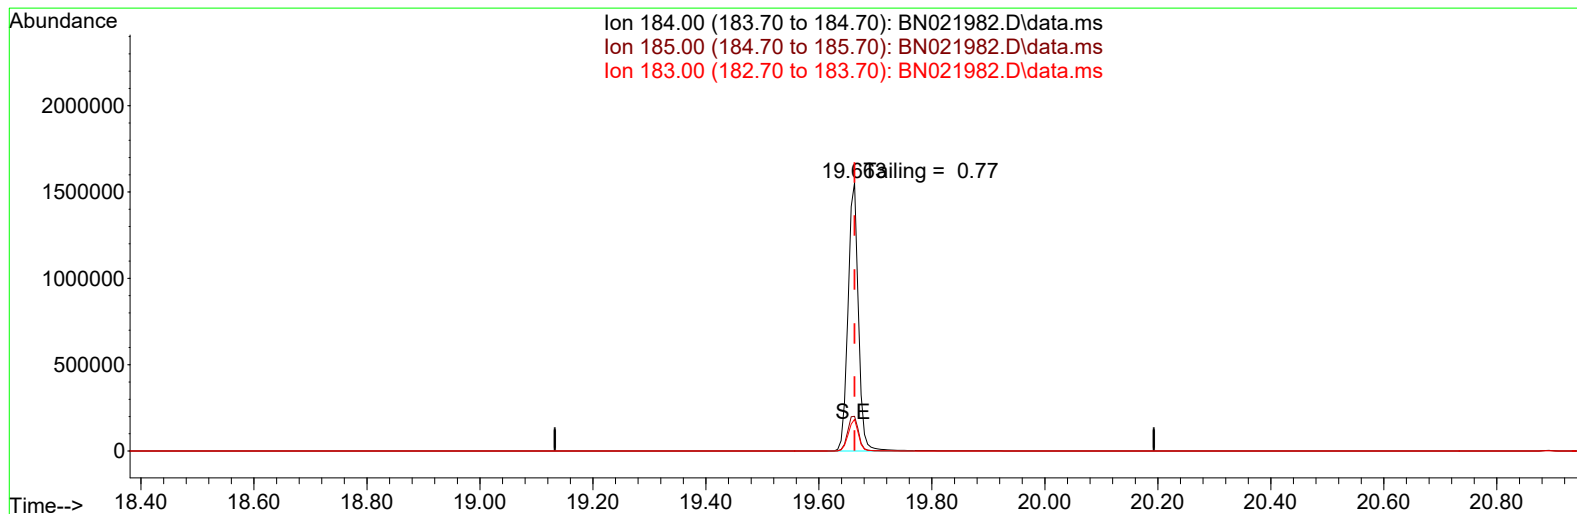

TIC: BN021982.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 0.00 ng

response 1989397

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.98
183.00	13.20	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2022	BNA_N	<u>BN021982.D</u>
Compound Name	Response	Retention Time
DDT	979207	20.892
DDD	7083	20.451
DDE	195	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7278	986485	0.74

Instrument :
BNA_N
ClientSampleId :
DFTPP