

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
 Data File : BN028016.D
 Acq On : 03 Oct 2023 19:06
 Operator : MA/JU
 Sample : PB155901BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK901

Quant Time: Oct 04 04:08:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	4410	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	15096	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	8978	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.346	188	19066	0.400	ng/ul	0.00
17) Chrysene-d12	21.533	240	16248	0.400	ng/ul	0.00
23) Perylene-d12	24.000	264	16732	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	35690	6.443	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	7603	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	17149	0.333	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.587	166	2610	0.072	ng/ul#	14
20) Pyrene	19.743	202	2434	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.840	252	4983	0.094	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
Data File : BN028016.D
Acq On : 03 Oct 2023 19:06
Operator : MA/JU
Sample : PB155901BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK901

Quant Time: Oct 04 04:08:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration




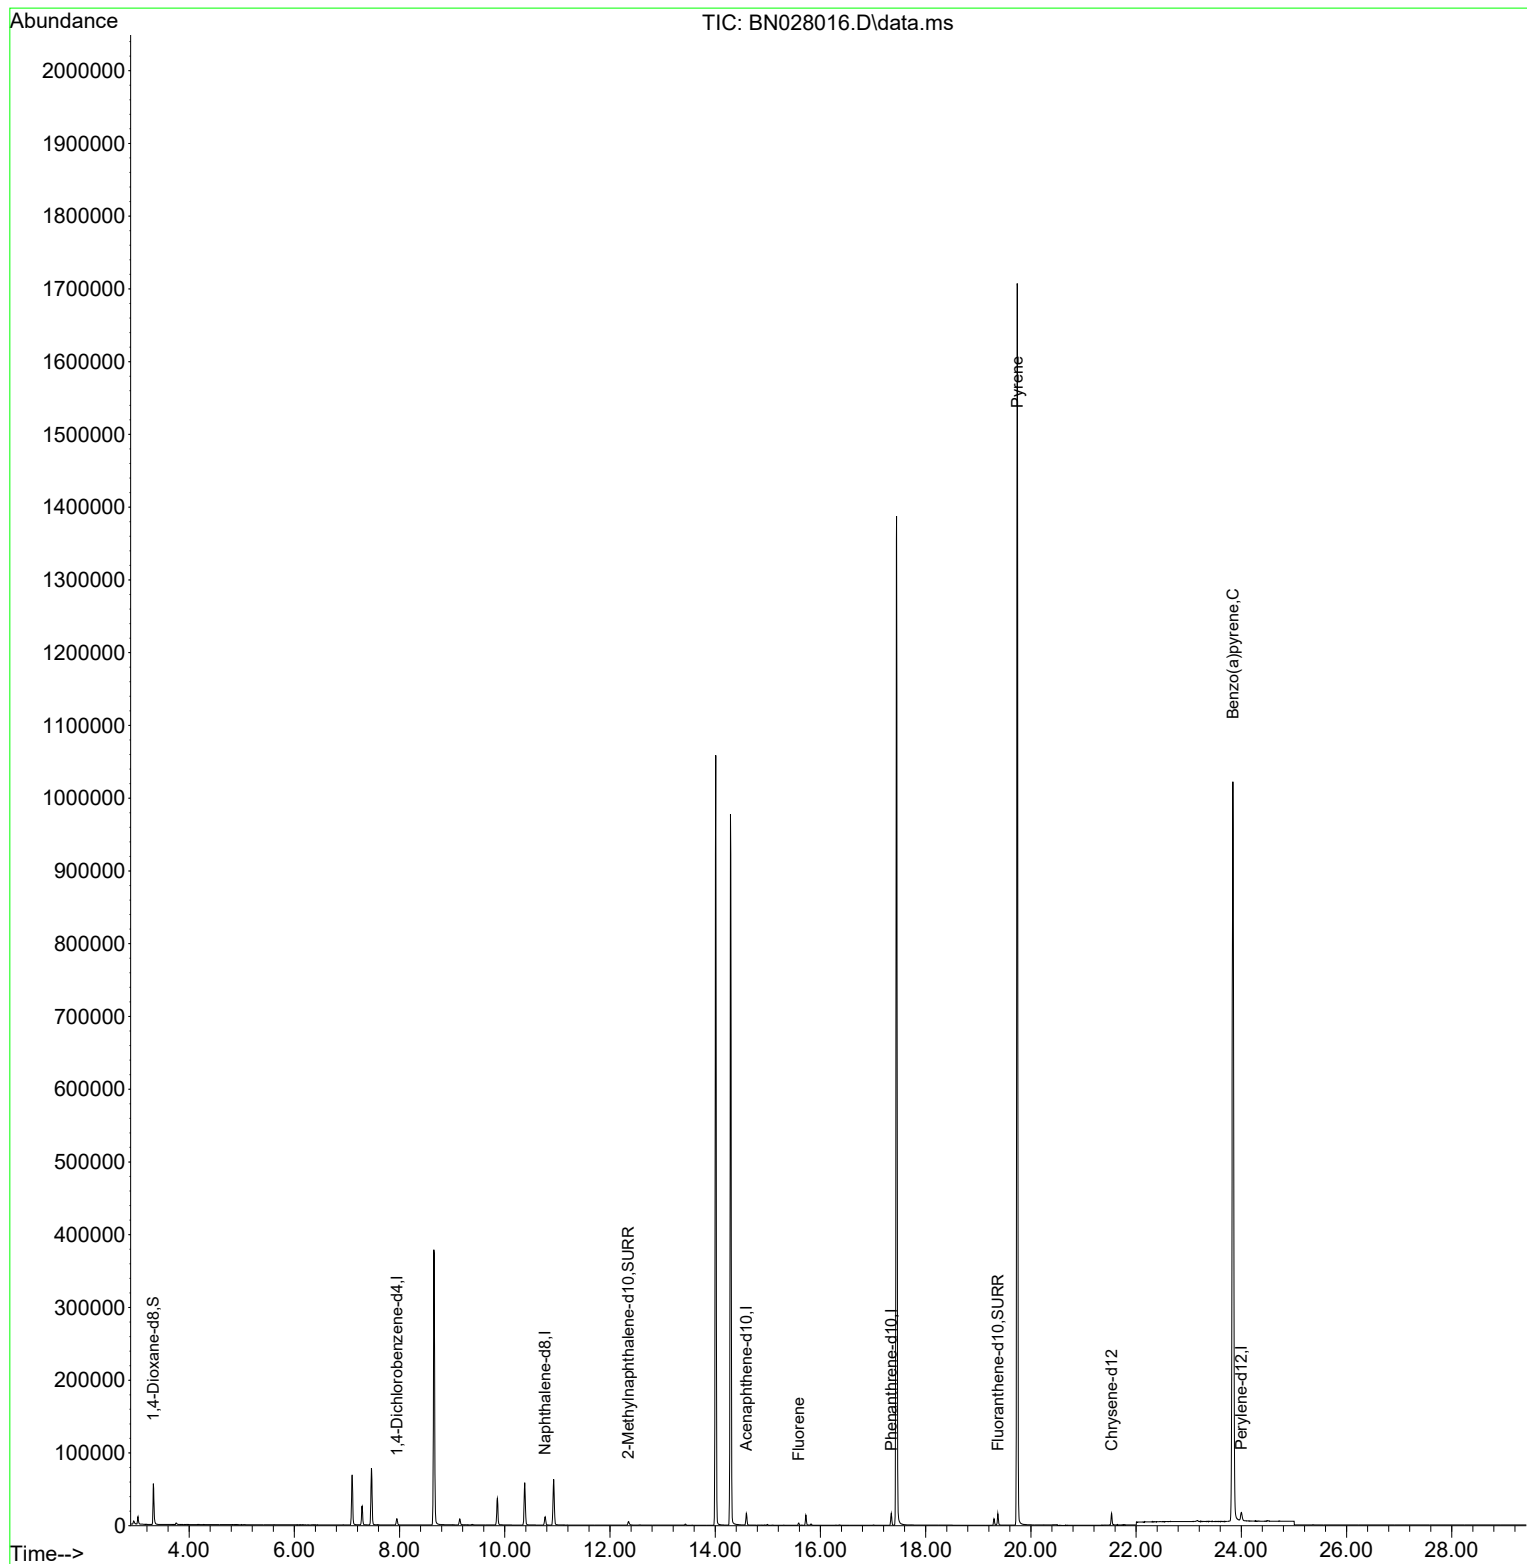


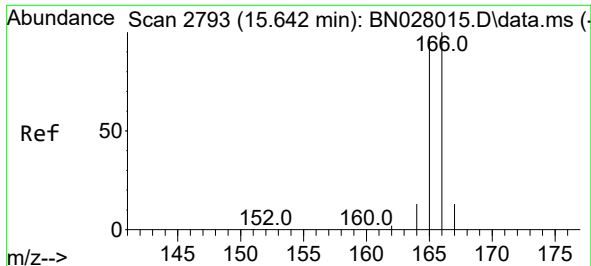

#12
Fluorene
Concen: 0.072 ng/ul
RT: 15.587 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN028016.D
Acq: 03 Oct 2023 19:06




Instrument :
BNA_N
ClientSampleId :
SBLK901


Tgt Ion:166 Resp: 2610
Ion Ratio Lower Upper
166 100
165 8.2 78.5 117.7#
167 36.0 11.2 16.8#

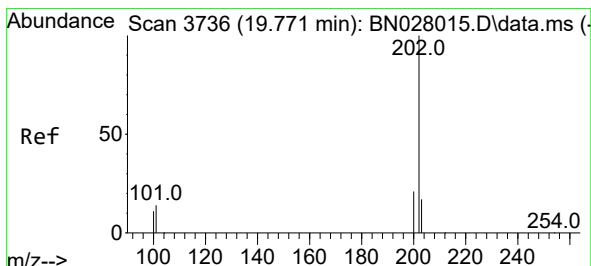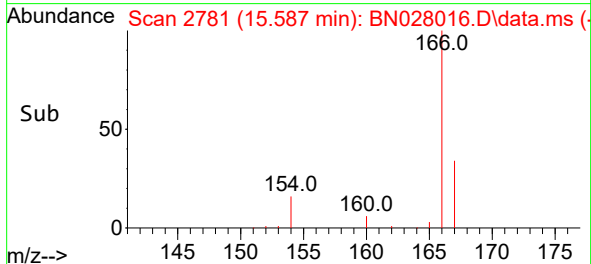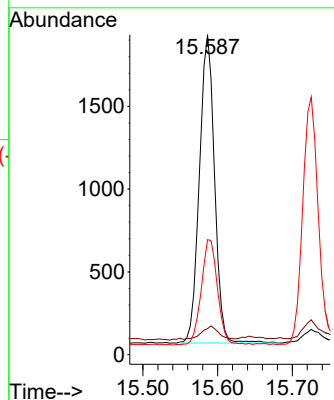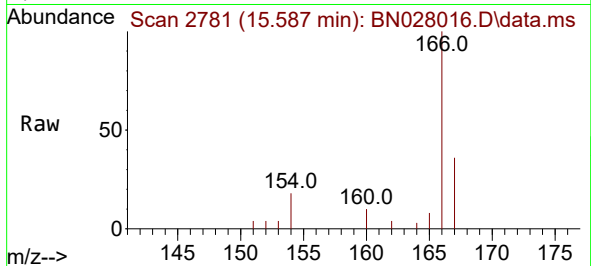

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.743 min Scan# 3730
Delta R.T. -0.028 min
Lab File: BN028016.D
Acq: 03 Oct 2023 19:06


Tgt Ion:202 Resp: 2434
Ion Ratio Lower Upper
202 100
101 157.0 11.2 16.8#
100 1074.6 9.1 13.7#

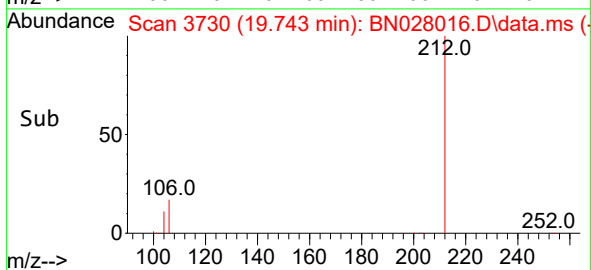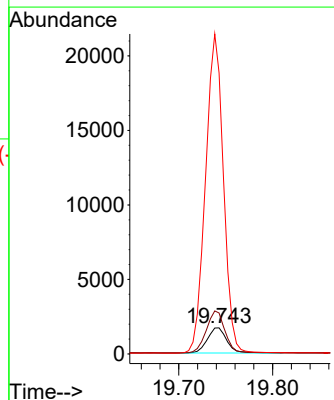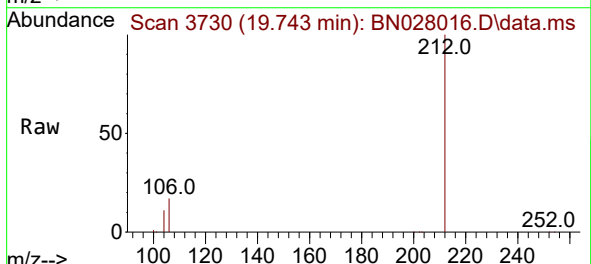

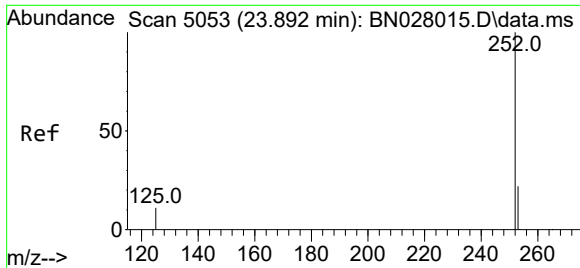

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.840 min Scan# 50
Delta R.T. -0.055 min
Lab File: BN028016.D
Acq: 03 Oct 2023 19:06

Instrument :
BNA_N
ClientSampleId :
SBLK901

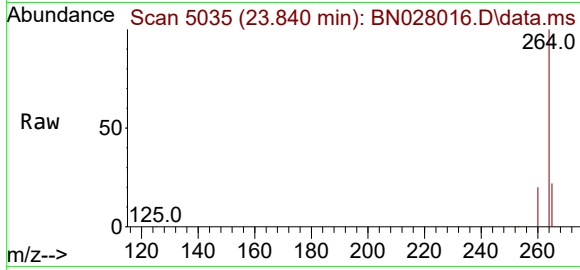

Tgt Ion:252 Resp: 4983
Ion Ratio Lower Upper
252 100
253 54.1 23.4 35.2#
125 42.9 15.3 22.9#

