

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
 Data File : BN028019.D
 Acq On : 03 Oct 2023 20:58
 Operator : MA/JU
 Sample : 04480-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJN2

Quant Time: Oct 04 04:08:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	3580	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	11952	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	7191	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.346	188	15972	0.400	ng/ul	0.00
17) Chrysene-d12	21.533	240	14133	0.400	ng/ul	0.00
23) Perylene-d12	24.000	264	14269	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	14675	3.264	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	3949	0.205	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	11414	0.255	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.359	88	1190	0.250	ng/ul#	85
20) Pyrene	19.738	202	1937	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.837	252	3280	0.073	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
Data File : BN028019.D
Acq On : 03 Oct 2023 20:58
Operator : MA/JU
Sample : 04480-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJN2

Quant Time: Oct 04 04:08:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration




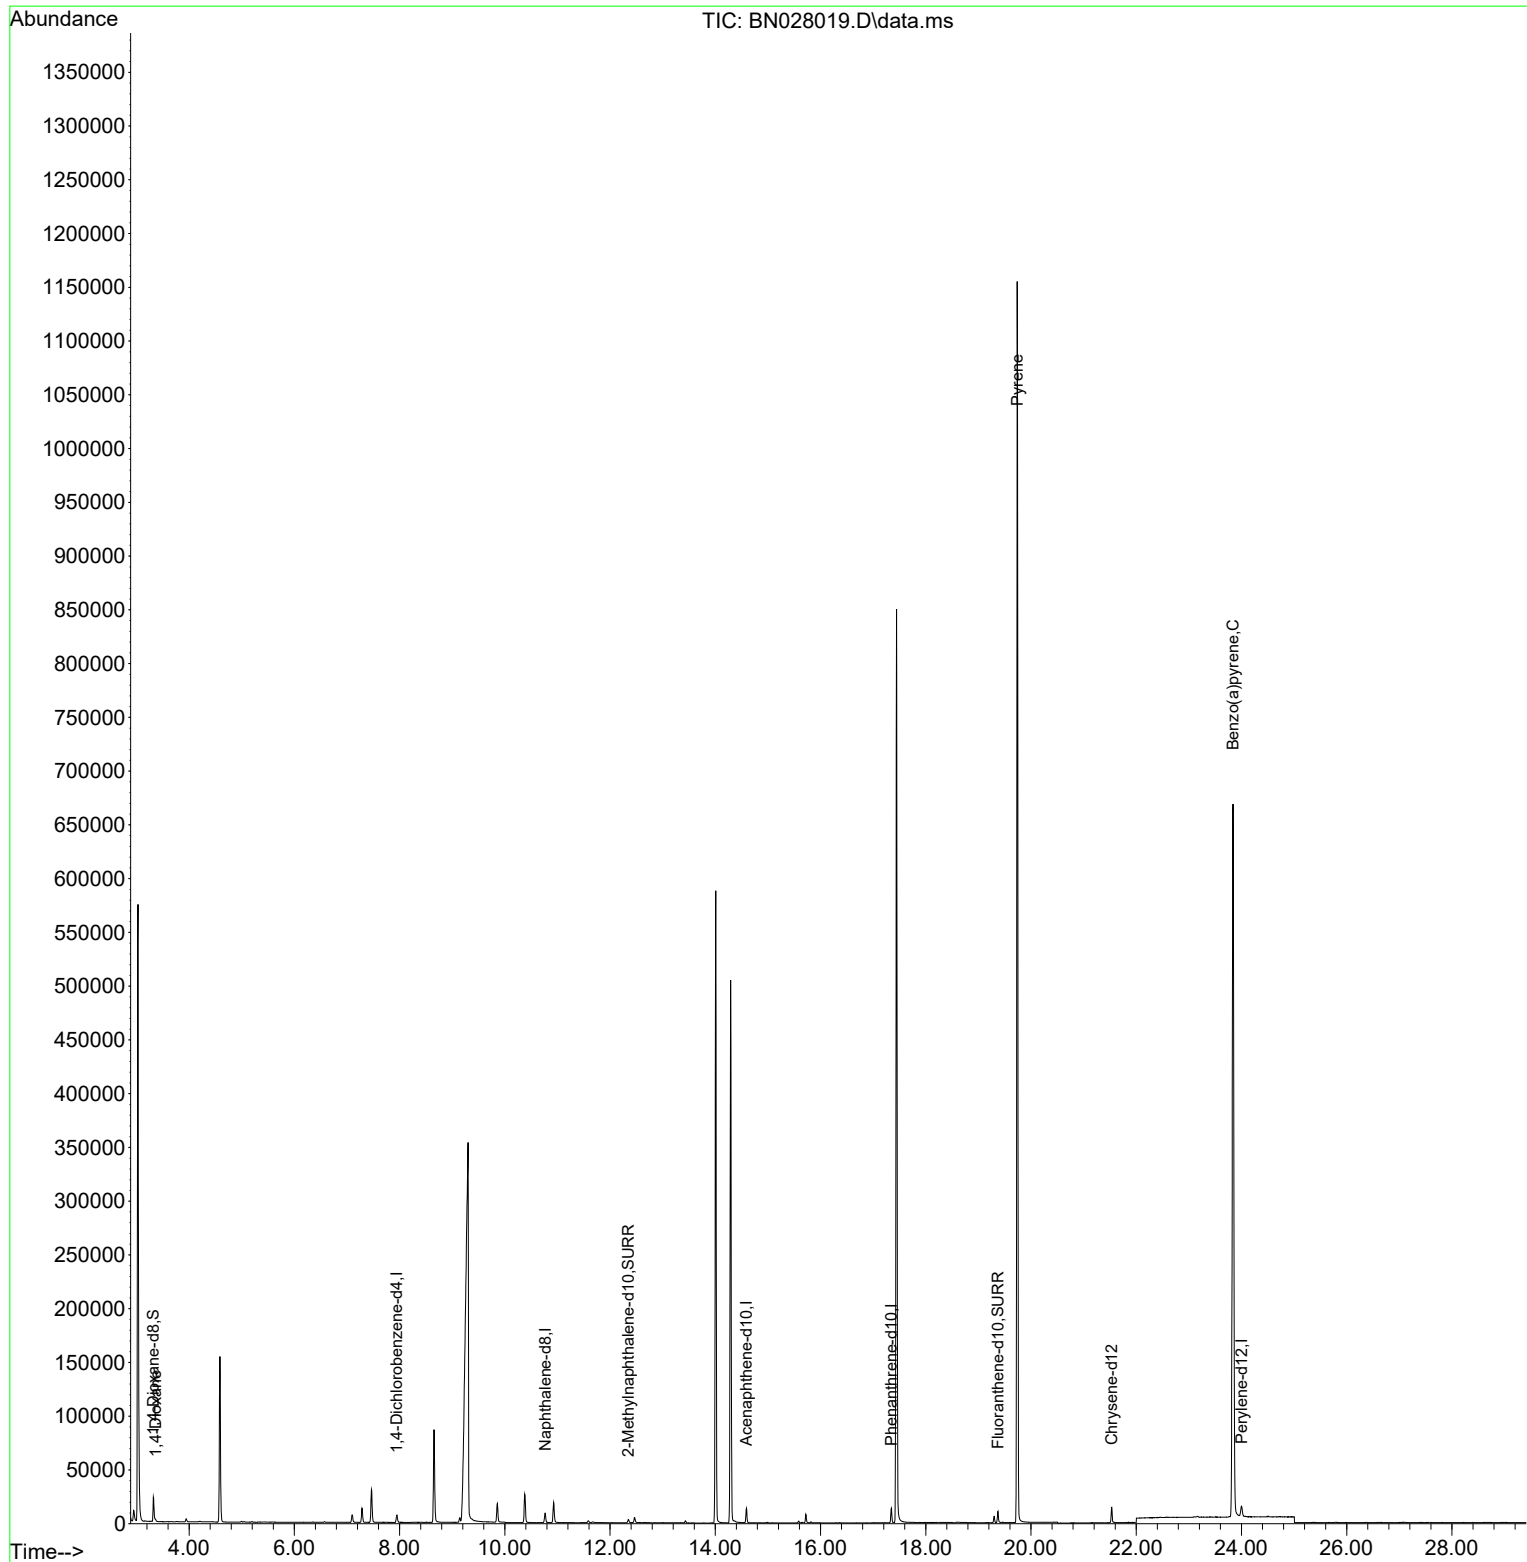


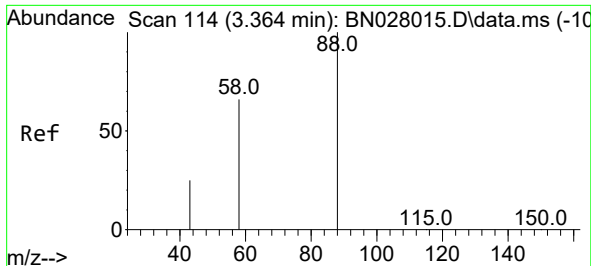

#2
1,4-Dioxane
Concen: 0.250 ng/ul
RT: 3.359 min Scan# 114
Delta R.T. -0.004 min
Lab File: BN028019.D
Acq: 03 Oct 2023 20:58




Instrument :
BNA_N
ClientSampleId :
BBJN2


Tgt Ion: 88 Resp: 1190
Ion Ratio Lower Upper
88 100
43 61.4 33.4 50.2#
58 54.3 45.7 68.5

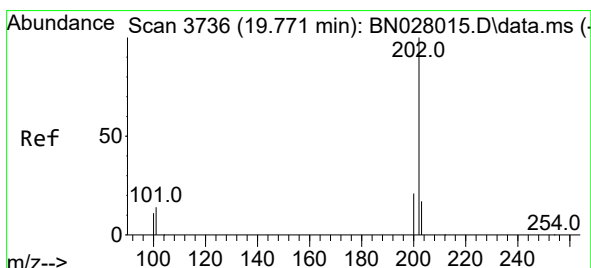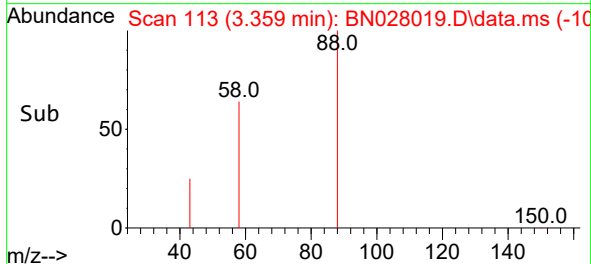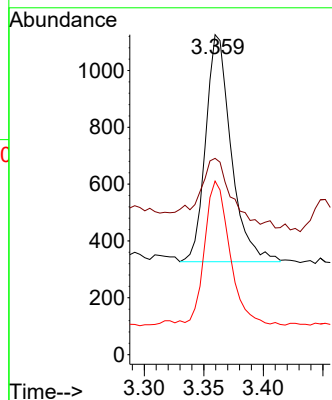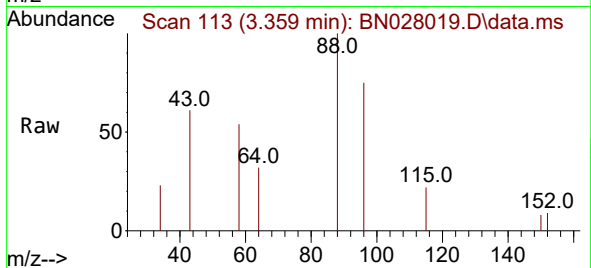

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.738 min Scan# 3729
Delta R.T. -0.032 min
Lab File: BN028019.D
Acq: 03 Oct 2023 20:58


Tgt Ion: 202 Resp: 1937
Ion Ratio Lower Upper
202 100
101 156.3 11.2 16.8#
100 1109.4 9.1 13.7#

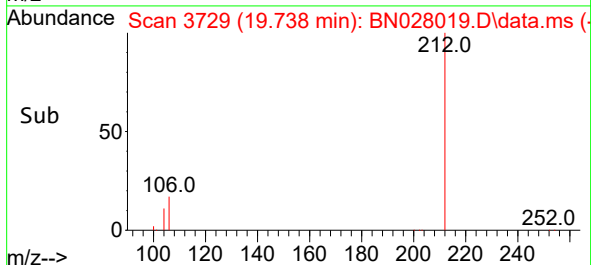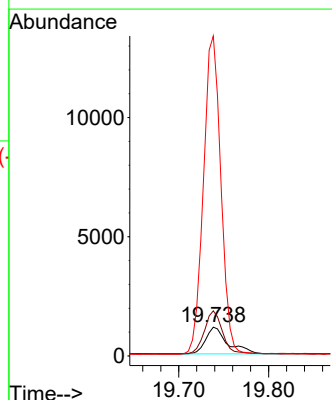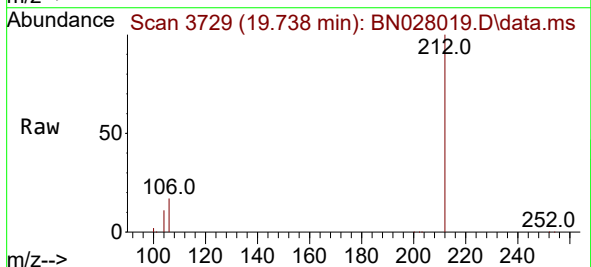

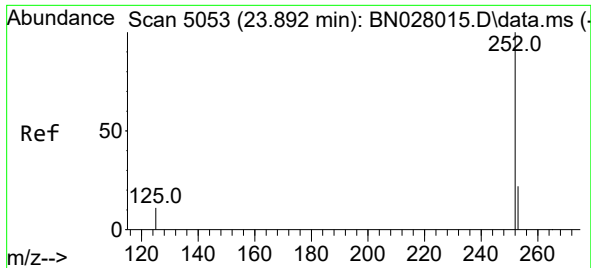

#26
 Benzo(a)pyrene
 Concen: 0.073 ng/ul
 RT: 23.837 min Scan# 50
 Delta R.T. -0.058 min
 Lab File: BN028019.D
 Acq: 03 Oct 2023 20:58

Instrument :
 BNA_N
 ClientSampleId :
 BBJN2

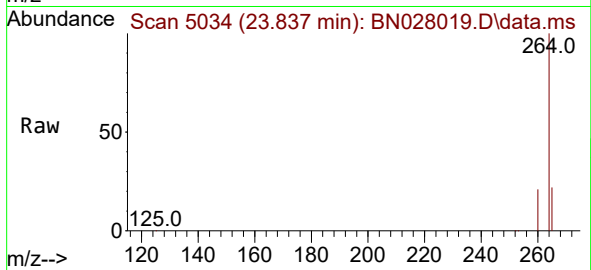

Tgt Ion:252 Resp: 3280
 Ion Ratio Lower Upper
 252 100
 253 66.6 23.4 35.2#
 125 55.5 15.3 22.9#

