

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
 Data File : BN028026.D
 Acq On : 04 Oct 2023 01:16
 Operator : MA/JU
 Sample : 04497-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBN2

Quant Time: Oct 04 04:09:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	4957	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	16379	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	10060	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.346	188	22938	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240	21586	0.400	ng/ul	0.00
23) Perylene-d12	23.997	264	22996	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	20544	3.300	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5316	0.201	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	16353	0.239	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.359	88	1294	0.196	ng/ul#	87
5) Naphthalene	10.812	128	3797	0.082	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
Data File : BN028026.D
Acq On : 04 Oct 2023 01:16
Operator : MA/JU
Sample : 04497-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBBN2

Quant Time: Oct 04 04:09:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration




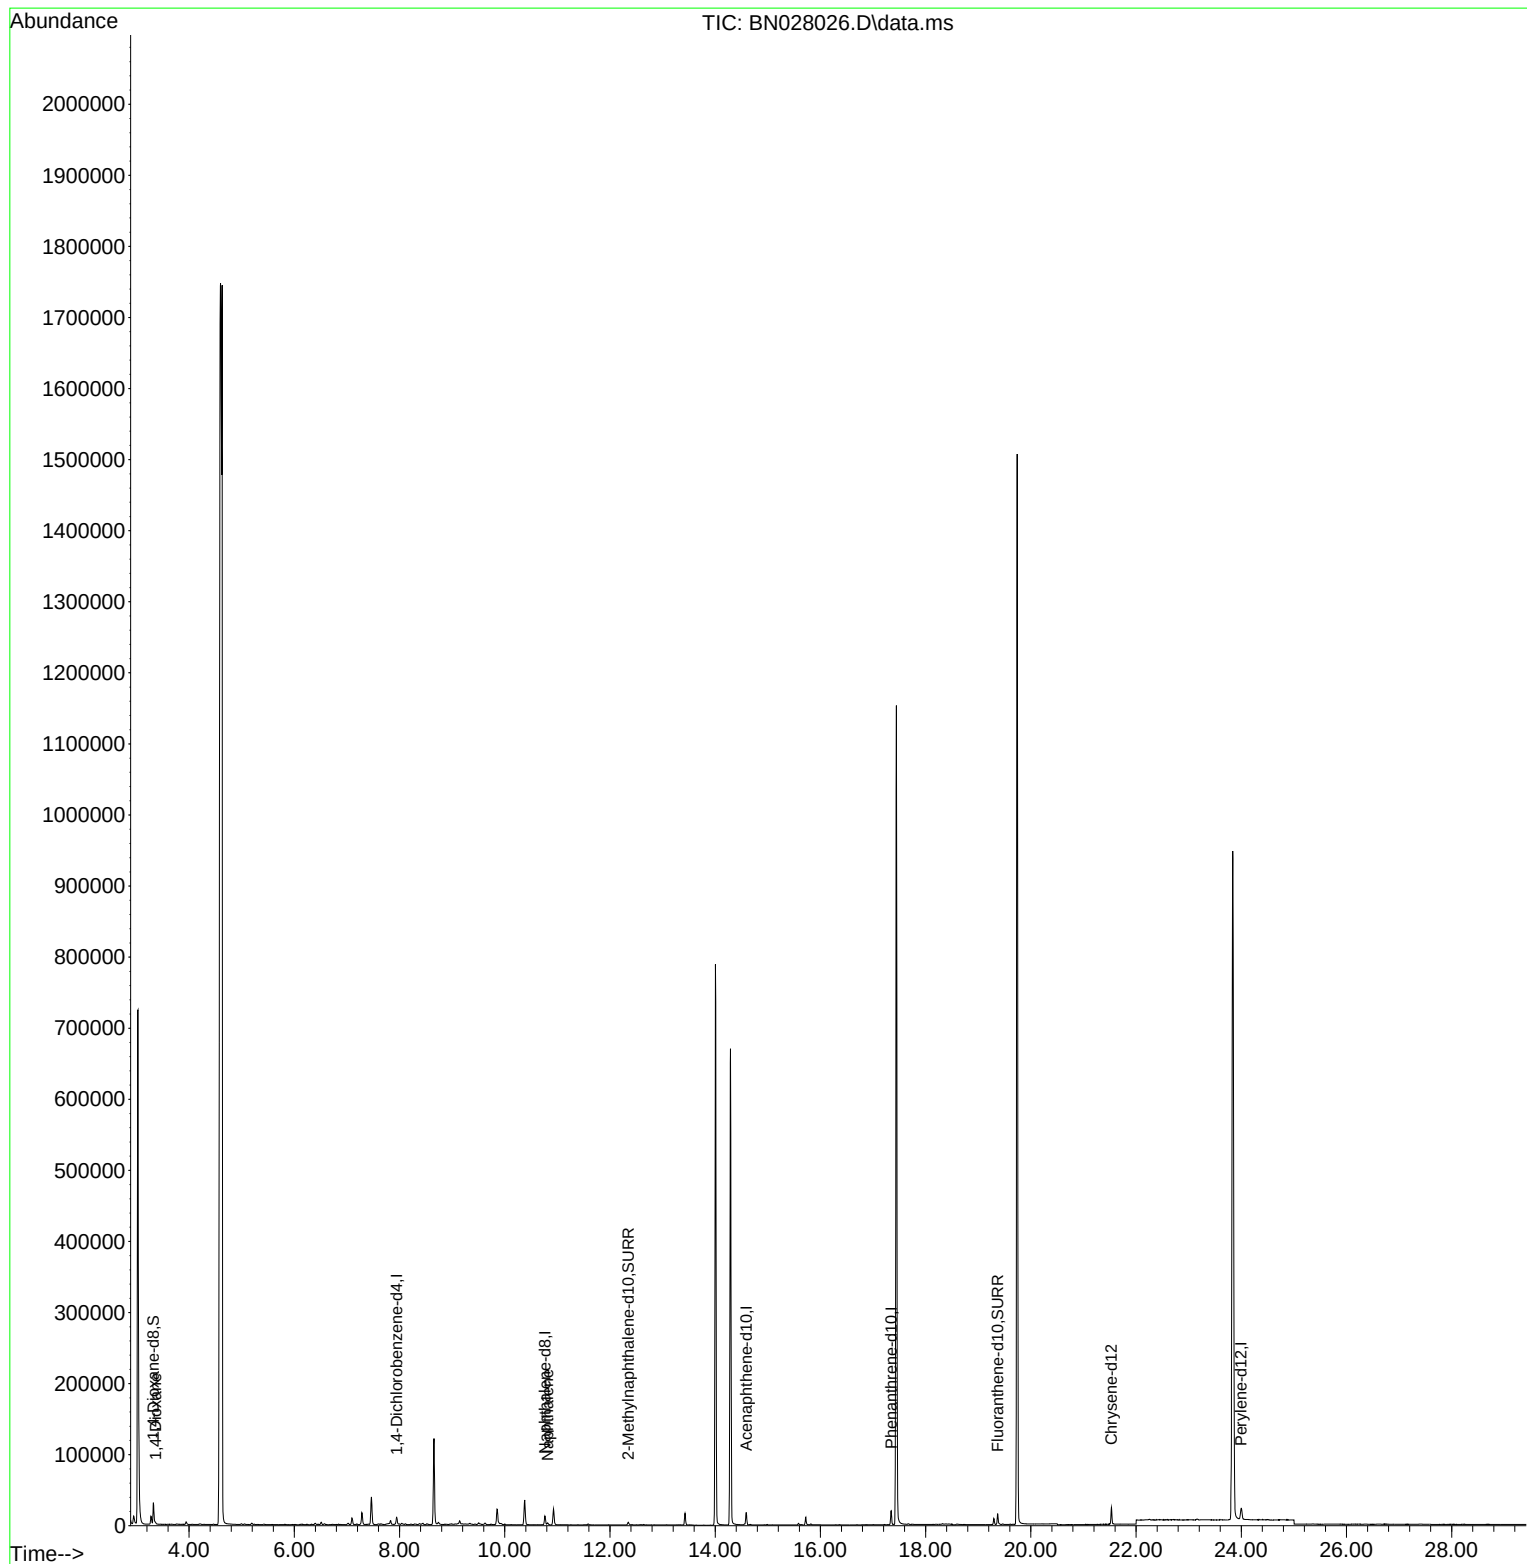


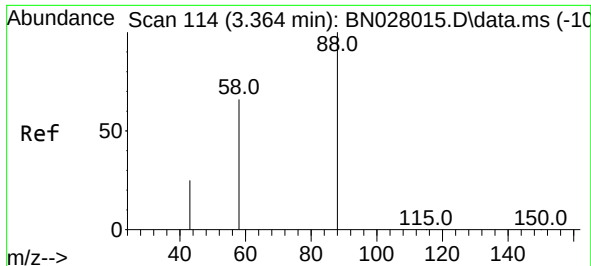

#2
1,4-Dioxane
Concen: 0.196 ng/ul
RT: 3.359 min Scan# 114
Delta R.T. -0.004 min
Lab File: BN028026.D
Acq: 04 Oct 2023 01:16

Instrument :
BNA_N
ClientSampleId :
BBBN2

Tgt Ion: 88 Resp: 1294
Ion Ratio Lower Upper
88 100
43 60.2 33.4 50.2#
58 56.8 45.7 68.5

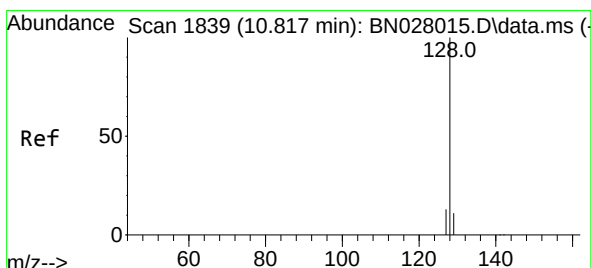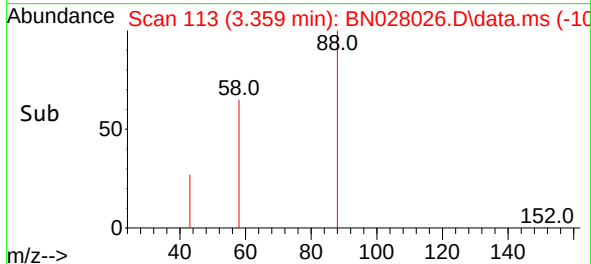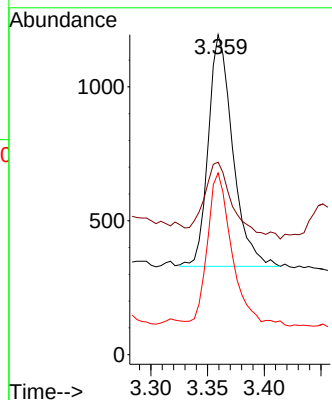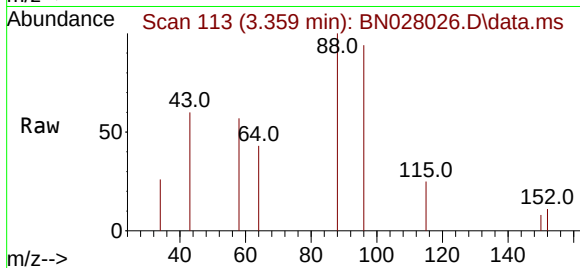

#5
Naphthalene
Concen: 0.082 ng/ul
RT: 10.812 min Scan# 1838
Delta R.T. -0.006 min
Lab File: BN028026.D
Acq: 04 Oct 2023 01:16

Tgt Ion: 128 Resp: 3797
Ion Ratio Lower Upper
128 100
129 15.3 9.4 14.0#
127 16.4 11.0 16.4#

