

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
 Data File : BN028027.D
 Acq On : 04 Oct 2023 01:53
 Operator : MA/JU
 Sample : 04497-04RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJR3RE

Quant Time: Oct 04 04:54:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	5597	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.768	136	19616	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.592	164	39811	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.350	188	24423	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.530	240	16233	0.400	ng/ul	# 0.00
23) Perylene-d12	24.000	264	15673	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	23550	3.350	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	15365	0.486	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	26218	0.509	ng/ul	0.00
Target Compounds						
						Qvalue
8) 1-Methylnaphthalene	12.627	142	6707	0.184	ng/ul#	26
12) Fluorene	15.642	166	7268	0.045	ng/ul#	66
20) Pyrene	19.771	202	3093	0.048	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100323\
Data File : BN028027.D
Acq On : 04 Oct 2023 01:53
Operator : MA/JU
Sample : 04497-04RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJR3RE

Quant Time: Oct 04 04:54:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration

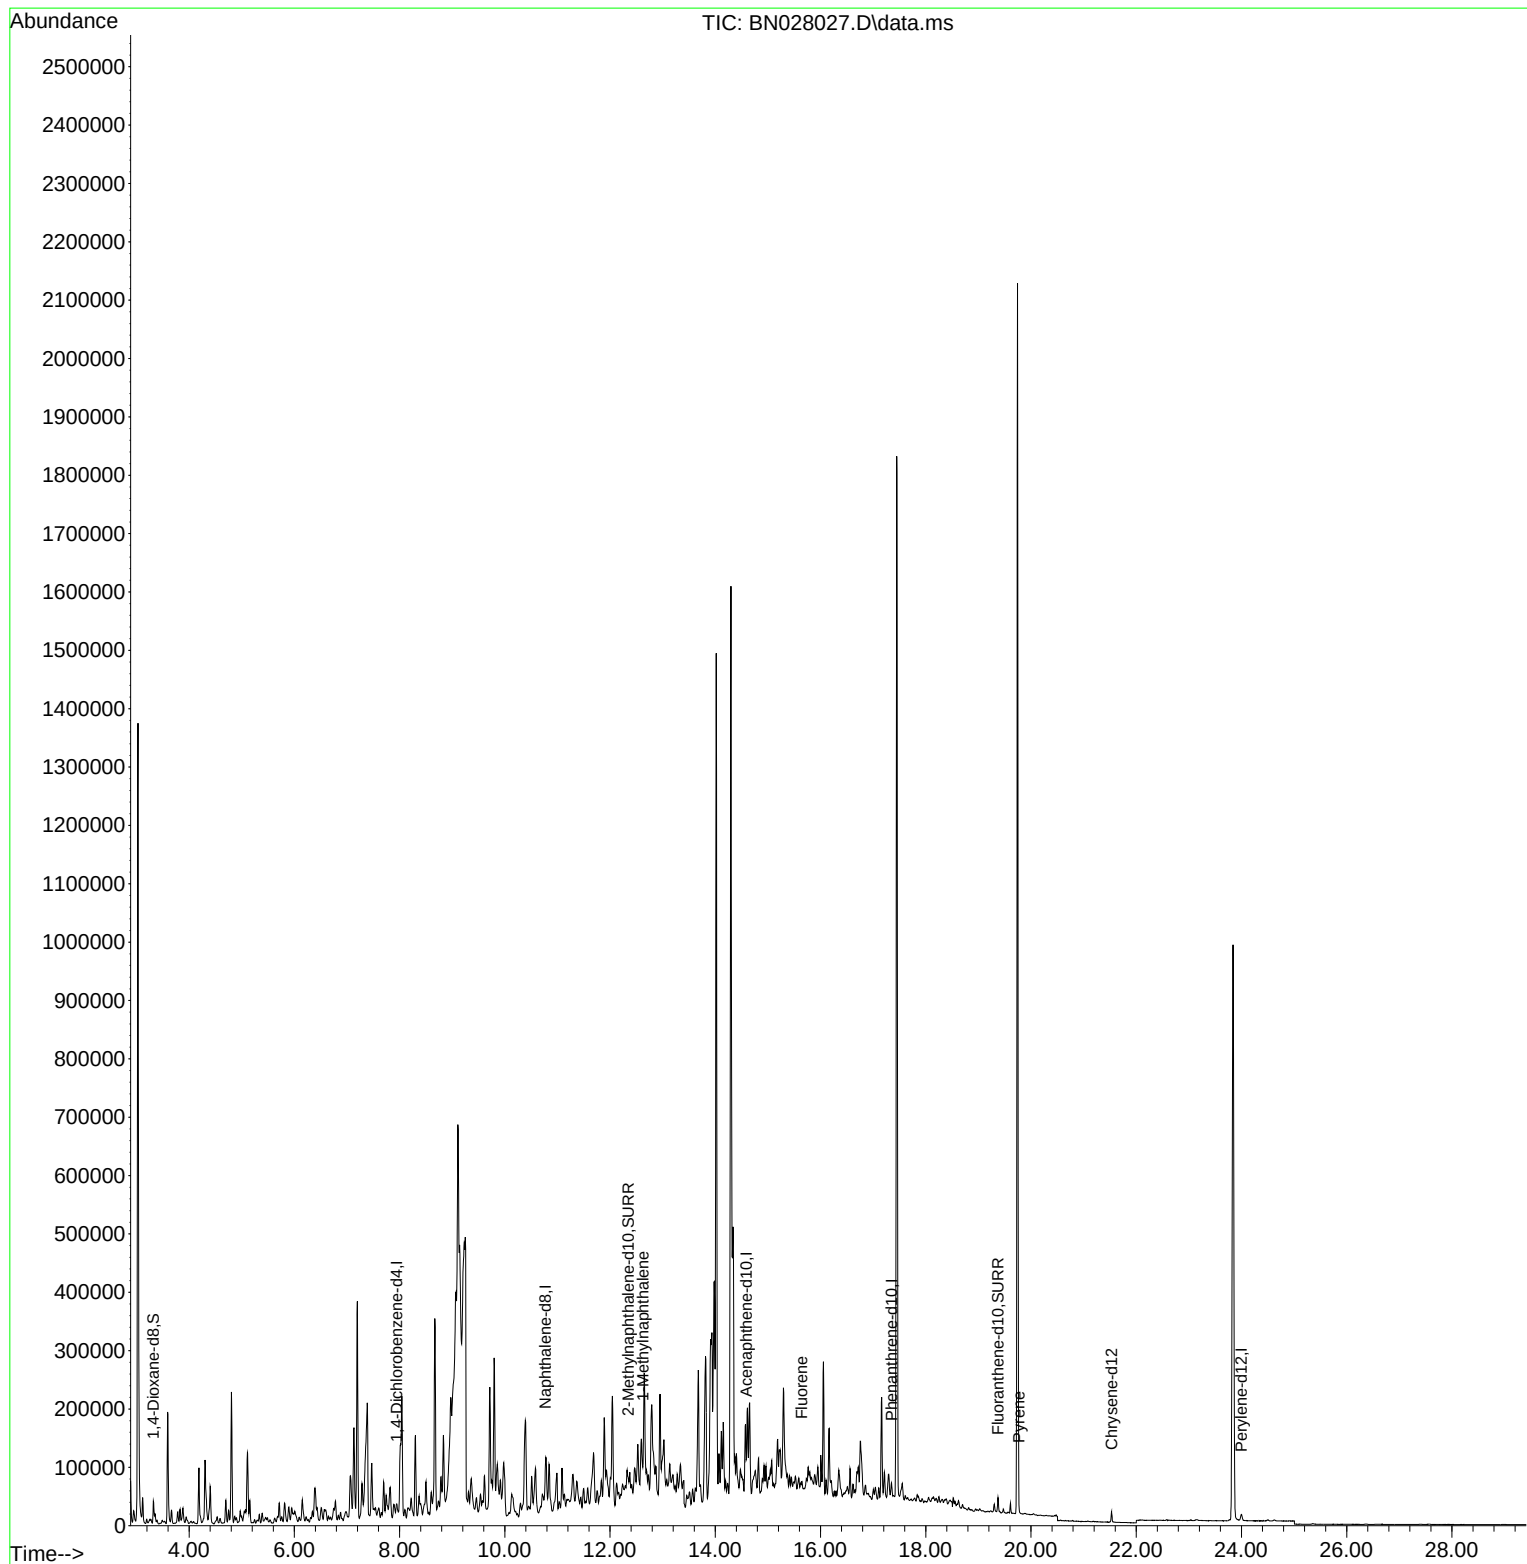

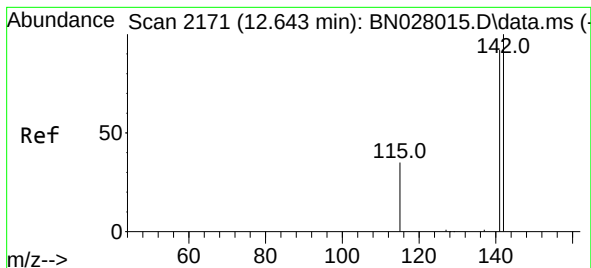

#8

1-Methylnaphthalene

Concen: 0.184 ng/ul

RT: 12.627 min Scan# 2168

Delta R.T. -0.017 min

Lab File: BN028027.D

Acq: 04 Oct 2023 01:53

Instrument :

BNA_N

ClientSampleId :





BBJR3RE

Tgt Ion:142 Resp: 6707

Ion Ratio Lower Upper

142 100

141 164.2 74.4 111.6#

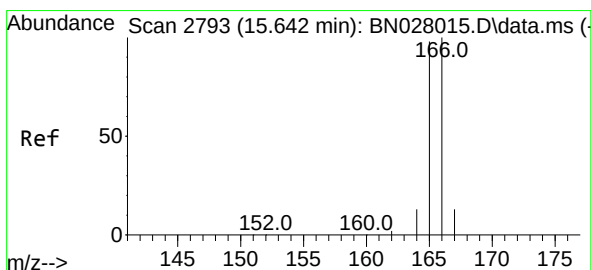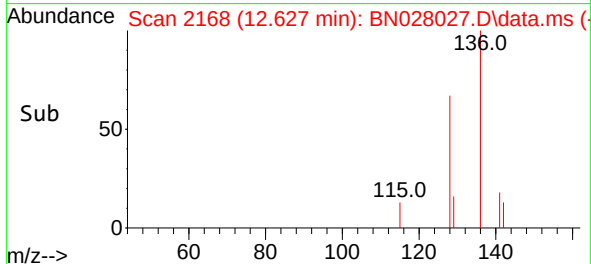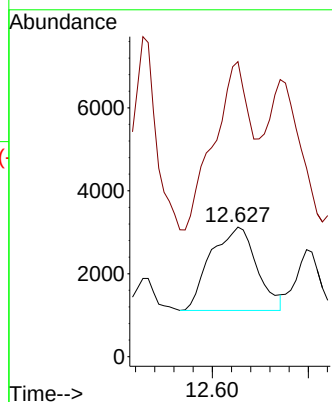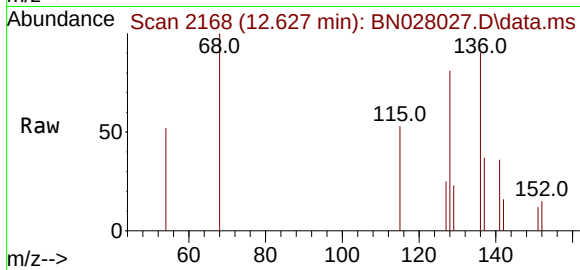

#12

Fluorene

Concen: 0.045 ng/ul

RT: 15.642 min Scan# 2793

Delta R.T. -0.000 min

Lab File: BN028027.D

Acq: 04 Oct 2023 01:53




Tgt Ion:166 Resp: 7268


Ion Ratio Lower Upper

166 100

165 120.7 78.5 117.7#

167 60.2 11.2 16.8#

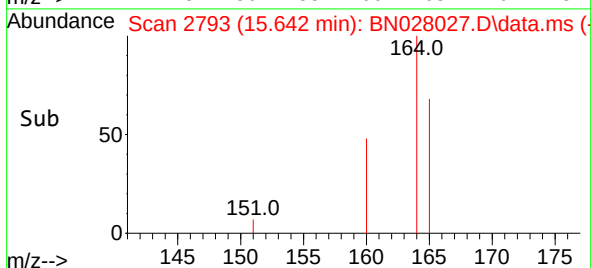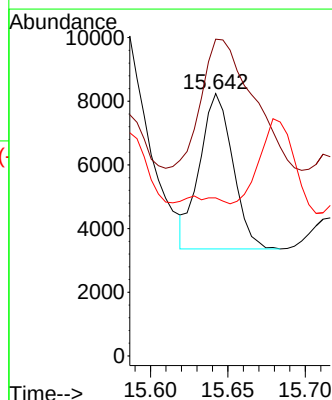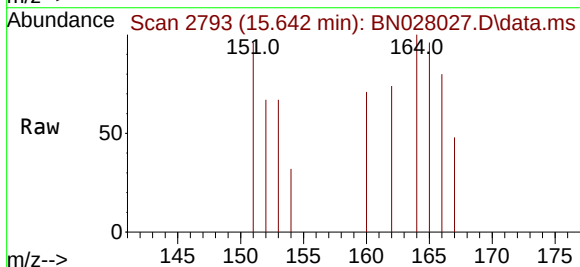

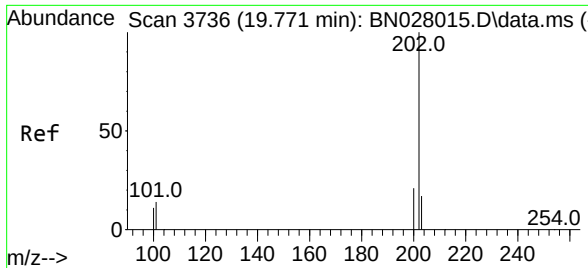

#20
 Pyrene
 Concen: 0.048 ng/ul
 RT: 19.771 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN028027.D
 Acq: 04 Oct 2023 01:53

Instrument :
 BNA_N
 ClientSampleId :
 BBJR3RE

Tgt Ion:	202	Resp:	3093
Ion Ratio	Lower	Upper	
202	100		
101	37.5	11.2	16.8#
100	25.8	9.1	13.7#

