
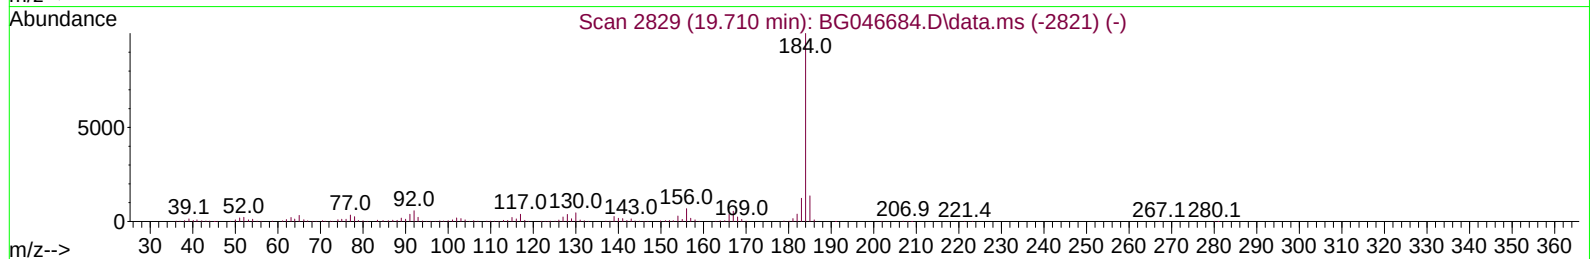
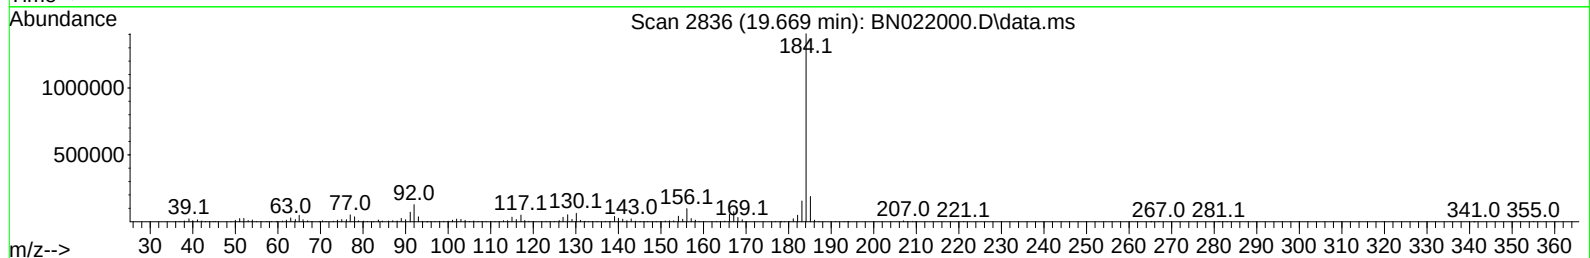


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100422\
Data File : BN022000.D
Acq On : 04 Oct 2022 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 23:59:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 23:59:26 2022
Response via : Initial Calibration

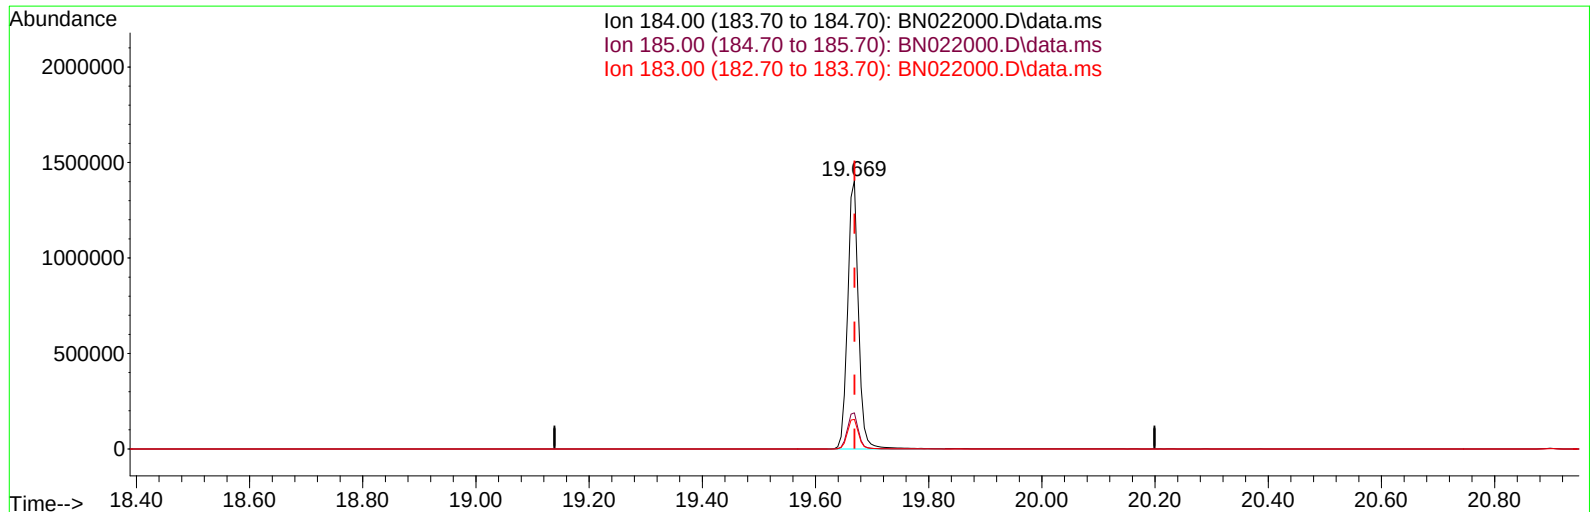

TIC: BN022000.D\data.ms

(77) Benzidine




19.669min (0.000) 0.00 ng

response 1859028

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.45
183.00	13.20	11.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100422\
Data File : BN022000.D
Acq On : 04 Oct 2022 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 23:55:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 01:32:21 2022
Response via : Initial Calibration

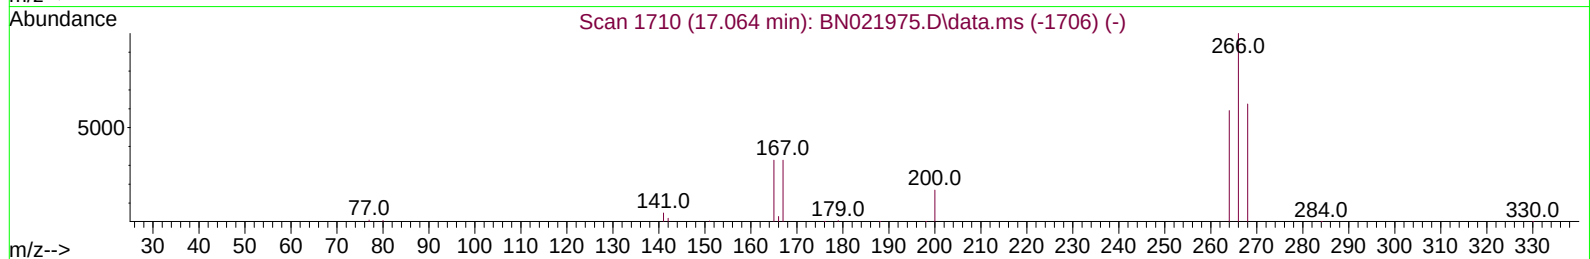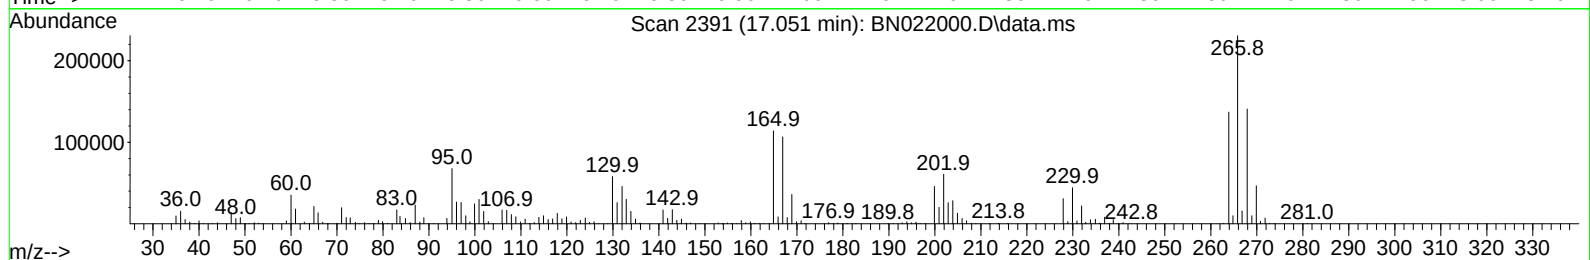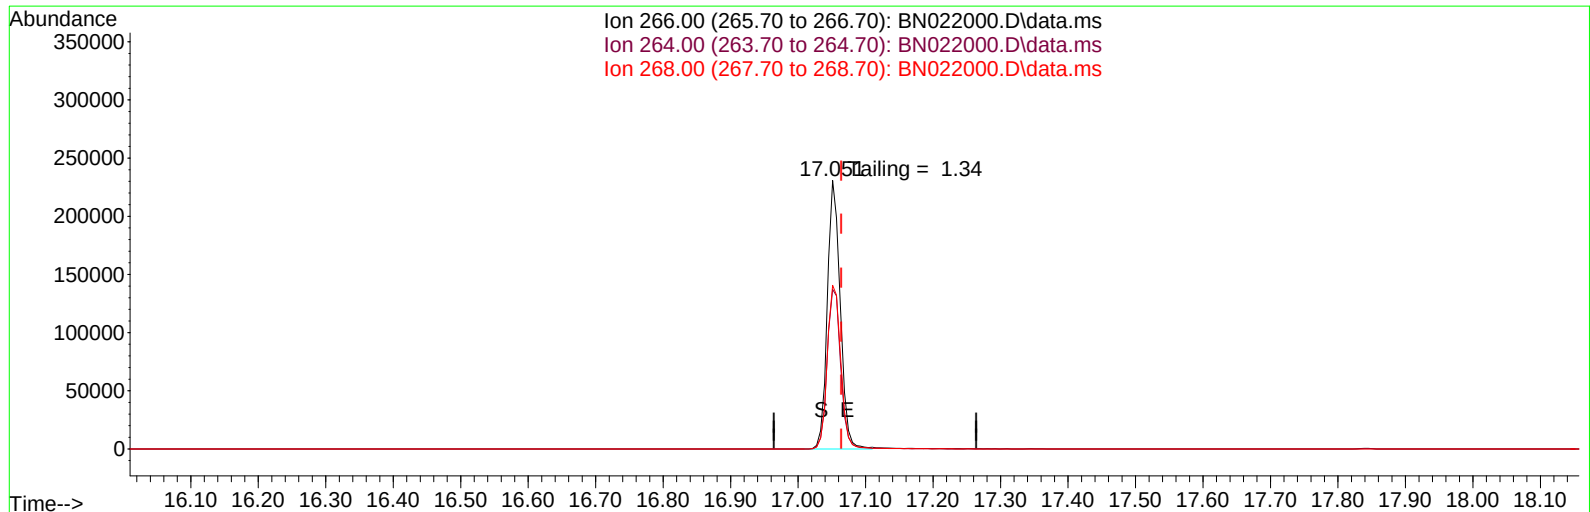

TIC: BN022000.D\data.ms

(24) Pentachlorophenol

17.051min (-0.013) 0.00 ng

response 309039

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.20	62.11
268.00	62.00	64.10
0.00	0.00	0.00