


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100422\
 Data File : BN022000.D
 Acq On : 04 Oct 2022 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 11 04:42:07 2022

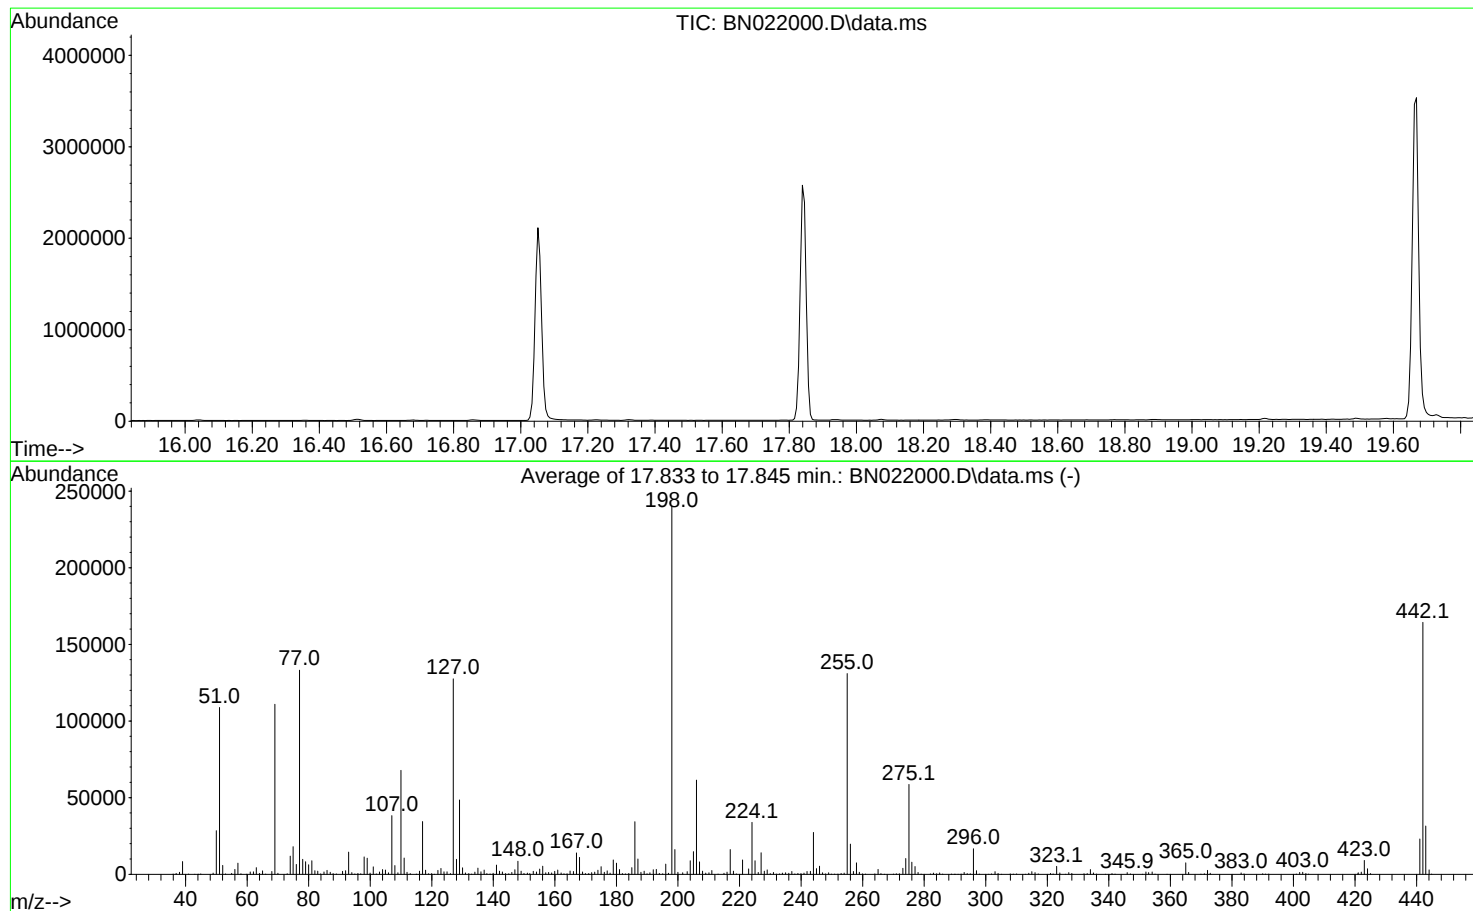

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	108797	PASS
68	69	0.00	2	1.7	1845	PASS
69	198	0.00	100	46.2	110880	PASS
70	69	0.00	2	0.6	667	PASS
127	198	10	80	53.1	127544	PASS
197	198	0.00	2	0.3	675	PASS
198	198	100	100	100.0	240000	PASS
199	198	5	9	6.7	16165	PASS
275	198	10	60	24.4	58619	PASS
365	198	1	100	3.1	7488	PASS
441	198	0.01	100	9.6	22995	PASS
442	442	50	100	100.0	164368	PASS
443	442	15	24	19.2	31493	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/4/2022	BNA_N	<u>BN022000.D</u>
Compound Name	Response	Retention Time
DDT	862429	20.898
DDD	7357	20.457
DDE	312	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7669	870098	0.88

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100422\
Data File : BN022000.D
Acq On : 04 Oct 2022 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 23:59:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 23:59:26 2022
Response via : Initial Calibration

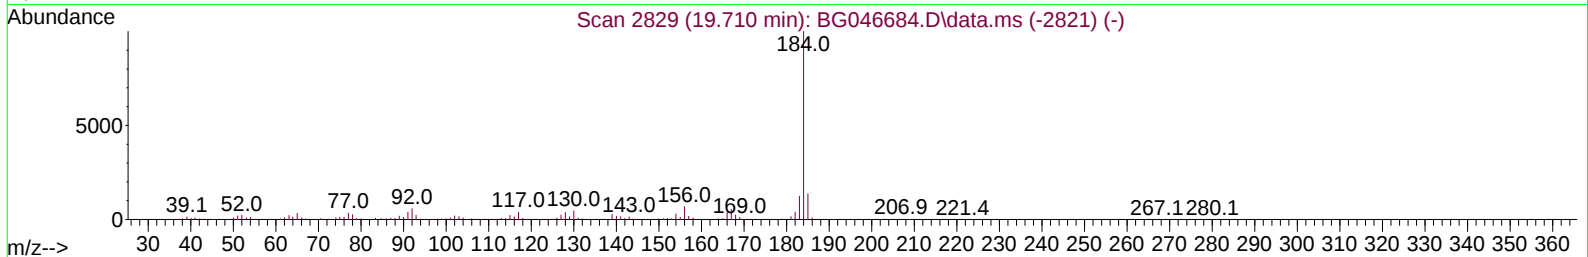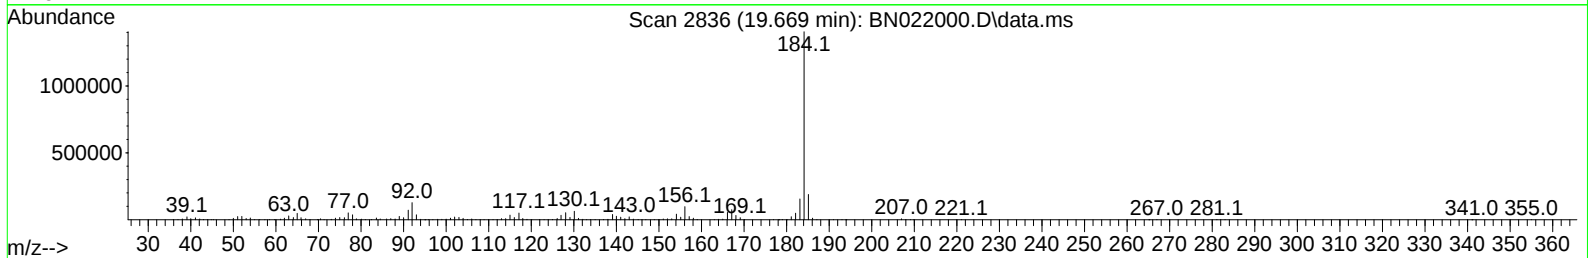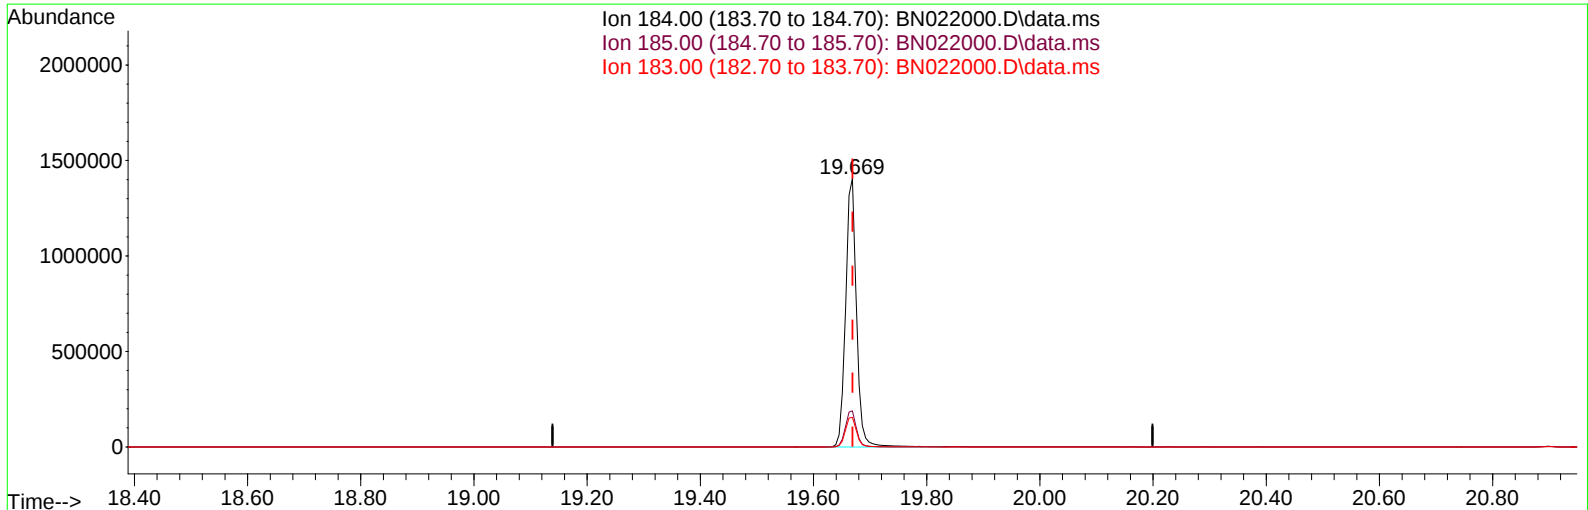

TIC: BN022000.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng




response 1859028

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.45
183.00	13.20	11.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100422\
Data File : BN022000.D
Acq On : 04 Oct 2022 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 04 23:55:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 01:32:21 2022
Response via : Initial Calibration

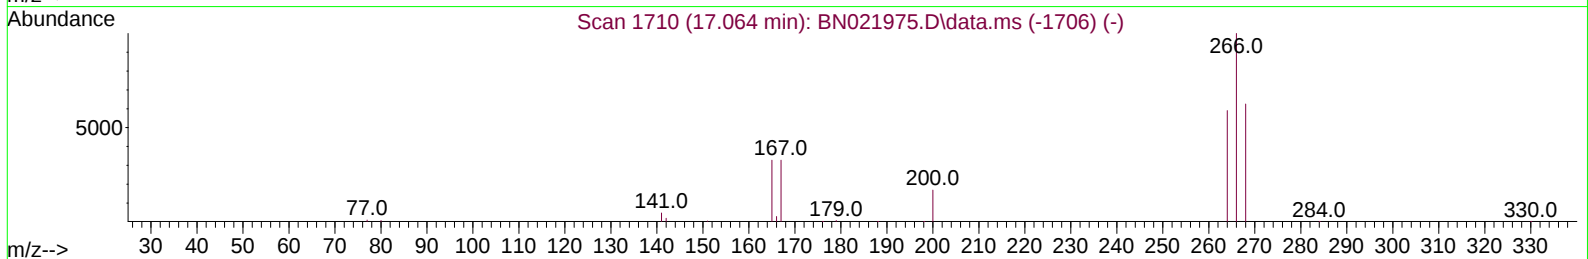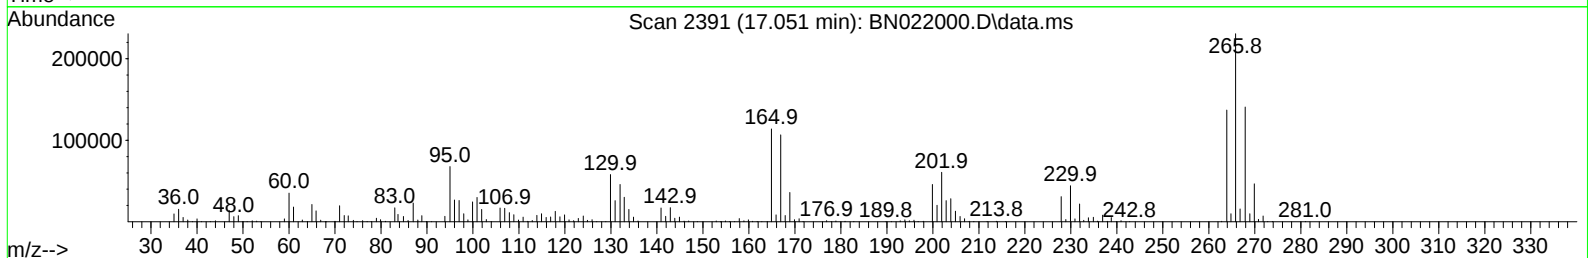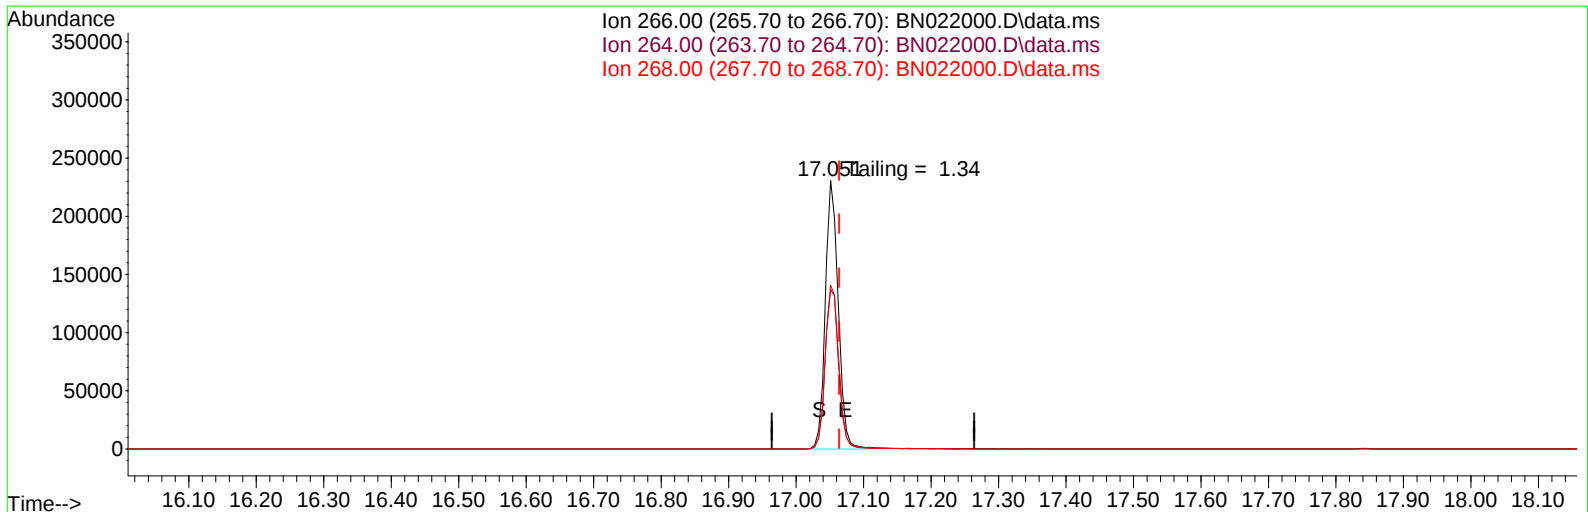

TIC: BN022000.D\data.ms

(24) Pentachlorophenol

17.051min (-0.013) 0.00 ng

response 309039

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.20	62.11
268.00	62.00	64.10
0.00	0.00	0.00