

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100423\
 Data File : BN028036.D
 Acq On : 04 Oct 2023 15:03
 Operator : MA/JU
 Sample : PB155913BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK913

Quant Time: Oct 05 02:05:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	4445	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	14817	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.587	164	9295	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.342	188	18770	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240	12134	0.400	ng/ul #	0.00
23) Perylene-d12	23.997	264	13183	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	42876	7.680	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	10050	0.421	ng/ul	-0.01
18) Fluoranthene-d10	19.371	212	18905	0.491	ng/ul	0.00
Target Compounds						
					Qvalue	
10) Acenaphthylene	14.314	152	1748	0.041	ng/ul#	67
20) Pyrene	19.738	202	2394	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.837	252	4542	0.109	ng/ul#	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100423\
Data File : BN028036.D
Acq On : 04 Oct 2023 15:03
Operator : MA/JU
Sample : PB155913BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK913

Quant Time: Oct 05 02:05:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration




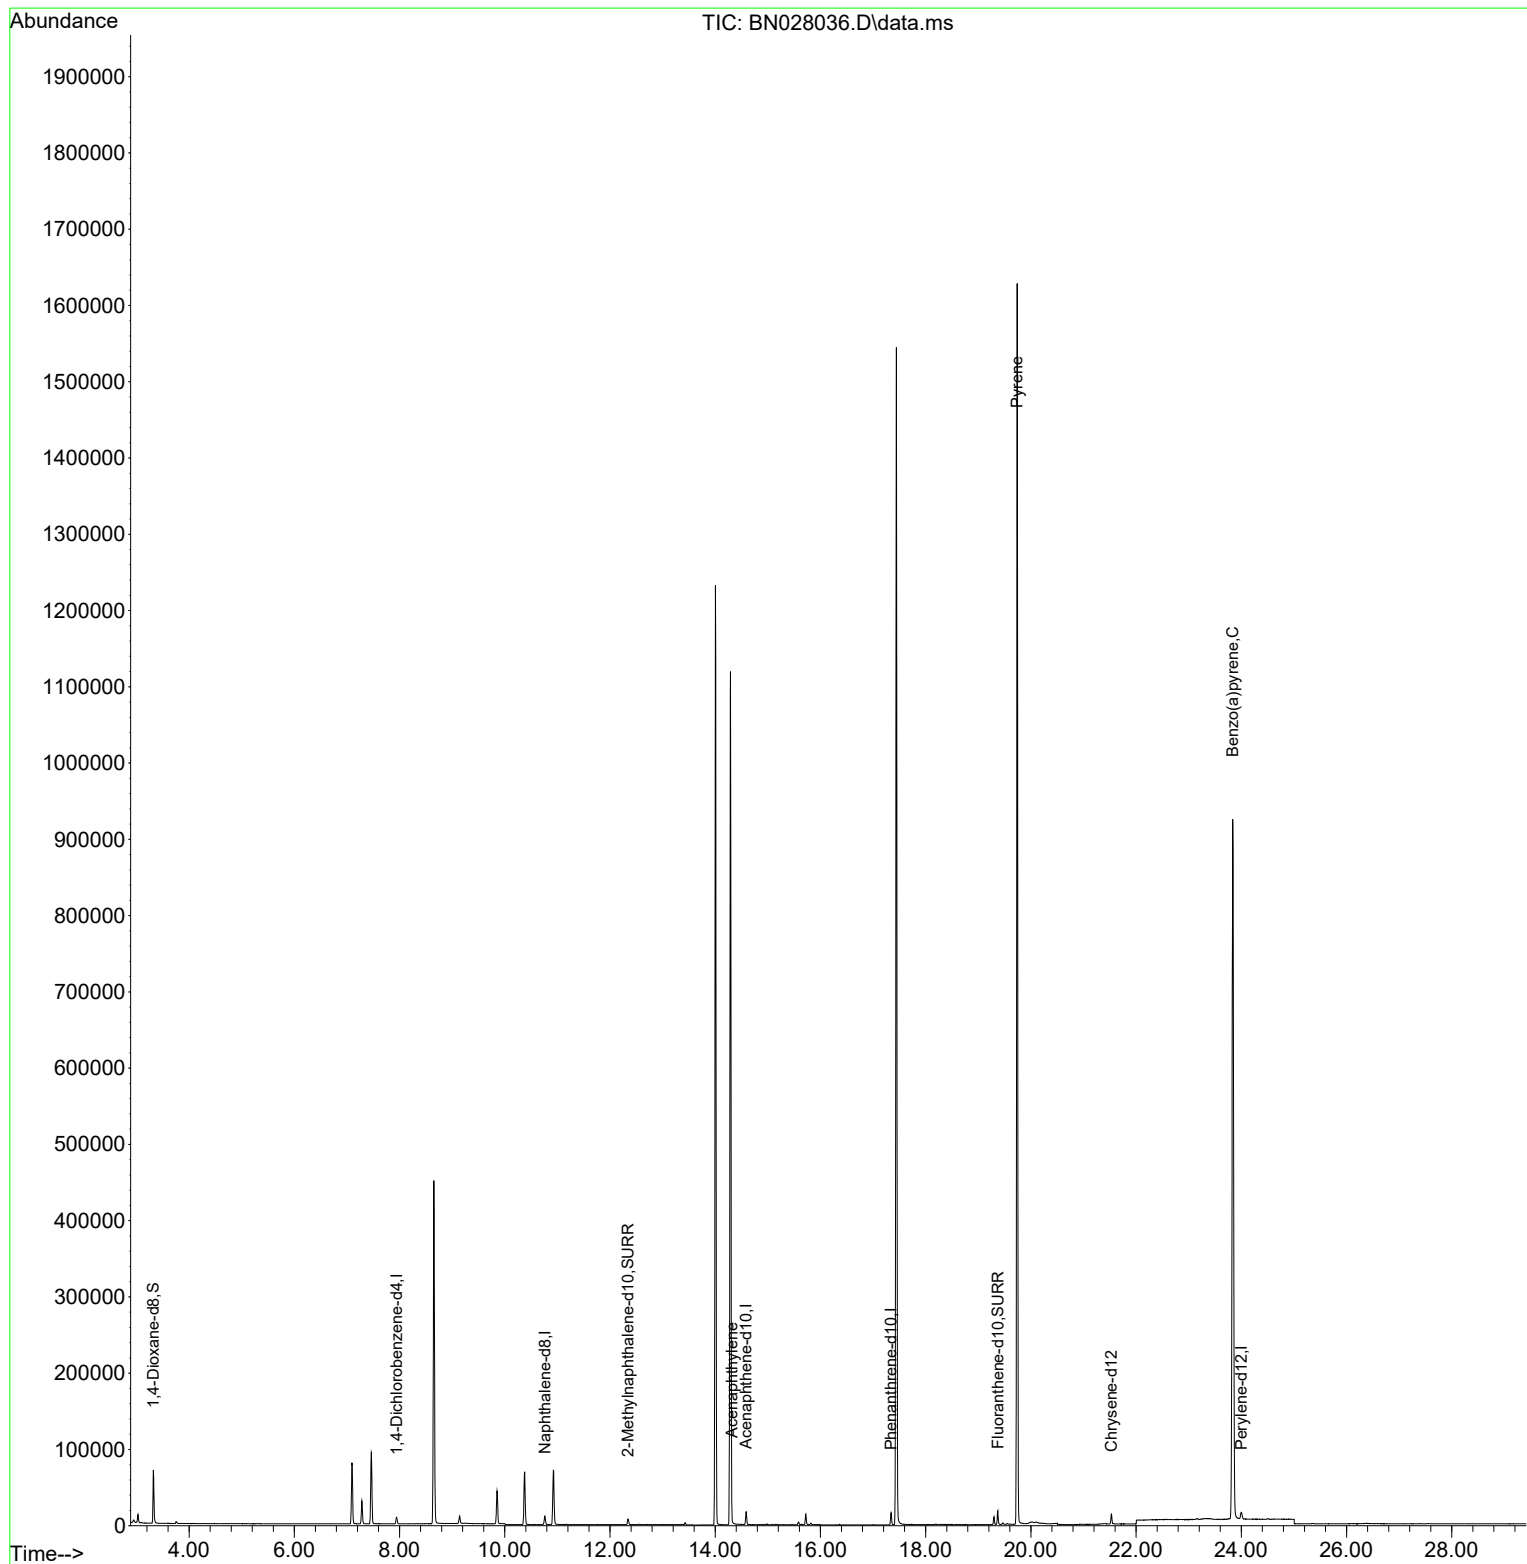


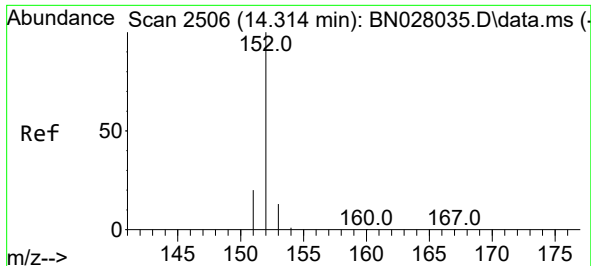

#10
Acenaphthylene
Concen: 0.041 ng/ul
RT: 14.314 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN028036.D
Acq: 04 Oct 2023 15:03




Instrument :
BNA_N
ClientSampleId :
SBLK913


Tgt Ion:152 Resp: 1748
Ion Ratio Lower Upper
152 100
151 31.6 16.4 24.6#
153 32.3 10.9 16.3#

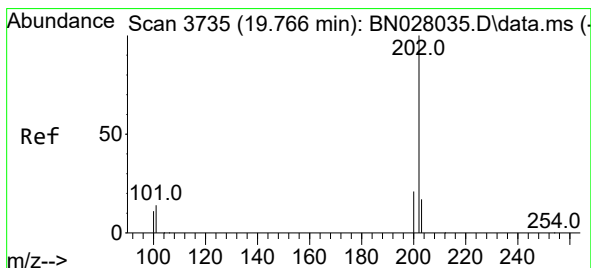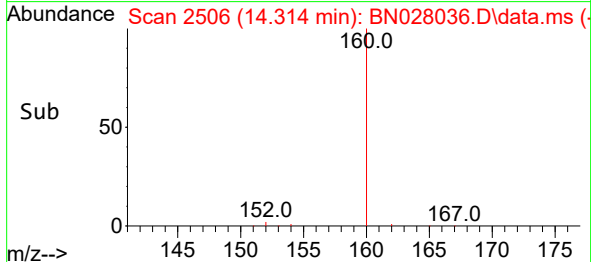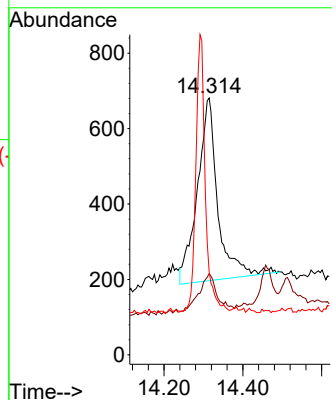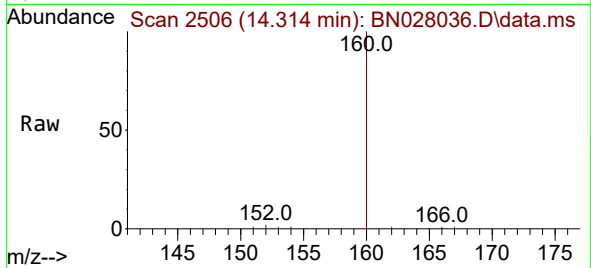

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.738 min Scan# 3729
Delta R.T. -0.032 min
Lab File: BN028036.D
Acq: 04 Oct 2023 15:03


Tgt Ion:202 Resp: 2394
Ion Ratio Lower Upper
202 100
101 152.6 11.2 16.8#
100 1034.2 9.1 13.7#

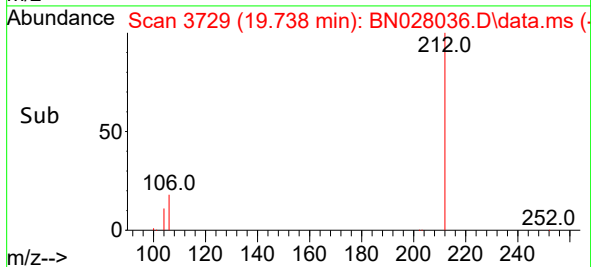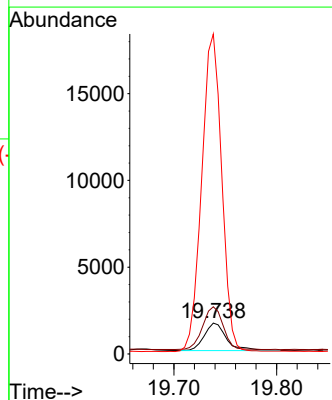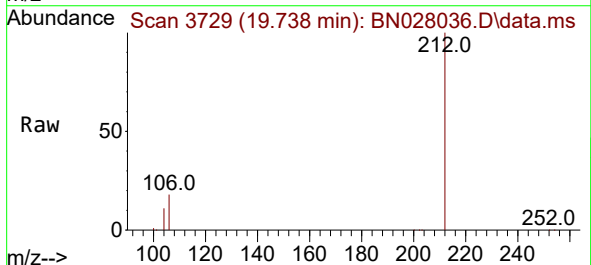

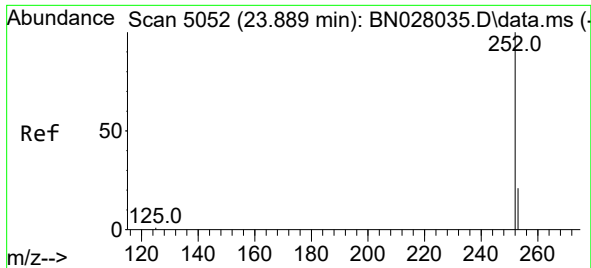

#26
 Benzo(a)pyrene
 Concen: 0.109 ng/ul
 RT: 23.837 min Scan# 50
 Delta R.T. -0.058 min
 Lab File: BN028036.D
 Acq: 04 Oct 2023 15:03

Instrument :
 BNA_N
 ClientSampleId :
 SBLK913

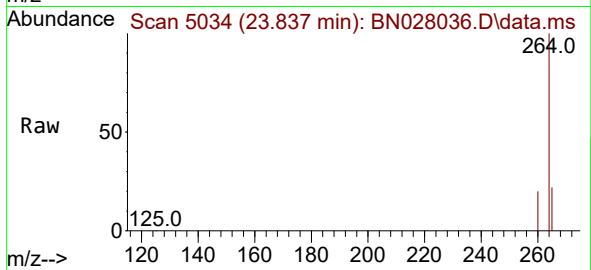

Tgt Ion:252 Resp: 4542
 Ion Ratio Lower Upper
 252 100
 253 66.9 23.4 35.2#
 125 69.6 15.3 22.9#

