

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100423\
 Data File : BN028042.D
 Acq On : 04 Oct 2023 19:25
 Operator : MA/JU
 Sample : 04588-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKH3


Quant Time: Oct 05 02:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	5047	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	16610	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.587	164	9996	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.342	188	20449	0.400	ng/ul	0.00
17) Chrysene-d12	21.527	240	13720	0.400	ng/ul	0.00
23) Perylene-d12	23.994	264	15267	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	24896	3.927	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	8818	0.329	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	18776	0.431	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.359	88	1217	0.181	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 05 02:05:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration

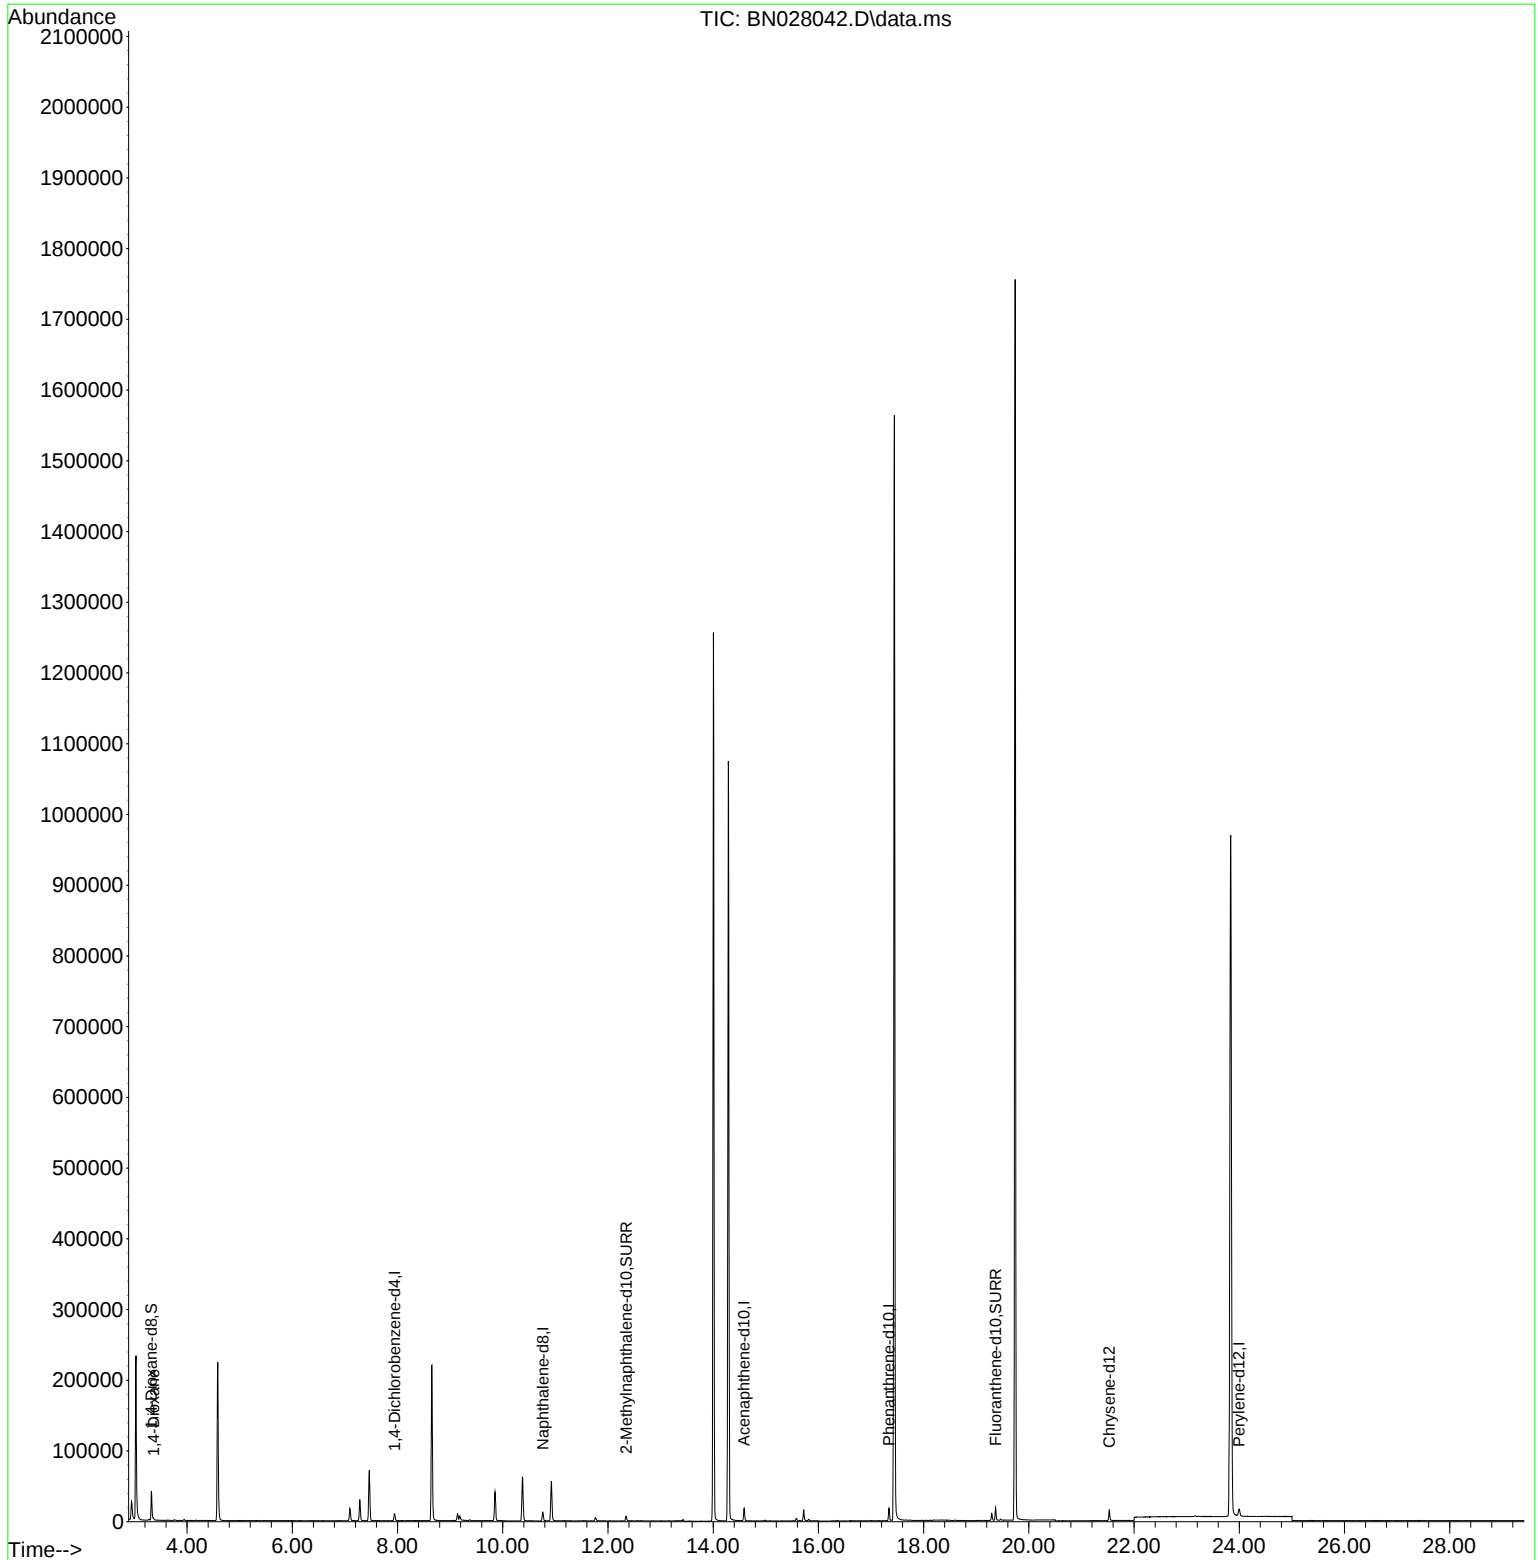

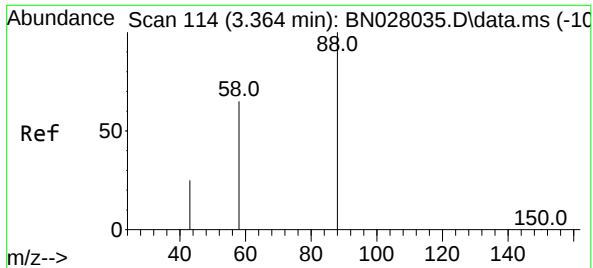

#2
1,4-Dioxane
Concen: 0.181 ng/ul
RT: 3.359 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN028042.D
Acq: 04 Oct 2023 19:25

Instrument :
BNA_N
ClientSampleId :
BBKH3

Tgt Ion:	88	Resp:	1217
Ion	Ratio	Lower	Upper
88	100		
43	77.4	33.4	50.2#
58	56.5	45.7	68.5

