

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034401.D
 Acq On : 04 Oct 2024 22:38
 Operator : RC/JU
 Sample : PB163807BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK807

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	15	19	27	rVB	61431	83516	2.71%	0.201%
2	3.387	81	85	108	rBV	651196	1013547	32.92%	2.434%
3	3.687	132	136	143	rVB	31204	45515	1.48%	0.109%
4	4.140	207	213	216	rBV5	7973	15850	0.51%	0.038%
5	6.063	537	540	542	rBV4	2425	3141	0.10%	0.008%
6	6.581	621	628	644	rBV	749920	1217320	39.53%	2.924%
7	6.734	648	654	666	rVB	637964	994250	32.29%	2.388%
8	6.922	679	686	698	rBV	825850	1312435	42.62%	3.152%
9	7.381	757	764	772	rBV	880036	1357767	44.09%	3.261%
10	8.093	878	885	905	rBV	917201	1511434	49.08%	3.630%
11	8.522	950	958	968	rBV	725740	1163578	37.79%	2.795%
12	8.640	976	978	983	rVB6	2423	3339	0.11%	0.008%
13	8.975	1029	1035	1042	rBV7	4097	6692	0.22%	0.016%
14	9.234	1072	1079	1092	rBV	597402	952488	30.93%	2.288%
15	9.769	1161	1170	1181	rBV	917437	1493806	48.51%	3.588%
16	10.134	1225	1232	1245	rBV	1128287	1833014	59.53%	4.403%
17	10.281	1250	1257	1279	rBV	823087	1509641	49.03%	3.626%
18	11.740	1499	1505	1514	rBV2	11275	27082	0.88%	0.065%
19	13.457	1791	1797	1806	rBV	1382387	1952068	63.39%	4.689%
20	13.716	1835	1841	1855	rBV	1662404	2532234	82.23%	6.082%
21	13.892	1866	1871	1873	rBV2	8101	10459	0.34%	0.025%
22	14.034	1888	1895	1903	rBV	1550076	2270293	73.73%	5.453%
23	14.098	1905	1906	1911	rVB5	3424	4751	0.15%	0.011%
24	14.263	1928	1934	1956	rBV	347182	677229	21.99%	1.627%
25	15.034	2059	2065	2082	rBV	1978785	2990718	97.12%	7.183%
26	15.169	2082	2088	2101	rVV	424781	610236	19.82%	1.466%
27	15.275	2103	2106	2112	rVB3	10926	19555	0.64%	0.047%
28	15.833	2197	2201	2203	rBV5	3481	3990	0.13%	0.010%
29	16.163	2252	2257	2263	rBV4	3968	8097	0.26%	0.019%
30	16.469	2306	2309	2314	rBV6	3185	3385	0.11%	0.008%
31	16.580	2323	2328	2332	rBV6	4086	7053	0.23%	0.017%
32	16.704	2346	2349	2357	rVB6	3941	8518	0.28%	0.020%
33	16.792	2357	2364	2374	rBV	1648933	2312579	75.10%	5.554%
34	16.886	2374	2380	2399	rVV2	2008298	2894622	94.00%	6.952%
35	17.263	2440	2444	2445	rBV3	3601	4346	0.14%	0.010%
36	17.398	2464	2467	2472	rVB5	2738	4606	0.15%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034401.D
Acq On : 04 Oct 2024 22:38
Operator : RC/JU
Sample : PB163807BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK807

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	17.739	2517	2525	2533	rBV7	15028	46407	1.51%	0.111%
38	18.239	2607	2610	2615	rBV7	3482	4323	0.14%	0.010%
39	18.463	2646	2648	2650	rBV3	3313	3151	0.10%	0.008%
40	18.757	2694	2698	2705	rBV4	24097	36368	1.18%	0.087%
41	18.833	2708	2711	2716	rVB	24193	30068	0.98%	0.072%
42	18.880	2716	2719	2721	rBV4	3638	3821	0.12%	0.009%
43	19.198	2767	2773	2788	rBV	2225359	3034494	98.55%	7.288%
44	21.021	3078	3083	3093	rBV	1444253	2058955	66.86%	4.945%
45	23.539	3504	3511	3531	rVB	1425103	3079272	100.00%	7.396%
46	23.727	3535	3543	3560	rVB	1041542	2478829	80.50%	5.954%


Sum of corrected areas: 41634842

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034401.D
Acq On : 04 Oct 2024 22:38
Operator : RC/JU
Sample : PB163807BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK807

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

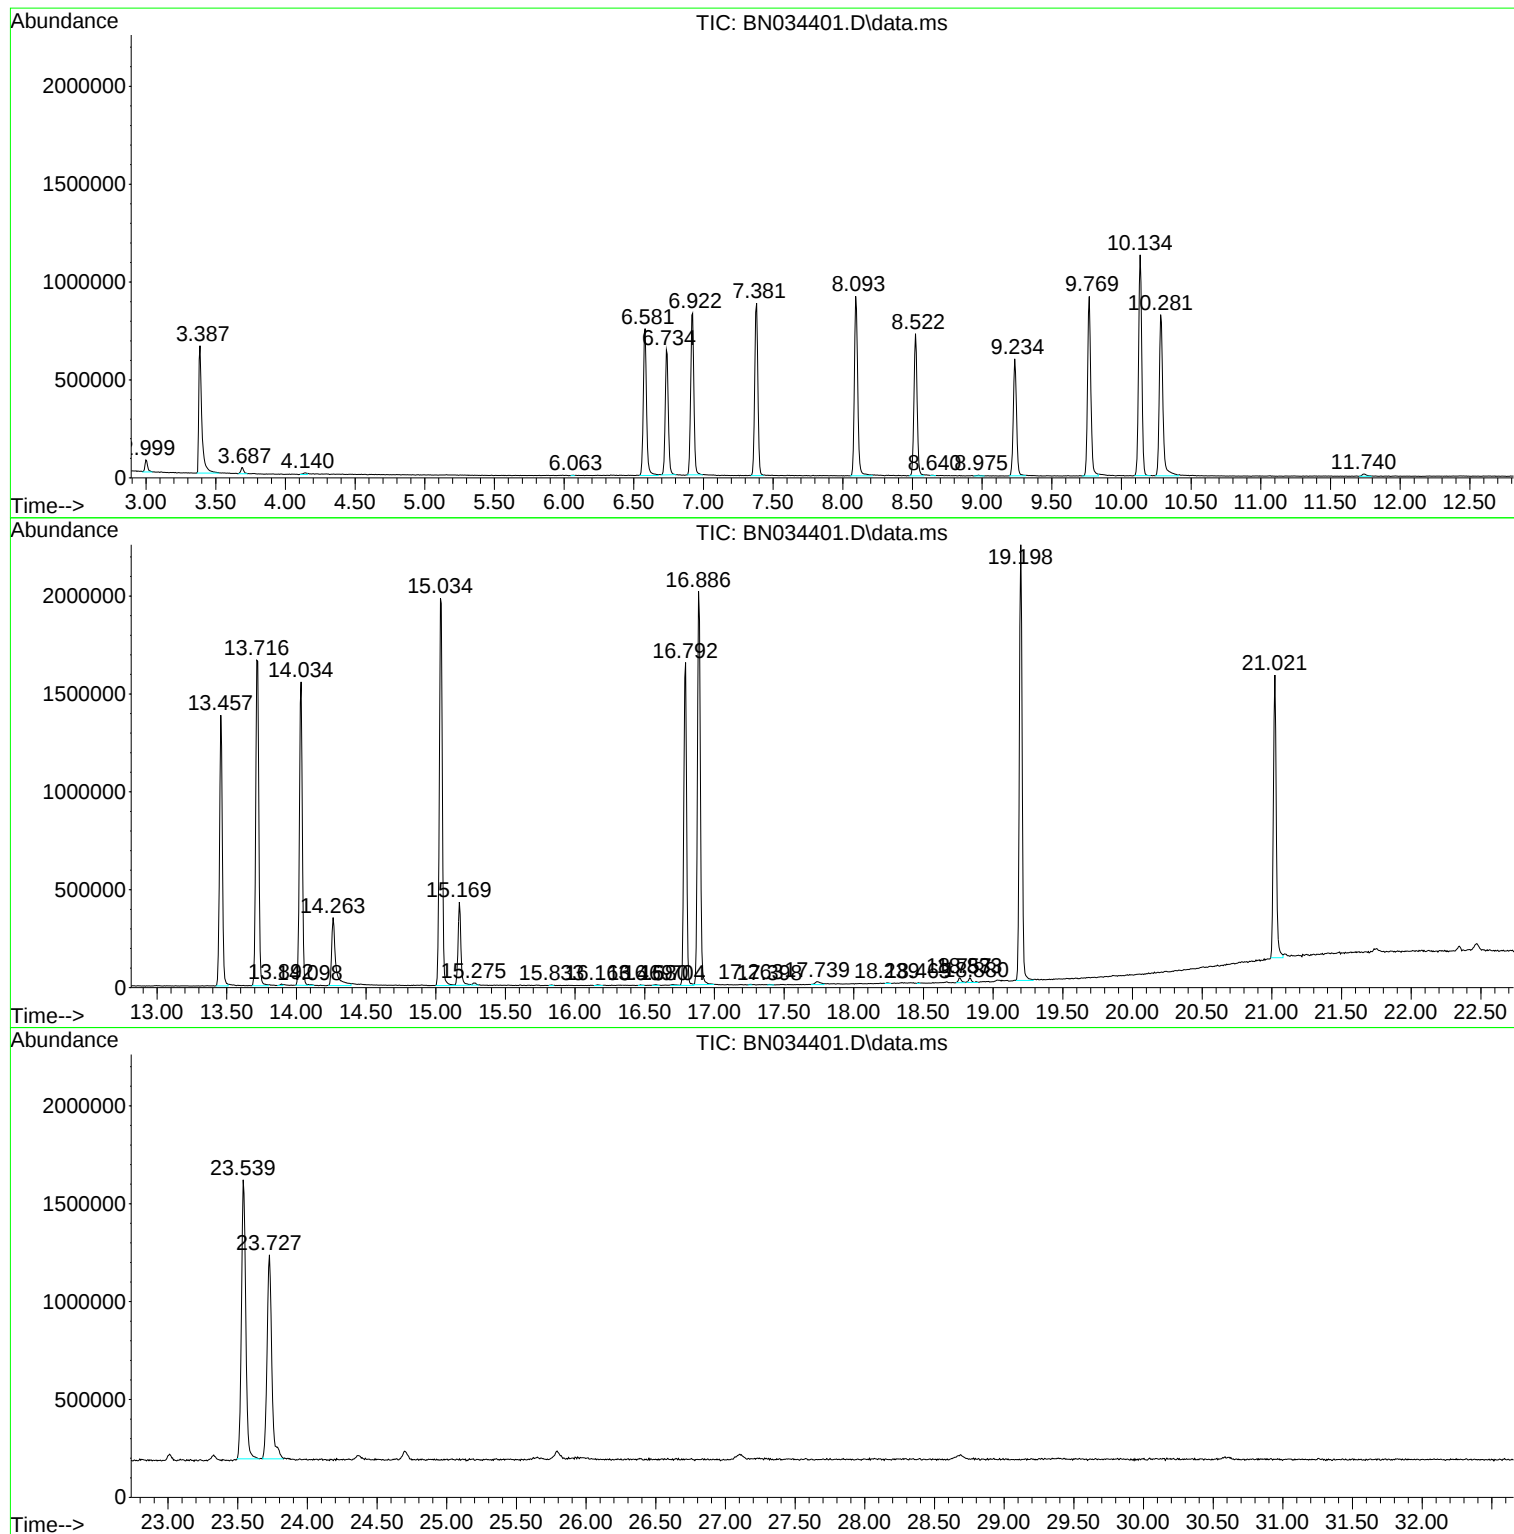

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034401.D
Acq On : 04 Oct 2024 22:38
Operator : RC/JU
Sample : PB163807BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK807

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034401.D
Acq On : 04 Oct 2024 22:38
Operator : RC/JU
Sample : PB163807BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK807

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------