

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034402.D
 Acq On : 04 Oct 2024 23:17
 Operator : RC/JU
 Sample : PB163787BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK787

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	16	20	29	rVB	51632	72821	1.84%	0.176%
2	3.387	81	85	106	rBV	580575	903118	22.87%	2.177%
3	3.693	132	137	142	rBV	27677	39232	0.99%	0.095%
4	4.140	209	213	220	rVB	7302	14128	0.36%	0.034%
5	6.581	620	628	641	rBV	655304	1056896	26.76%	2.547%
6	6.734	648	654	667	rVB	568119	875565	22.17%	2.110%
7	6.922	678	686	699	rBV	741207	1164476	29.49%	2.807%
8	7.040	705	706	714	rVB6	3218	4208	0.11%	0.010%
9	7.381	757	764	777	rBV	770711	1235865	31.30%	2.979%
10	8.093	878	885	906	rBV	795193	1319175	33.41%	3.180%
11	8.522	951	958	968	rBV	620055	999851	25.32%	2.410%
12	8.975	1030	1035	1038	rVB6	3161	4734	0.12%	0.011%
13	9.234	1071	1079	1089	rBV	496048	815243	20.64%	1.965%
14	9.769	1163	1170	1184	rBV	774976	1295840	32.81%	3.123%
15	9.863	1184	1186	1190	rVB5	3834	5051	0.13%	0.012%
16	10.134	1225	1232	1243	rVB	1039400	1643745	41.62%	3.962%
17	10.281	1251	1257	1276	rBV	688756	1284446	32.53%	3.096%
18	11.381	1440	1444	1450	rVB7	2760	5948	0.15%	0.014%
19	11.740	1501	1505	1514	rVB3	9796	20488	0.52%	0.049%
20	13.457	1791	1797	1815	rBV	1249753	1780123	45.08%	4.291%
21	13.716	1835	1841	1861	rBV	1423439	2180975	55.23%	5.257%
22	13.893	1867	1871	1881	rBV7	6345	14580	0.37%	0.035%
23	14.034	1888	1895	1903	rBV	1414639	2030304	51.41%	4.894%
24	14.263	1928	1934	1953	rBV	380006	720495	18.25%	1.737%
25	15.040	2059	2066	2082	rBV	1794463	2688364	68.08%	6.480%
26	15.169	2082	2088	2100	rVV	494476	705394	17.86%	1.700%
27	15.281	2103	2107	2113	rVB4	11169	20912	0.53%	0.050%
28	16.575	2322	2327	2330	rBV3	4866	7834	0.20%	0.019%
29	16.704	2345	2349	2356	rBV6	4117	8841	0.22%	0.021%
30	16.792	2357	2364	2374	rVV	1621194	2316761	58.67%	5.584%
31	16.887	2374	2380	2398	rVB	2018743	2847100	72.10%	6.862%
32	17.751	2517	2527	2535	rBV	12850	44289	1.12%	0.107%
33	18.763	2694	2699	2704	rBV2	26399	37848	0.96%	0.091%
34	18.833	2707	2711	2715	rVV	21984	31567	0.80%	0.076%
35	19.028	2741	2744	2749	rBV6	8483	15309	0.39%	0.037%
36	19.198	2767	2773	2787	rBV	2581223	3429913	86.86%	8.267%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034402.D
Acq On : 04 Oct 2024 23:17
Operator : RC/JU
Sample : PB163787BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK787

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	21.022	3078	3083	3093	rBV2	1890721	2653667	67.20%	6.396%
38	23.545	3504	3512	3528	rVB	1823745	3948984	100.00%	9.518%
39	23.727	3535	3543	3561	rVB	1319845	3244850	82.17%	7.821%


Sum of corrected areas: 41488940

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034402.D
Acq On : 04 Oct 2024 23:17
Operator : RC/JU
Sample : PB163787BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

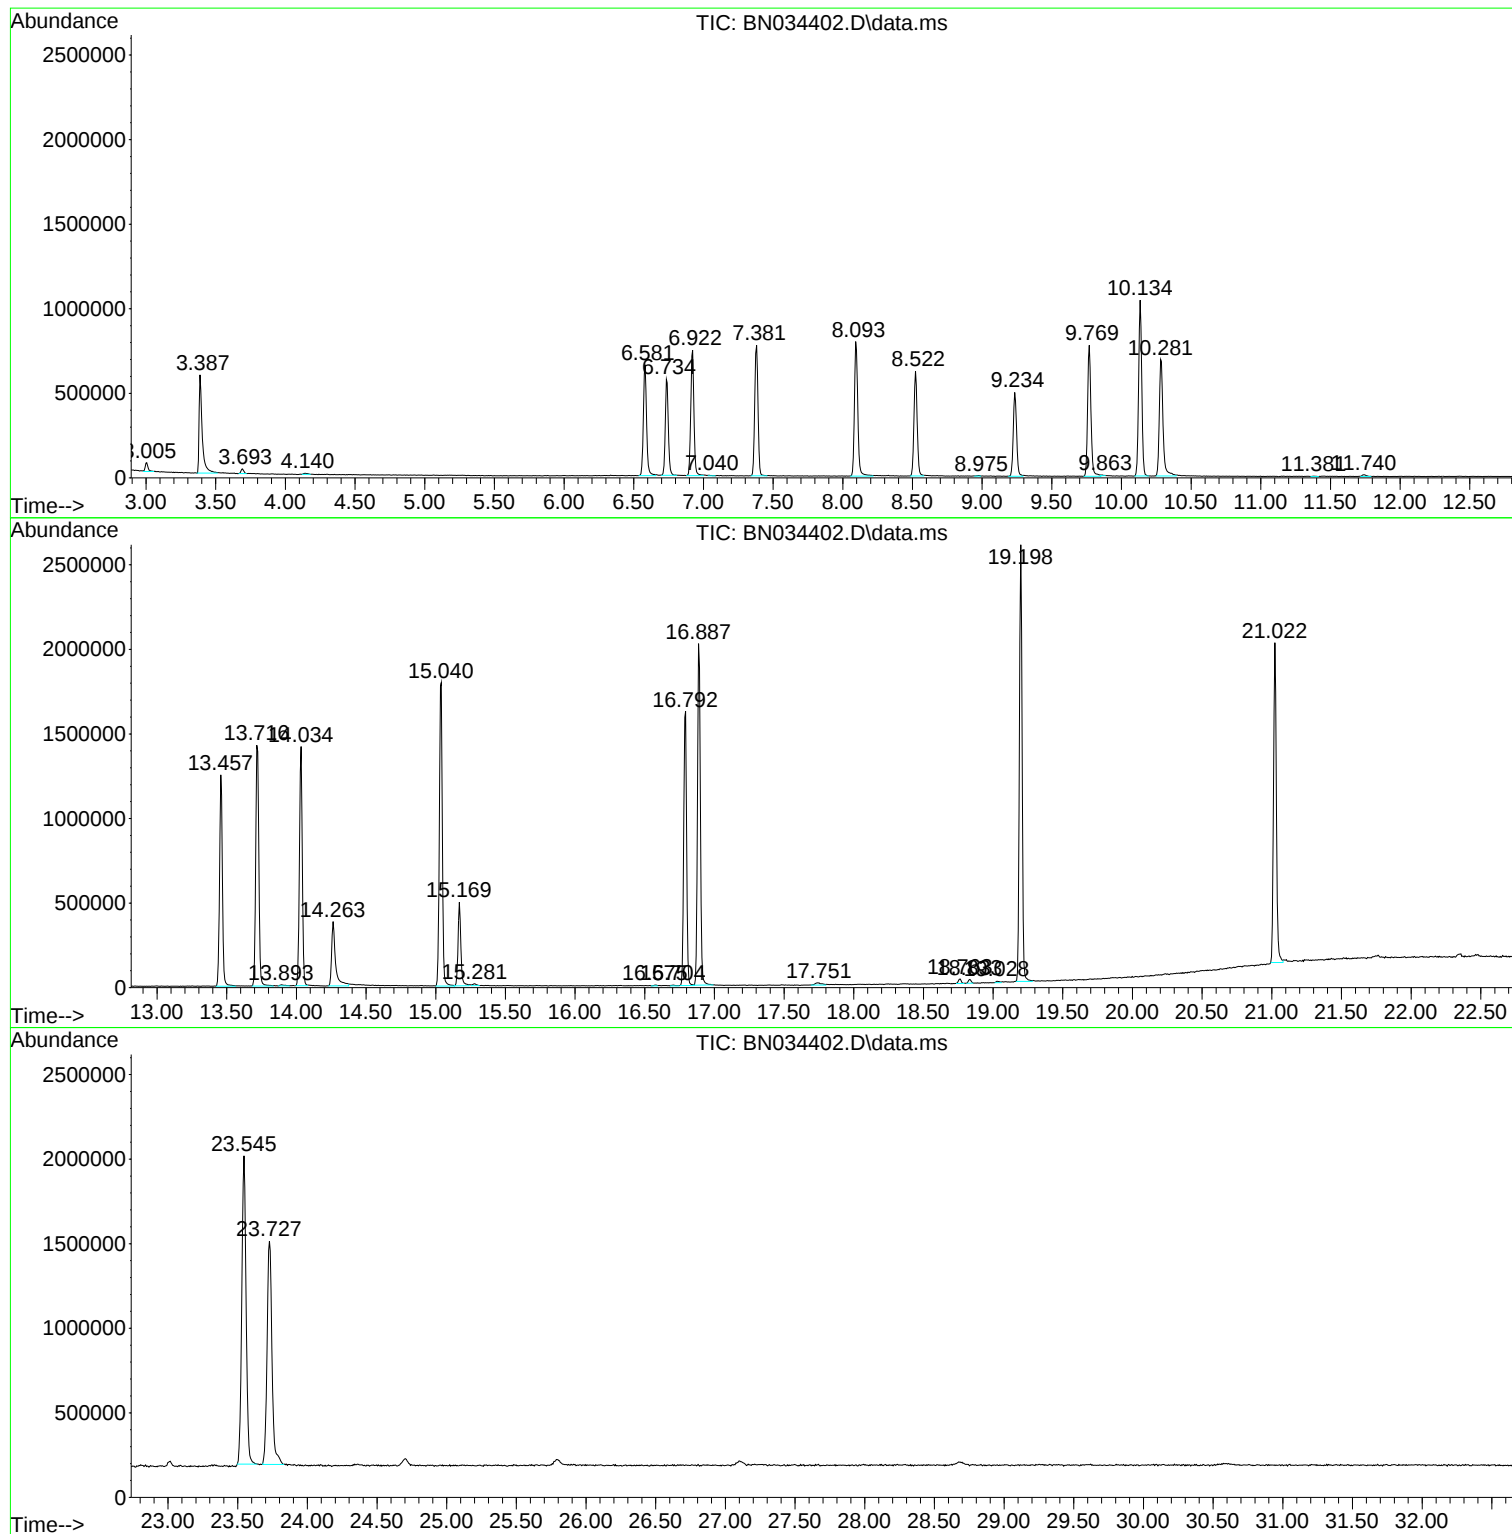

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034402.D
Acq On : 04 Oct 2024 23:17
Operator : RC/JU
Sample : PB163787BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034402.D
Acq On : 04 Oct 2024 23:17
Operator : RC/JU
Sample : PB163787BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK787

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------