

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034415.D
 Acq On : 05 Oct 2024 08:27
 Operator : RC/JU
 Sample : PB163786BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	16	19	27	rVB	64177	87049	2.08%	0.183%
2	3.387	81	85	108	rBV	698997	1115380	26.62%	2.339%
3	3.693	132	137	142	rVB	39332	57773	1.38%	0.121%
4	4.140	209	213	216	rBV3	6451	10948	0.26%	0.023%
5	6.581	621	628	643	rBV	824792	1336638	31.90%	2.803%
6	6.734	648	654	667	rVB	724288	1116489	26.65%	2.341%
7	6.922	679	686	698	rBV	920993	1475966	35.23%	3.095%
8	7.381	756	764	773	rBV	857914	1361616	32.50%	2.855%
9	8.093	878	885	903	rBV	1033523	1655547	39.51%	3.471%
10	8.522	950	958	971	rBV	806510	1287372	30.72%	2.699%
11	9.234	1072	1079	1090	rBV	670722	1076040	25.68%	2.256%
12	9.769	1163	1170	1183	rBV	1005456	1673917	39.95%	3.510%
13	9.857	1183	1185	1187	rVB3	5492	4588	0.11%	0.010%
14	10.134	1223	1232	1240	rBV	1123774	1834327	43.78%	3.846%
15	10.281	1250	1257	1276	rBV	916338	1657651	39.56%	3.476%
16	11.740	1500	1505	1515	rBV4	12540	27216	0.65%	0.057%
17	13.457	1789	1797	1809	rBV	1632559	2256655	53.86%	4.732%
18	13.716	1835	1841	1857	rBV	1897787	2798160	66.78%	5.867%
19	14.028	1886	1894	1905	rBV	1564265	2280039	54.42%	4.781%
20	14.263	1928	1934	1954	rBV	437360	833363	19.89%	1.747%
21	15.034	2059	2065	2082	rBV	2405825	3353084	80.03%	7.030%
22	15.169	2082	2088	2102	rVV	628351	861167	20.55%	1.806%
23	15.281	2102	2107	2113	rVB	13476	22113	0.53%	0.046%
24	16.575	2323	2327	2330	rBV4	3901	5840	0.14%	0.012%
25	16.786	2357	2363	2374	rBV	1750236	2442725	58.30%	5.122%
26	16.886	2374	2380	2396	rVV	2455705	3432457	81.92%	7.197%
27	17.480	2478	2481	2487	rBV6	4857	9298	0.22%	0.019%
28	17.728	2519	2523	2532	rBV9	13699	35274	0.84%	0.074%
29	18.033	2571	2575	2578	rBV5	3379	4610	0.11%	0.010%
30	18.757	2694	2698	2705	rBV4	29434	44321	1.06%	0.093%
31	18.827	2707	2710	2716	rVV	24279	36624	0.87%	0.077%
32	19.027	2741	2744	2749	rBV6	6661	12247	0.29%	0.026%
33	19.198	2767	2773	2784	rBV	2832052	3852059	91.93%	8.077%
34	21.021	3078	3083	3094	rBV2	1775414	2513376	59.98%	5.270%
35	23.545	3504	3512	3529	rVB	1900531	4190023	100.00%	8.785%
36	23.727	3535	3543	3558	rVB	1272638	2931761	69.97%	6.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034415.D
Acq On : 05 Oct 2024 08:27
Operator : RC/JU
Sample : PB163786BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47693713

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034415.D
Acq On : 05 Oct 2024 08:27
Operator : RC/JU
Sample : PB163786BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

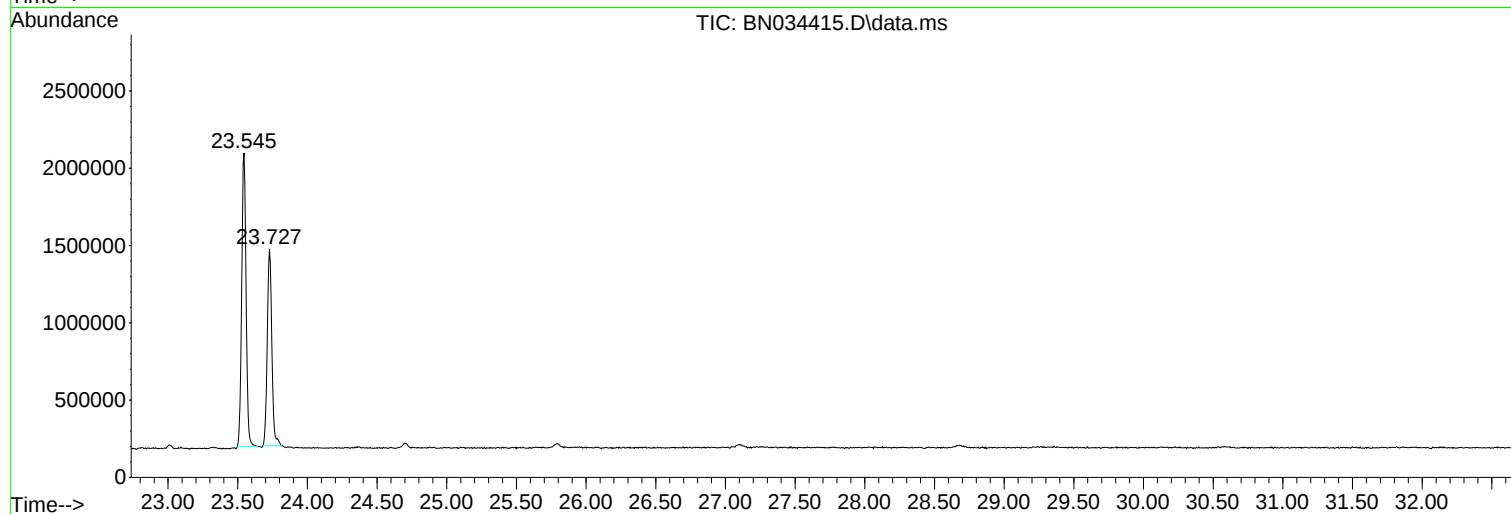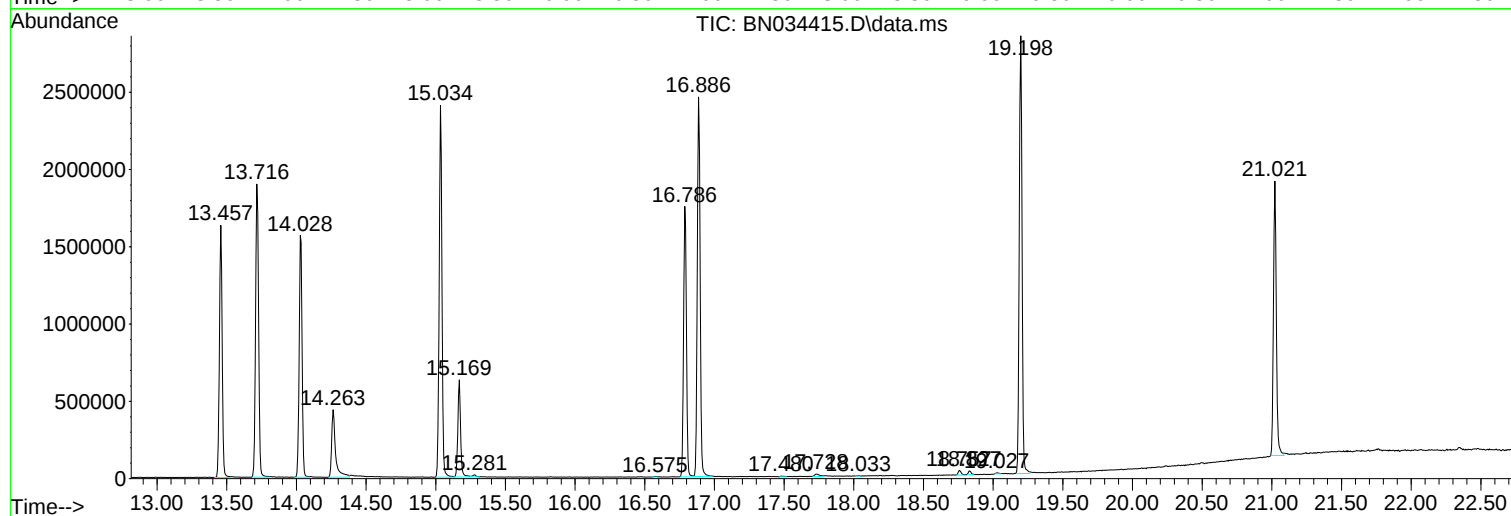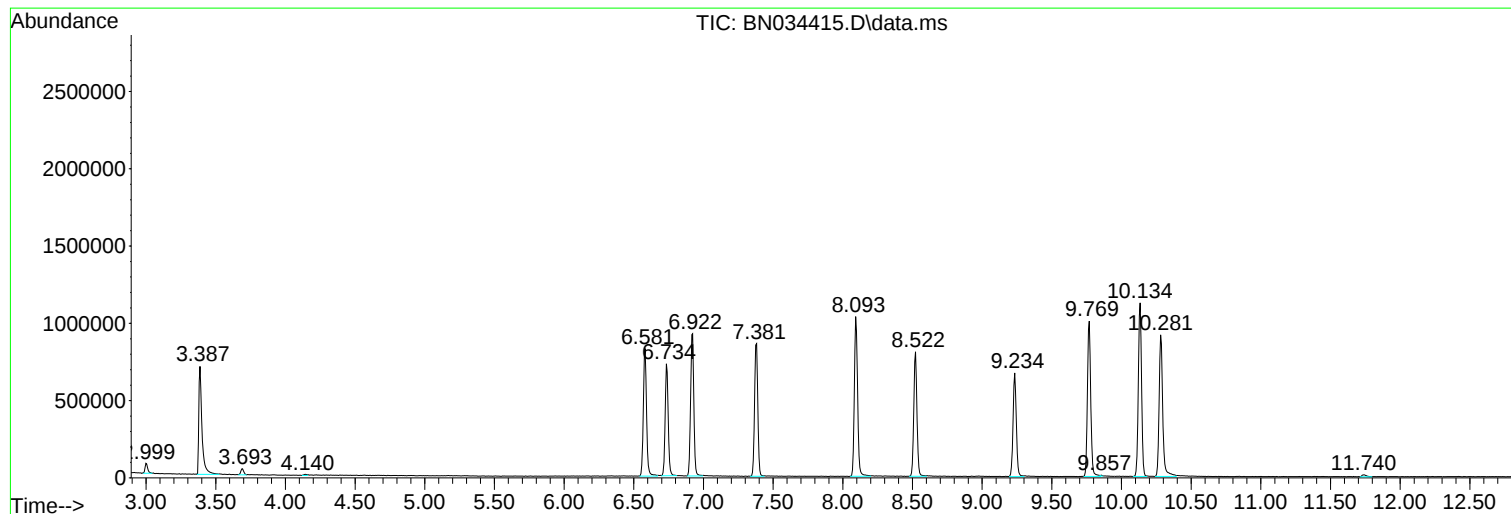

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034415.D
Acq On : 05 Oct 2024 08:27
Operator : RC/JU
Sample : PB163786BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034415.D
Acq On : 05 Oct 2024 08:27
Operator : RC/JU
Sample : PB163786BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------