

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034426.D
 Acq On : 05 Oct 2024 16:18
 Operator : RC/JU
 Sample : P4227-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PMW-8D(20240926)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.993	15	18	20	rBV	50956	55007	1.00%	0.095%
2	3.028	20	24	34	rVB	215738	303945	5.52%	0.525%
3	3.252	58	62	76	rVB4	15004	35126	0.64%	0.061%
4	3.381	81	84	100	rBV	292548	505581	9.19%	0.873%
5	3.687	132	136	142	rVB	13485	20159	0.37%	0.035%
6	4.069	195	201	206	rBV	47929	65188	1.18%	0.113%
7	4.116	206	209	215	rVB3	5671	7961	0.14%	0.014%
8	4.446	262	265	271	rVB2	12629	16768	0.30%	0.029%
9	4.563	282	285	291	rVB	12020	17955	0.33%	0.031%
10	4.757	313	318	327	rVB	47638	73001	1.33%	0.126%
11	5.022	360	363	369	rBV7	4166	6650	0.12%	0.011%
12	5.151	380	385	392	rVB8	3698	7018	0.13%	0.012%
13	5.357	417	420	429	rBV4	7547	12956	0.24%	0.022%
14	5.675	468	474	480	rBV3	27258	43464	0.79%	0.075%
15	6.134	545	552	562	rBV	47114	79524	1.44%	0.137%
16	6.245	567	571	579	rVB9	5098	9045	0.16%	0.016%
17	6.363	586	591	596	rBV7	5589	9101	0.17%	0.016%
18	6.575	619	627	640	rBV	450533	745238	13.54%	1.287%
19	6.734	648	654	663	rBV	814780	1207603	21.94%	2.085%
20	6.828	667	670	673	rVB3	6097	7398	0.13%	0.013%
21	6.916	678	685	694	rBV	1028704	1596082	29.00%	2.756%
22	6.981	694	696	699	rVV3	8267	9807	0.18%	0.017%
23	7.022	699	703	708	rVB4	6025	10365	0.19%	0.018%
24	7.210	731	735	739	rBV6	2972	6369	0.12%	0.011%
25	7.263	739	744	751	rVB	63112	98829	1.80%	0.171%
26	7.375	756	763	767	rBV	895256	1454615	26.43%	2.512%
27	7.410	767	769	776	rVB	397756	502362	9.13%	0.867%
28	7.740	818	825	830	rVB6	10717	23387	0.42%	0.040%
29	7.863	840	846	849	rVB6	5456	9349	0.17%	0.016%
30	8.092	878	885	901	rBV	1028556	1642275	29.84%	2.836%
31	8.475	946	950	951	rVV	5281	6448	0.12%	0.011%
32	8.522	951	958	974	rVB	860954	1435188	26.08%	2.478%
33	8.875	1012	1018	1026	rBV2	48508	90113	1.64%	0.156%
34	8.987	1031	1037	1047	rVV	39905	72386	1.32%	0.125%
35	9.234	1072	1079	1087	rBV	753734	1230108	22.35%	2.124%
36	9.292	1087	1089	1092	rVV3	9571	9465	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034426.D
Acq On : 05 Oct 2024 16:18
Operator : RC/JU
Sample : P4227-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PMW-8D(20240926)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	9.357	1096	1100	1104	rVB6	5843	8317	0.15%	0.014%
38	9.439	1106	1114	1120	rVB10	4003	8759	0.16%	0.015%
39	9.522	1120	1128	1134	rBV2	13342	26743	0.49%	0.046%
40	9.663	1148	1152	1158	rBV3	7573	14476	0.26%	0.025%
41	9.769	1162	1170	1184	rBV	1182650	1974843	35.88%	3.410%
42	9.998	1205	1209	1214	rVB7	5413	9609	0.17%	0.017%
43	10.134	1224	1232	1244	rBV	1179708	1921102	34.91%	3.317%
44	10.281	1249	1257	1271	rBV	993503	1765760	32.08%	3.049%
45	10.392	1272	1276	1285	rVB6	16945	35164	0.64%	0.061%
46	10.628	1310	1316	1322	rBV8	3232	7135	0.13%	0.012%
47	10.975	1368	1375	1384	rBV8	6259	16886	0.31%	0.029%
48	11.357	1433	1440	1446	rVV8	7644	15263	0.28%	0.026%
49	11.422	1446	1451	1461	rVB7	11723	26002	0.47%	0.045%
50	11.563	1470	1475	1477	rBV4	5981	6511	0.12%	0.011%
51	11.733	1497	1504	1510	rVB	17869	29189	0.53%	0.050%
52	12.375	1608	1613	1617	rVB8	3708	5602	0.10%	0.010%
53	12.492	1629	1633	1638	rBV8	3500	6809	0.12%	0.012%
54	12.604	1648	1652	1656	rBV7	4299	9505	0.17%	0.016%
55	12.680	1662	1665	1672	rVB6	5777	9519	0.17%	0.016%
56	12.951	1707	1711	1714	rBV5	4208	7139	0.13%	0.012%
57	13.069	1726	1731	1736	rVV7	7586	14328	0.26%	0.025%
58	13.210	1750	1755	1760	rBV7	6016	9283	0.17%	0.016%
59	13.457	1788	1797	1814	rBV	2014332	2800204	50.88%	4.835%
60	13.716	1834	1841	1852	rBV2	2282417	3323425	60.39%	5.739%
61	13.851	1860	1864	1871	rVB	20312	34331	0.62%	0.059%
62	14.027	1888	1894	1908	rBV	1738011	2608660	47.40%	4.505%
63	14.133	1908	1912	1920	rVB6	15674	29823	0.54%	0.051%
64	14.198	1920	1923	1928	rVB	10682	13904	0.25%	0.024%
65	14.269	1928	1935	1947	rBV	141117	308154	5.60%	0.532%
66	14.486	1968	1972	1981	rVB10	11556	23499	0.43%	0.041%
67	14.586	1984	1989	1995	rVV	33673	49962	0.91%	0.086%
68	14.869	2034	2037	2038	rBV3	4961	5577	0.10%	0.010%
69	15.033	2058	2065	2081	rBV	2951015	4156875	75.53%	7.178%
70	15.169	2081	2088	2101	rVV	981430	1342722	24.40%	2.319%
71	15.274	2103	2106	2115	rVB2	17944	29078	0.53%	0.050%
72	15.416	2125	2130	2136	rBV2	19747	30144	0.55%	0.052%
73	15.680	2172	2175	2177	rBV4	5629	6063	0.11%	0.010%
74	15.792	2190	2194	2197	rBV6	3236	5708	0.10%	0.010%
75	15.851	2197	2204	2213	rVV	52311	94516	1.72%	0.163%
76	16.580	2324	2328	2332	rVB3	6201	8142	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034426.D
 Acq On : 05 Oct 2024 16:18
 Operator : RC/JU
 Sample : P4227-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PMW-8D(20240926)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

77	16.745	2349	2356	2357	rBV6	12667	15861	0.29%	0.027%
78	16.786	2357	2363	2374	rVV	2156672	2976237	54.08%	5.139%
79	16.886	2374	2380	2393	rVV2	3357839	4595599	83.50%	7.936%
80	17.004	2398	2400	2409	rVB10	7012	13446	0.24%	0.023%
81	17.104	2414	2417	2422	rVB	7699	11032	0.20%	0.019%
82	17.174	2425	2429	2434	rBV5	5805	10697	0.19%	0.018%
83	17.386	2462	2465	2468	rVB2	6783	7592	0.14%	0.013%
84	17.480	2478	2481	2487	rVB7	7747	11713	0.21%	0.020%
85	17.598	2499	2501	2508	rVB8	3404	6956	0.13%	0.012%
86	17.721	2517	2522	2529	rBV	90441	154462	2.81%	0.267%
87	17.786	2530	2533	2537	rVB	21776	28556	0.52%	0.049%
88	18.004	2567	2570	2578	rVB9	8371	17883	0.32%	0.031%
89	18.757	2694	2698	2704	rBV	50231	61417	1.12%	0.106%
90	18.827	2706	2710	2715	rBV	45093	65076	1.18%	0.112%
91	19.021	2739	2743	2751	rBV	67180	100185	1.82%	0.173%
92	19.198	2764	2773	2787	rBV	4114710	5503421	100.00%	9.503%
93	21.021	3077	3083	3094	rBV	2364293	3301016	59.98%	5.700%
94	23.545	3503	3512	3525	rBV2	2448065	5315023	96.58%	9.178%
95	23.727	3535	3543	3565	rVB	1523317	3491121	63.44%	6.028%




Sum of corrected areas: 57911860

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034426.D
Acq On : 05 Oct 2024 16:18
Operator : RC/JU
Sample : P4227-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PMW-8D(20240926)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

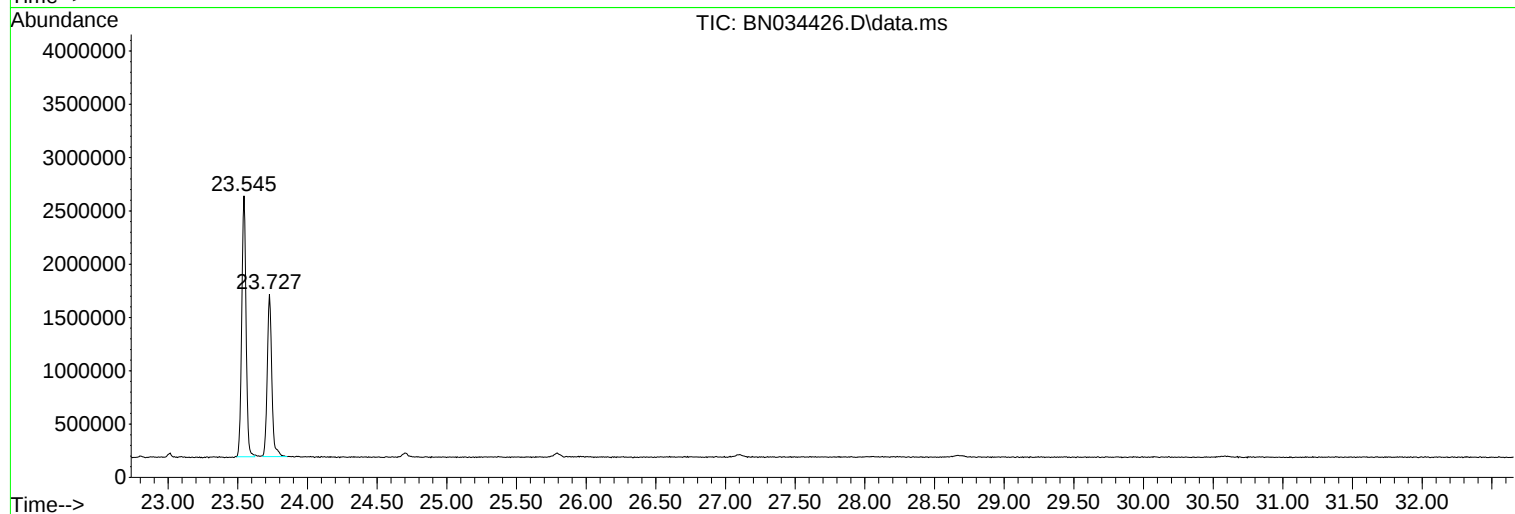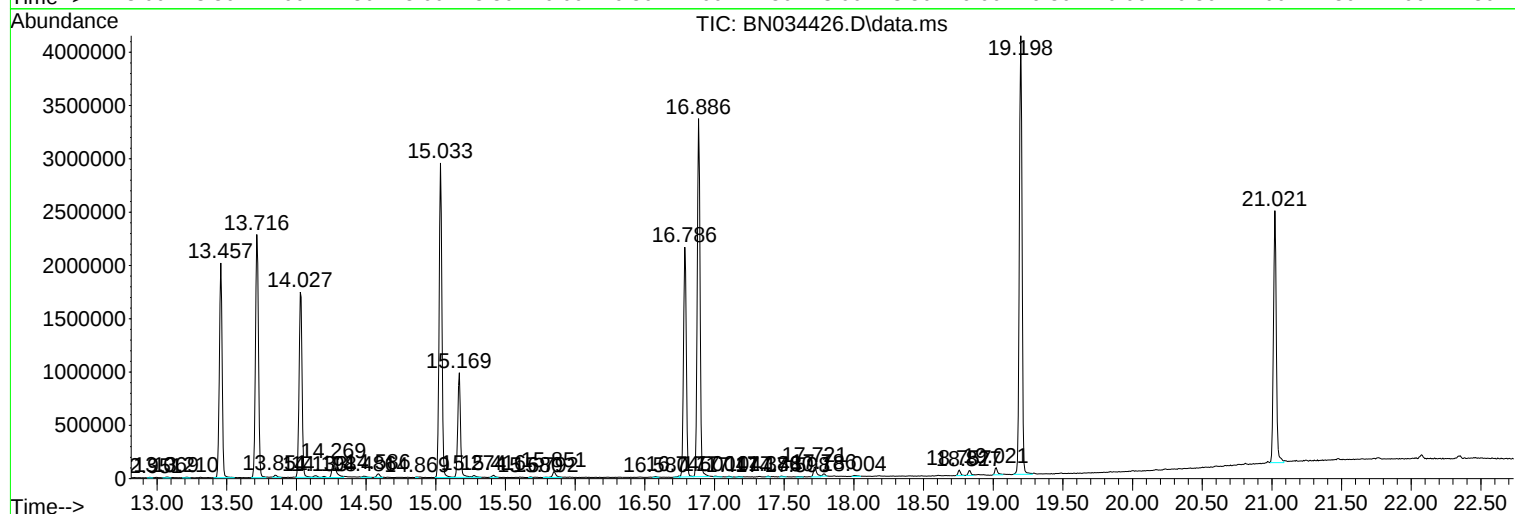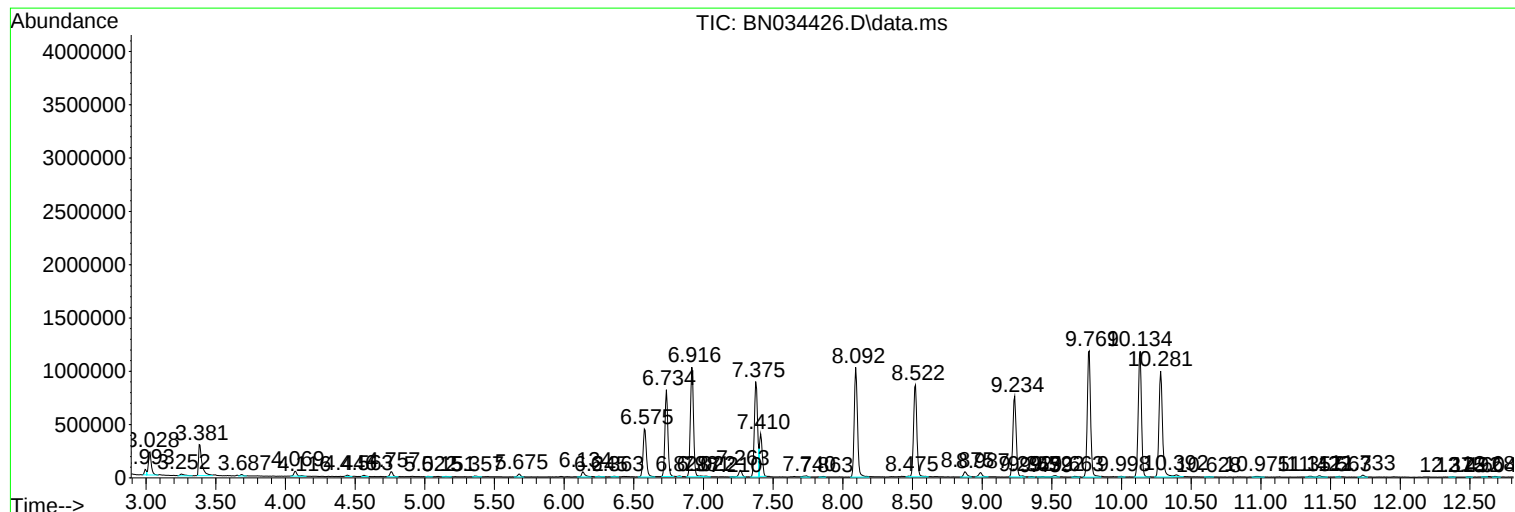

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034426.D
Acq On : 05 Oct 2024 16:18
Operator : RC/JU
Sample : P4227-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PMW-8D(20240926)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034426.D
Acq On : 05 Oct 2024 16:18
Operator : RC/JU
Sample : P4227-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PMW-8D(20240926)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------