

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034428.D
 Acq On : 05 Oct 2024 18:16
 Operator : RC/JU
 Sample : PB163831BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK831

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.993	15	18	24	rVB	40208	53351	1.55%	0.143%
2	3.381	80	84	103	rBV	453740	765331	22.23%	2.058%
3	3.687	131	136	142	rVB	26748	38470	1.12%	0.103%
4	6.575	620	627	643	rBV	567467	920639	26.74%	2.475%
5	6.734	648	654	664	rBV	498726	759198	22.05%	2.041%
6	6.916	678	685	699	rBV	645366	1004636	29.18%	2.701%
7	7.375	756	763	776	rBV	642843	989114	28.73%	2.659%
8	8.093	878	885	903	rBV	727279	1160214	33.70%	3.119%
9	8.522	951	958	968	rBV	539687	892548	25.93%	2.400%
10	9.234	1072	1079	1094	rBV	445227	732459	21.28%	1.969%
11	9.769	1162	1170	1186	rBV	662650	1158893	33.66%	3.116%
12	10.134	1224	1232	1240	rBV	822493	1352326	39.28%	3.636%
13	10.281	1250	1257	1277	rBV	642532	1175055	34.13%	3.159%
14	10.446	1283	1285	1291	rVB6	3388	5020	0.15%	0.013%
15	11.734	1497	1504	1513	rBV3	8790	20876	0.61%	0.056%
16	12.998	1712	1719	1722	rVB7	1821	3500	0.10%	0.009%
17	13.457	1790	1797	1812	rBV	1251884	1721114	49.99%	4.627%
18	13.716	1833	1841	1860	rBV	1424519	2062369	59.91%	5.545%
19	14.028	1888	1894	1906	rBV	1218027	1778803	51.67%	4.782%
20	14.263	1928	1934	1953	rBV	306995	641988	18.65%	1.726%
21	15.034	2058	2065	2081	rBV	1827323	2571332	74.69%	6.913%
22	15.169	2082	2088	2103	rVV	486028	685434	19.91%	1.843%
23	15.275	2103	2106	2112	rVB3	9439	13808	0.40%	0.037%
24	15.604	2158	2162	2167	rBV7	1750	3570	0.10%	0.010%
25	16.786	2357	2363	2374	rBV	1513688	2095307	60.86%	5.633%
26	16.886	2374	2380	2392	rVV	1961283	2806063	81.51%	7.544%
27	17.486	2477	2482	2485	rBV7	3327	4664	0.14%	0.013%
28	17.745	2521	2526	2528	rBV6	4979	9209	0.27%	0.025%
29	18.557	2661	2664	2665	rBV3	2719	3454	0.10%	0.009%
30	18.610	2671	2673	2677	rBV5	3516	5254	0.15%	0.014%
31	18.763	2694	2699	2704	rBV2	24161	35640	1.04%	0.096%
32	18.828	2706	2710	2716	rBV	22411	32788	0.95%	0.088%
33	19.022	2741	2743	2750	rBV8	3975	8760	0.25%	0.024%
34	19.198	2766	2773	2789	rBV	2565677	3442653	100.00%	9.256%
35	21.022	3078	3083	3095	rBV	1714006	2382204	69.20%	6.405%
36	23.545	3503	3512	3524	rBV	1538465	3423743	99.45%	9.205%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034428.D
Acq On : 05 Oct 2024 18:16
Operator : RC/JU
Sample : PB163831BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK831

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	23.727	3535	3543	3551	rBV	1120246	2434531	70.72%	6.545%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 37194318

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034428.D
Acq On : 05 Oct 2024 18:16
Operator : RC/JU
Sample : PB163831BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK831

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

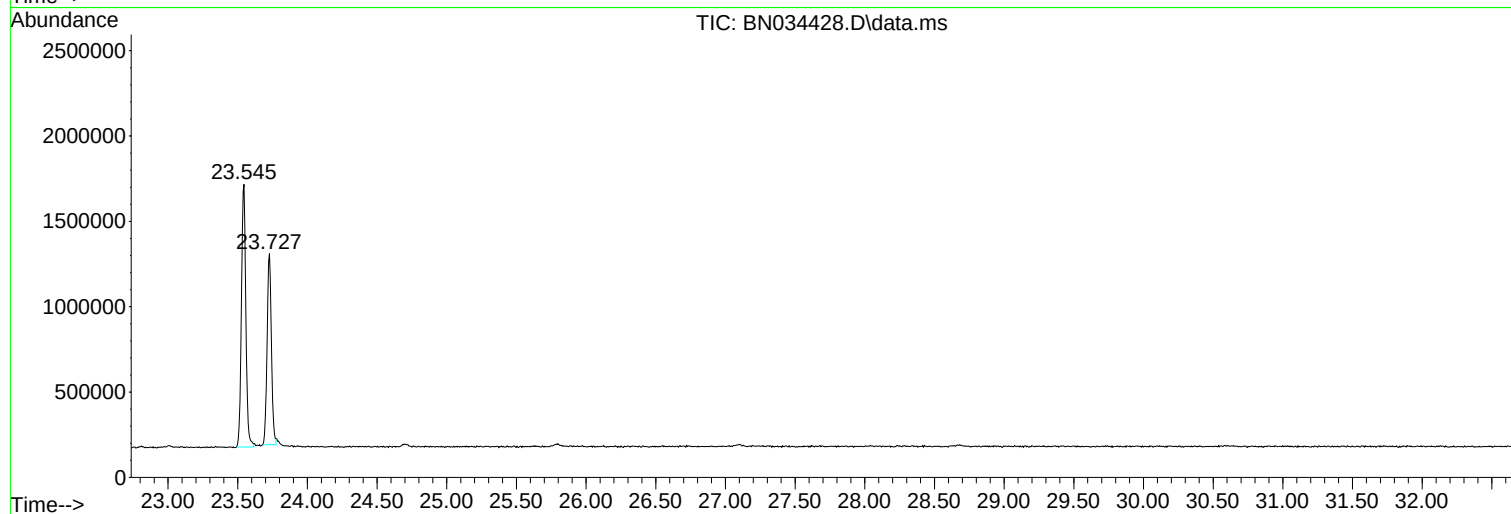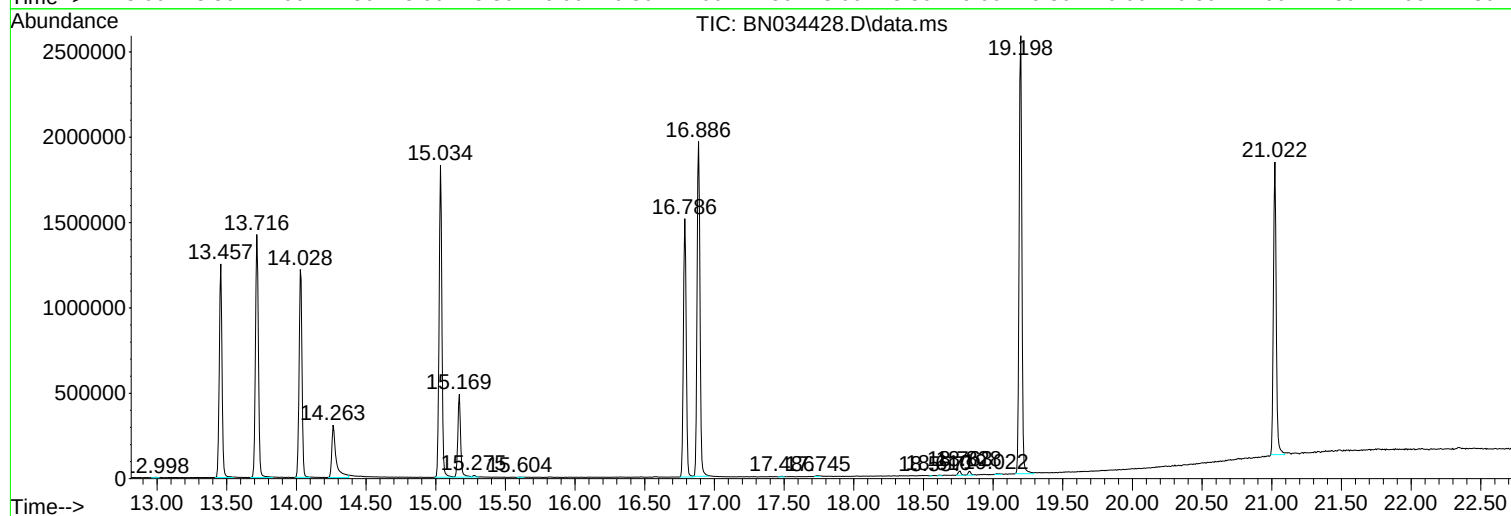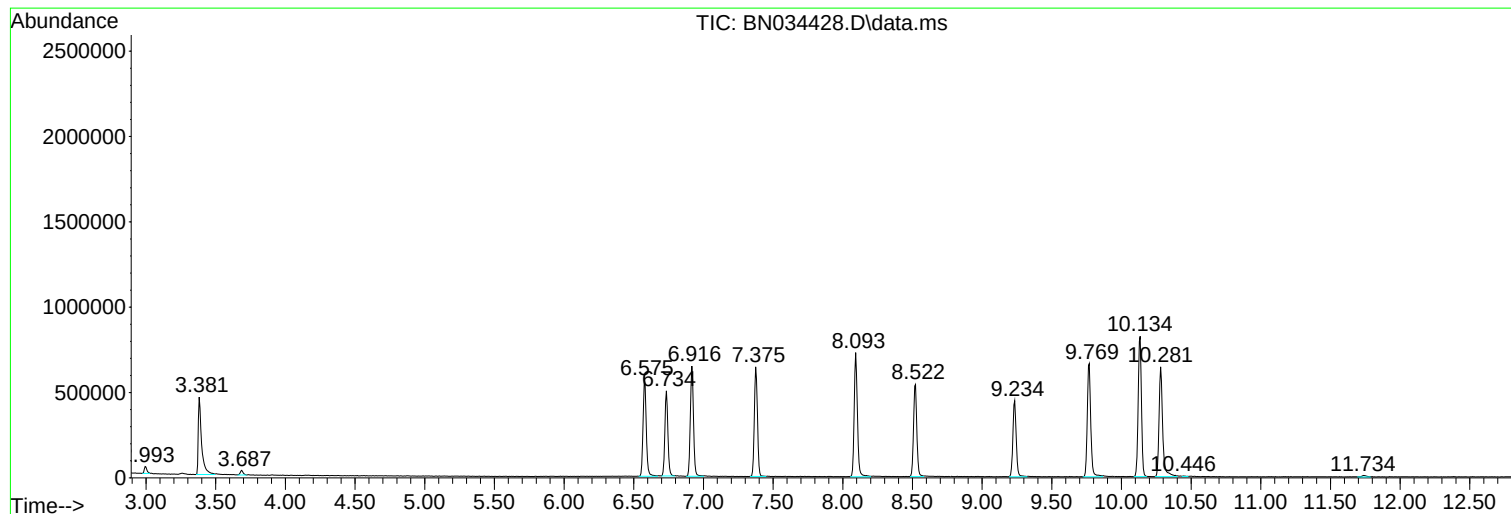

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034428.D
Acq On : 05 Oct 2024 18:16
Operator : RC/JU
Sample : PB163831BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK831

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034428.D
Acq On : 05 Oct 2024 18:16
Operator : RC/JU
Sample : PB163831BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK831

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc