

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
 Data File : BN034429.D
 Acq On : 05 Oct 2024 18:55
 Operator : RC/JU
 Sample : PB163748TB 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB748

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.993	15	18	28	rVB	56775	78274	1.76%	0.162%
2	3.258	59	63	72	rVB4	7895	15674	0.35%	0.032%
3	3.381	80	84	99	rBV	635155	952235	21.37%	1.974%
4	3.687	132	136	143	rVB	35460	48350	1.09%	0.100%
5	4.140	207	213	214	rBV4	5550	7424	0.17%	0.015%
6	6.575	620	627	638	rBV	715844	1154752	25.91%	2.393%
7	6.734	648	654	668	rVB	646039	968385	21.73%	2.007%
8	6.916	678	685	698	rBV	833011	1270041	28.50%	2.632%
9	7.375	756	763	773	rBV	815501	1240157	27.83%	2.570%
10	8.093	878	885	903	rBV	930353	1474637	33.09%	3.056%
11	8.516	950	957	971	rBV	698083	1153899	25.89%	2.392%
12	9.234	1071	1079	1092	rBV	591325	952309	21.37%	1.974%
13	9.763	1162	1169	1182	rBV	873410	1493793	33.52%	3.096%
14	10.134	1225	1232	1243	rVB	1050923	1741723	39.09%	3.610%
15	10.281	1250	1257	1278	rBV	840536	1522958	34.18%	3.157%
16	11.734	1497	1504	1515	rBV2	11865	27903	0.63%	0.058%
17	13.457	1790	1797	1811	rBV	1717848	2341180	52.54%	4.852%
18	13.716	1833	1841	1851	rBV	1853805	2712744	60.88%	5.622%
19	14.028	1888	1894	1906	rBV	1563358	2323961	52.15%	4.817%
20	14.263	1928	1934	1948	rBV	487270	904741	20.30%	1.875%
21	14.463	1965	1968	1972	rVB5	4273	6316	0.14%	0.013%
22	15.034	2057	2065	2078	rBV	2421519	3402760	76.36%	7.053%
23	15.169	2082	2088	2100	rVV	696356	970875	21.79%	2.012%
24	15.275	2103	2106	2114	rVB3	14035	22462	0.50%	0.047%
25	16.575	2322	2327	2330	rBV4	4509	7628	0.17%	0.016%
26	16.786	2356	2363	2374	rBV	1980774	2797212	62.77%	5.798%
27	16.886	2374	2380	2399	rVB	2593907	3699934	83.03%	7.669%
28	17.480	2478	2481	2487	rVB6	4880	6322	0.14%	0.013%
29	17.739	2517	2525	2530	rBV8	9472	26044	0.58%	0.054%
30	18.757	2694	2698	2702	rBV2	35443	46775	1.05%	0.097%
31	18.833	2706	2711	2716	rBV	32825	45443	1.02%	0.094%
32	19.022	2741	2743	2747	rBV5	5500	7347	0.16%	0.015%
33	19.198	2766	2773	2788	rBV	3234060	4456117	100.00%	9.236%
34	21.021	3077	3083	3094	rBV	2140017	3021851	67.81%	6.263%
35	23.545	3503	3512	3528	rBV	1908697	4225347	94.82%	8.758%
36	23.721	3535	3542	3559	rVB2	1302742	3120503	70.03%	6.468%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034429.D
Acq On : 05 Oct 2024 18:55
Operator : RC/JU
Sample : PB163748TB 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB748

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 48248076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034429.D
Acq On : 05 Oct 2024 18:55
Operator : RC/JU
Sample : PB163748TB 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB748

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

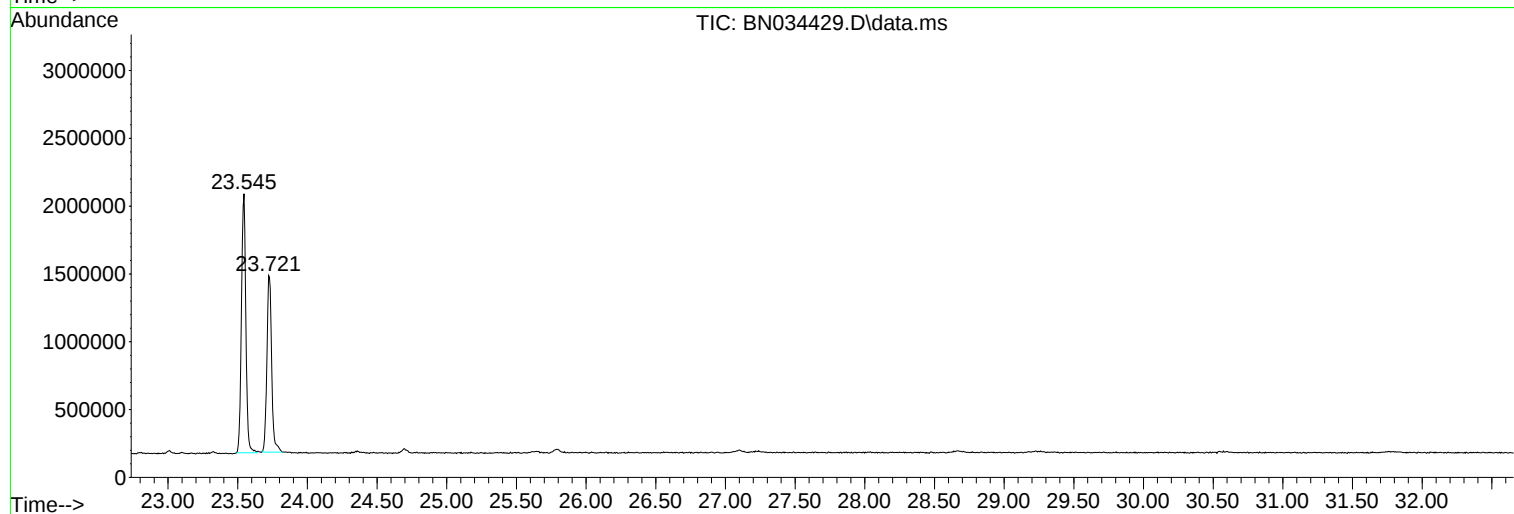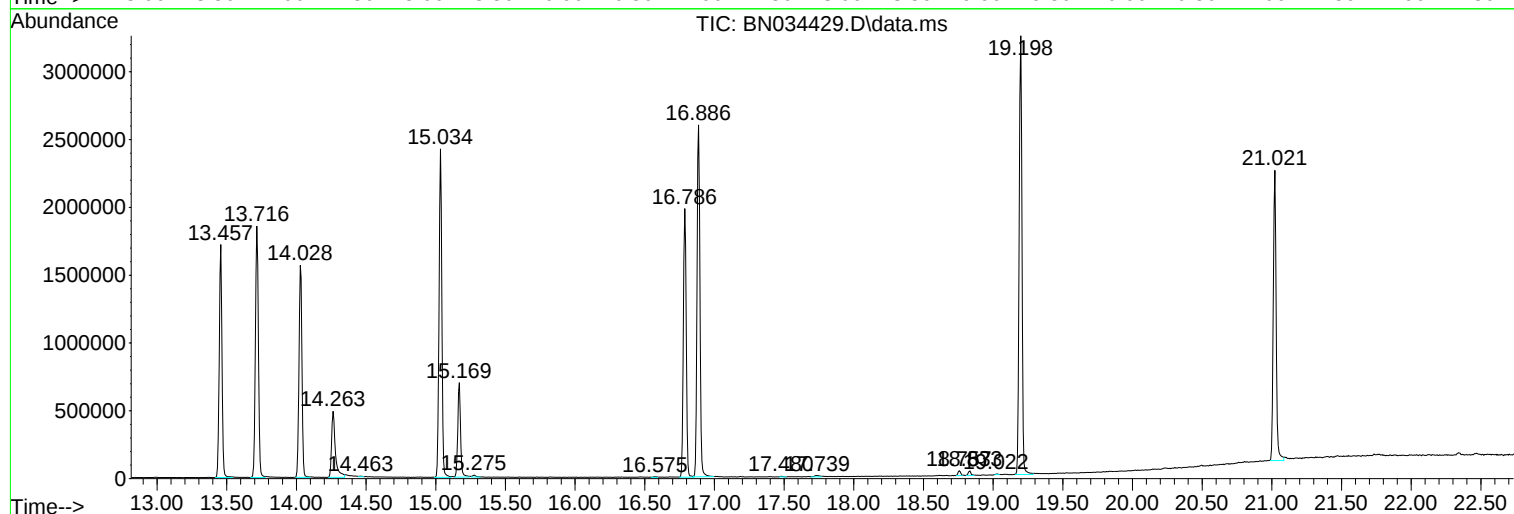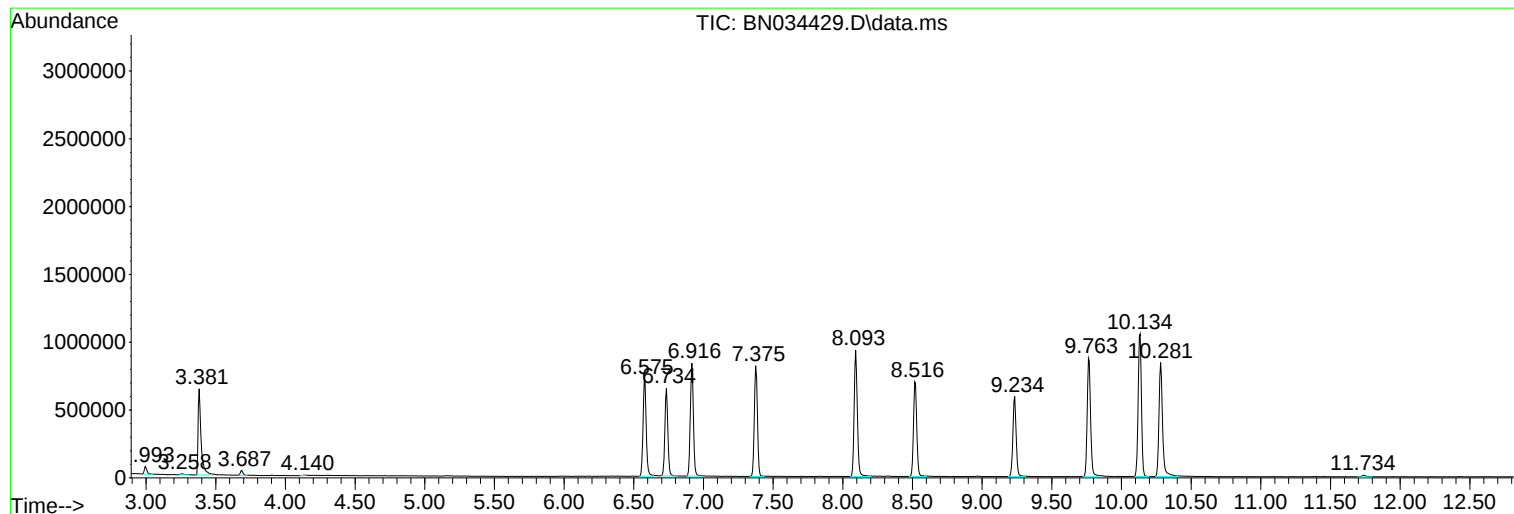

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034429.D
Acq On : 05 Oct 2024 18:55
Operator : RC/JU
Sample : PB163748TB 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB748

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100424\
Data File : BN034429.D
Acq On : 05 Oct 2024 18:55
Operator : RC/JU
Sample : PB163748TB 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB748

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc