

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100425\
 Data File : BN037999.D
 Acq On : 03 Oct 2025 16:07
 Operator : RC/JU
 Sample : PB169495BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	36	rVB	80311	109491	1.45%	0.136%
2	3.658	92	97	121	rBV	1122767	1728325	22.92%	2.146%
3	3.993	148	154	159	rBV	37963	58104	0.77%	0.072%
4	4.211	187	191	194	rBV3	7336	7706	0.10%	0.010%
5	4.616	255	260	265	rBV6	5278	9301	0.12%	0.012%
6	6.963	651	659	669	rBV	1336160	2108880	27.96%	2.618%
7	7.128	680	687	698	rVB	1125440	1719611	22.80%	2.135%
8	7.334	714	722	731	rBV	1357992	2138464	28.35%	2.655%
9	7.805	792	802	812	rBV	1067481	1703183	22.58%	2.114%
10	8.504	914	921	936	rBV	1798768	2793605	37.04%	3.468%
11	8.957	989	998	1008	rBV	1315494	2129263	28.23%	2.643%
12	9.081	1013	1019	1022	rBV6	5015	7915	0.10%	0.010%
13	9.687	1114	1122	1134	rBV	976754	1622614	21.51%	2.014%
14	10.222	1205	1213	1226	rBV	1732104	2770152	36.73%	3.439%
15	10.604	1270	1278	1288	rVB	1611878	2707701	35.90%	3.362%
16	10.740	1292	1301	1314	rBV	1828768	3069339	40.70%	3.811%
17	11.257	1385	1389	1395	rVB2	8767	15627	0.21%	0.019%
18	12.204	1544	1550	1555	rVB2	27858	42535	0.56%	0.053%
19	13.445	1755	1761	1765	rBV	32174	42946	0.57%	0.053%
20	13.869	1826	1833	1848	rBV	3284749	4363536	57.86%	5.417%
21	14.151	1873	1881	1895	rBV	3623042	5292752	70.18%	6.571%
22	14.463	1926	1934	1941	rBV	2600875	3738578	49.57%	4.641%
23	14.645	1958	1965	1979	rBV	1554790	2144563	28.44%	2.662%
24	14.875	2000	2004	2008	rVB4	6861	8553	0.11%	0.011%
25	15.457	2096	2103	2110	rBV	4604894	6481301	85.94%	8.046%
26	15.569	2115	2122	2135	rVV	1181922	1621713	21.50%	2.013%
27	15.698	2139	2144	2150	rVB3	20290	35262	0.47%	0.044%
28	16.245	2232	2237	2240	rBV5	5353	8365	0.11%	0.010%
29	16.992	2360	2364	2368	rBV3	9220	13673	0.18%	0.017%
30	17.210	2390	2401	2411	rBV2	2932165	4195545	55.63%	5.209%
31	17.310	2411	2418	2431	rVV	4967781	6915549	91.70%	8.586%
32	18.110	2551	2554	2558	rBV3	9294	11695	0.16%	0.015%
33	19.169	2730	2734	2741	rBV3	48002	64946	0.86%	0.081%
34	19.239	2741	2746	2750	rVV	48571	66289	0.88%	0.082%
35	19.310	2754	2758	2763	rVV	65542	77969	1.03%	0.097%
36	19.451	2778	2782	2789	rBV	66594	92880	1.23%	0.115%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100425\
Data File : BN037999.D
Acq On : 03 Oct 2025 16:07
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Title : SVOA CALIBRATION

37	19.545	2794	2798	2802	rBV	155375	182859	2.42%	0.227%
38	19.604	2802	2808	2815	rVV	5831533	7541880	100.00%	9.363%
39	19.663	2815	2818	2822	rVB2	21576	28191	0.37%	0.035%
40	20.386	2938	2941	2945	rVB5	31511	33726	0.45%	0.042%
41	20.592	2972	2976	2981	rBV2	93307	109381	1.45%	0.136%
42	21.463	3118	3124	3133	rBV	2743366	3974155	52.69%	4.934%
43	24.321	3601	3610	3624	rVB	2332845	5563233	73.76%	6.907%
44	24.527	3637	3645	3654	rBV	1307907	3197684	42.40%	3.970%




Sum of corrected areas: 80549040

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100425\
Data File : BN037999.D
Acq On : 03 Oct 2025 16:07
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

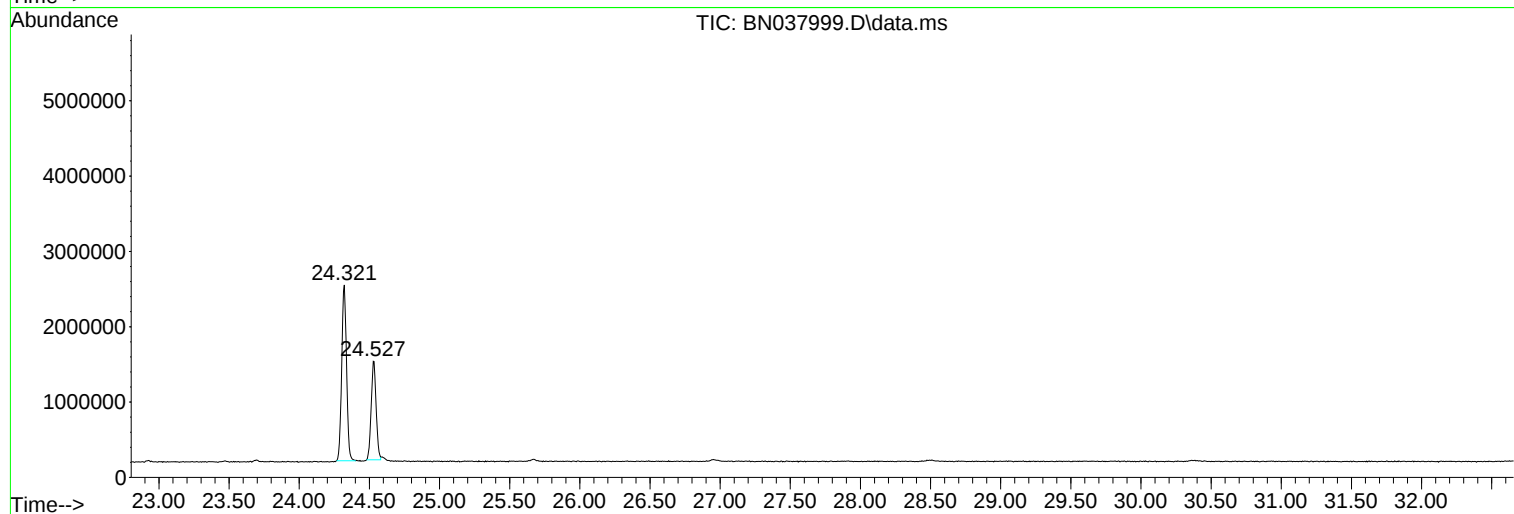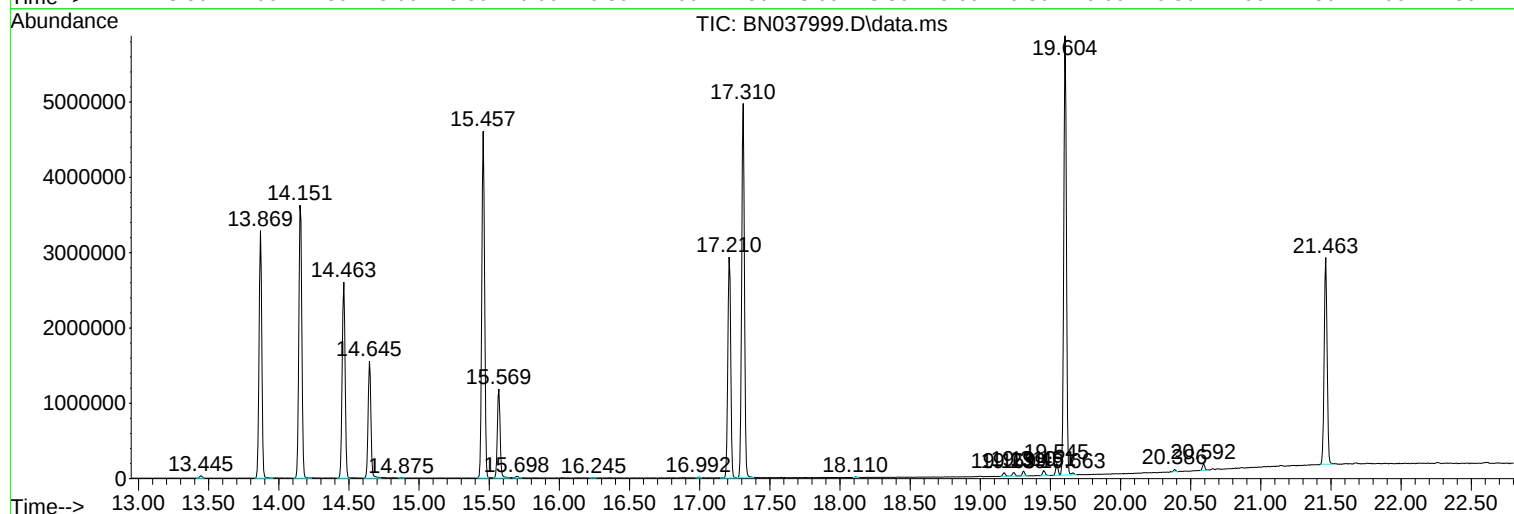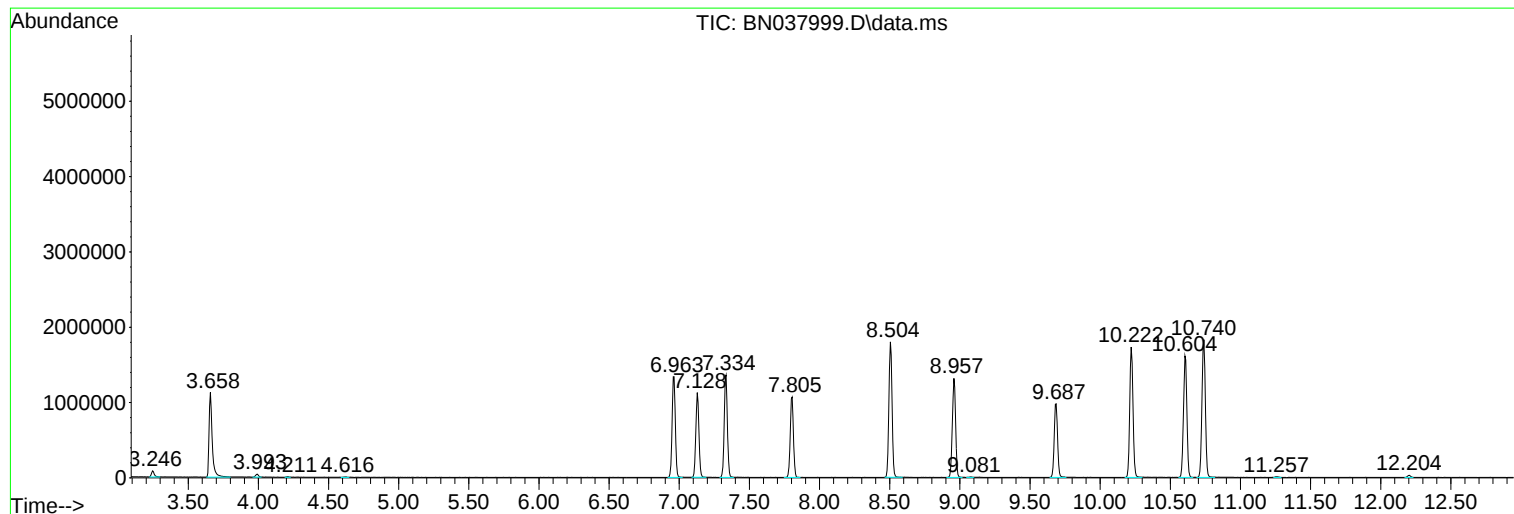

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100425\
Data File : BN037999.D
Acq On : 03 Oct 2025 16:07
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100425\
Data File : BN037999.D
Acq On : 03 Oct 2025 16:07
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc